

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007504.D
 Acq On : 13 Sep 2018 04:36
 Operator : SY/MD
 Sample : J4872-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KP1

Quant Time: Sep 13 07:37:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 07:19:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	116267	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	104316	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	54824	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	32401	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	24971	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.13	63	52103	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.20%
20) 2-Butanone-d5	3.96	46	61547	45.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.88%
24) Chloroform-d	4.41	84	61920	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.09	65	32194	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	5.10	84	121459	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
36) 1,2-Dichloropropane-d6	6.13	67	36453	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.36	98	125617	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
43) trans-1,3-Dichloropropene-	7.67	79	15904	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.14	63	40266	48.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	25473	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	49627	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	23681	3.45 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007504.D
Acq On : 13 Sep 2018 04:36
Operator : SY/MD
Sample : J4872-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KP1

Quant Time: Sep 13 07:37:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 07:19:10 2018
Response via : Initial Calibration

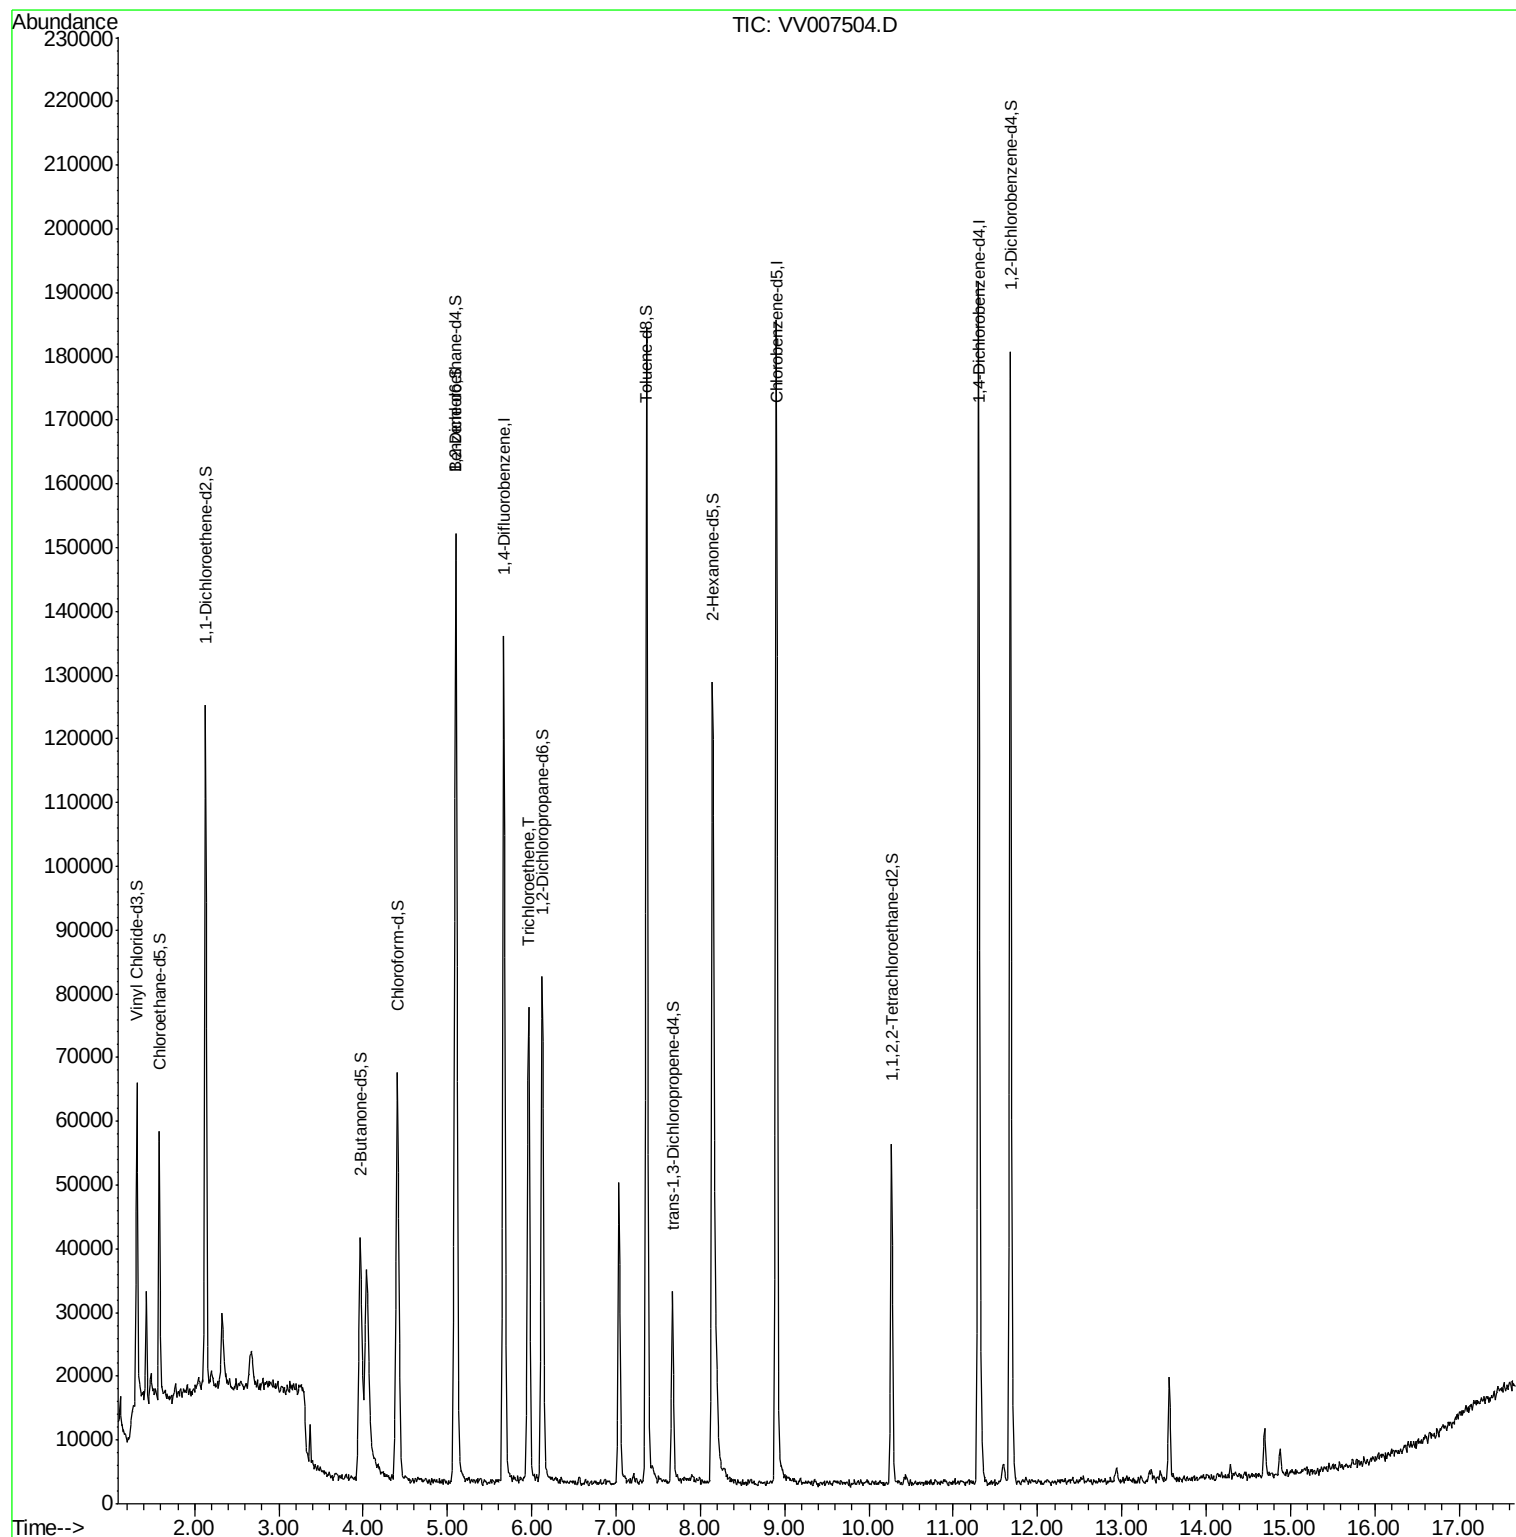

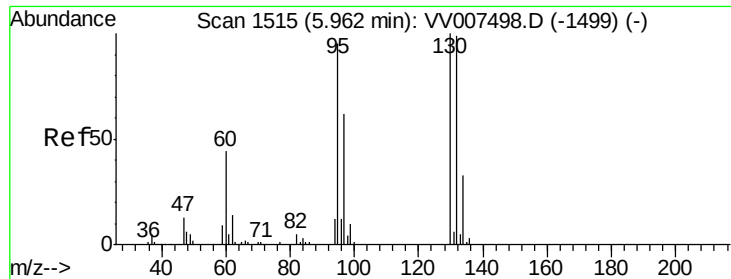

#34

Trichloroethene

Concen: 3.45 ug/L

RT: 5.96 min Scan# 1516

Delta R.T. 0.00 min

Lab File: VV007504.D


Acq: 13 Sep 2018 04:36

Instrument :

MSVOA_V

ClientSampleId :

C0KP1

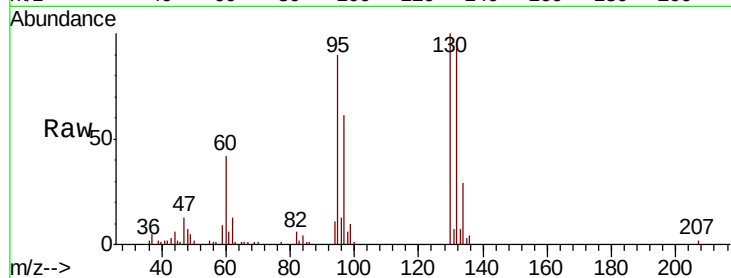

Tot Ion: 95 Resp: 23681

Ion Ratio Lower Upper

95 100

97 67.1 42.8 79.4

132 102.8 67.6 125.6

130 110.8 69.6 129.2

