

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007508.D
 Acq On : 13 Sep 2018 06:25
 Operator : SY/MD
 Sample : J4872-07
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KP7

Quant Time: Sep 13 08:03:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 07:19:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	119794	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	106191	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	54729	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	33371	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	26403	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	55435	4.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.80%
20) 2-Butanone-d5	3.97	46	63655	46.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.22%
24) Chloroform-d	4.41	84	63499	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.09	65	33593	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	124772	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
36) 1,2-Dichloropropane-d6	6.13	67	36956	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.36	98	126455	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
43) trans-1,3-Dichloropropene-	7.67	79	16415	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
46) 2-Hexanone-d5	8.14	63	36743	43.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	25050	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	50366	5.37	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.40%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	3906	0.56 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007508.D
Acq On : 13 Sep 2018 06:25
Operator : SY/MD
Sample : J4872-07
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KP7

Quant Time: Sep 13 08:03:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 07:19:10 2018
Response via : Initial Calibration

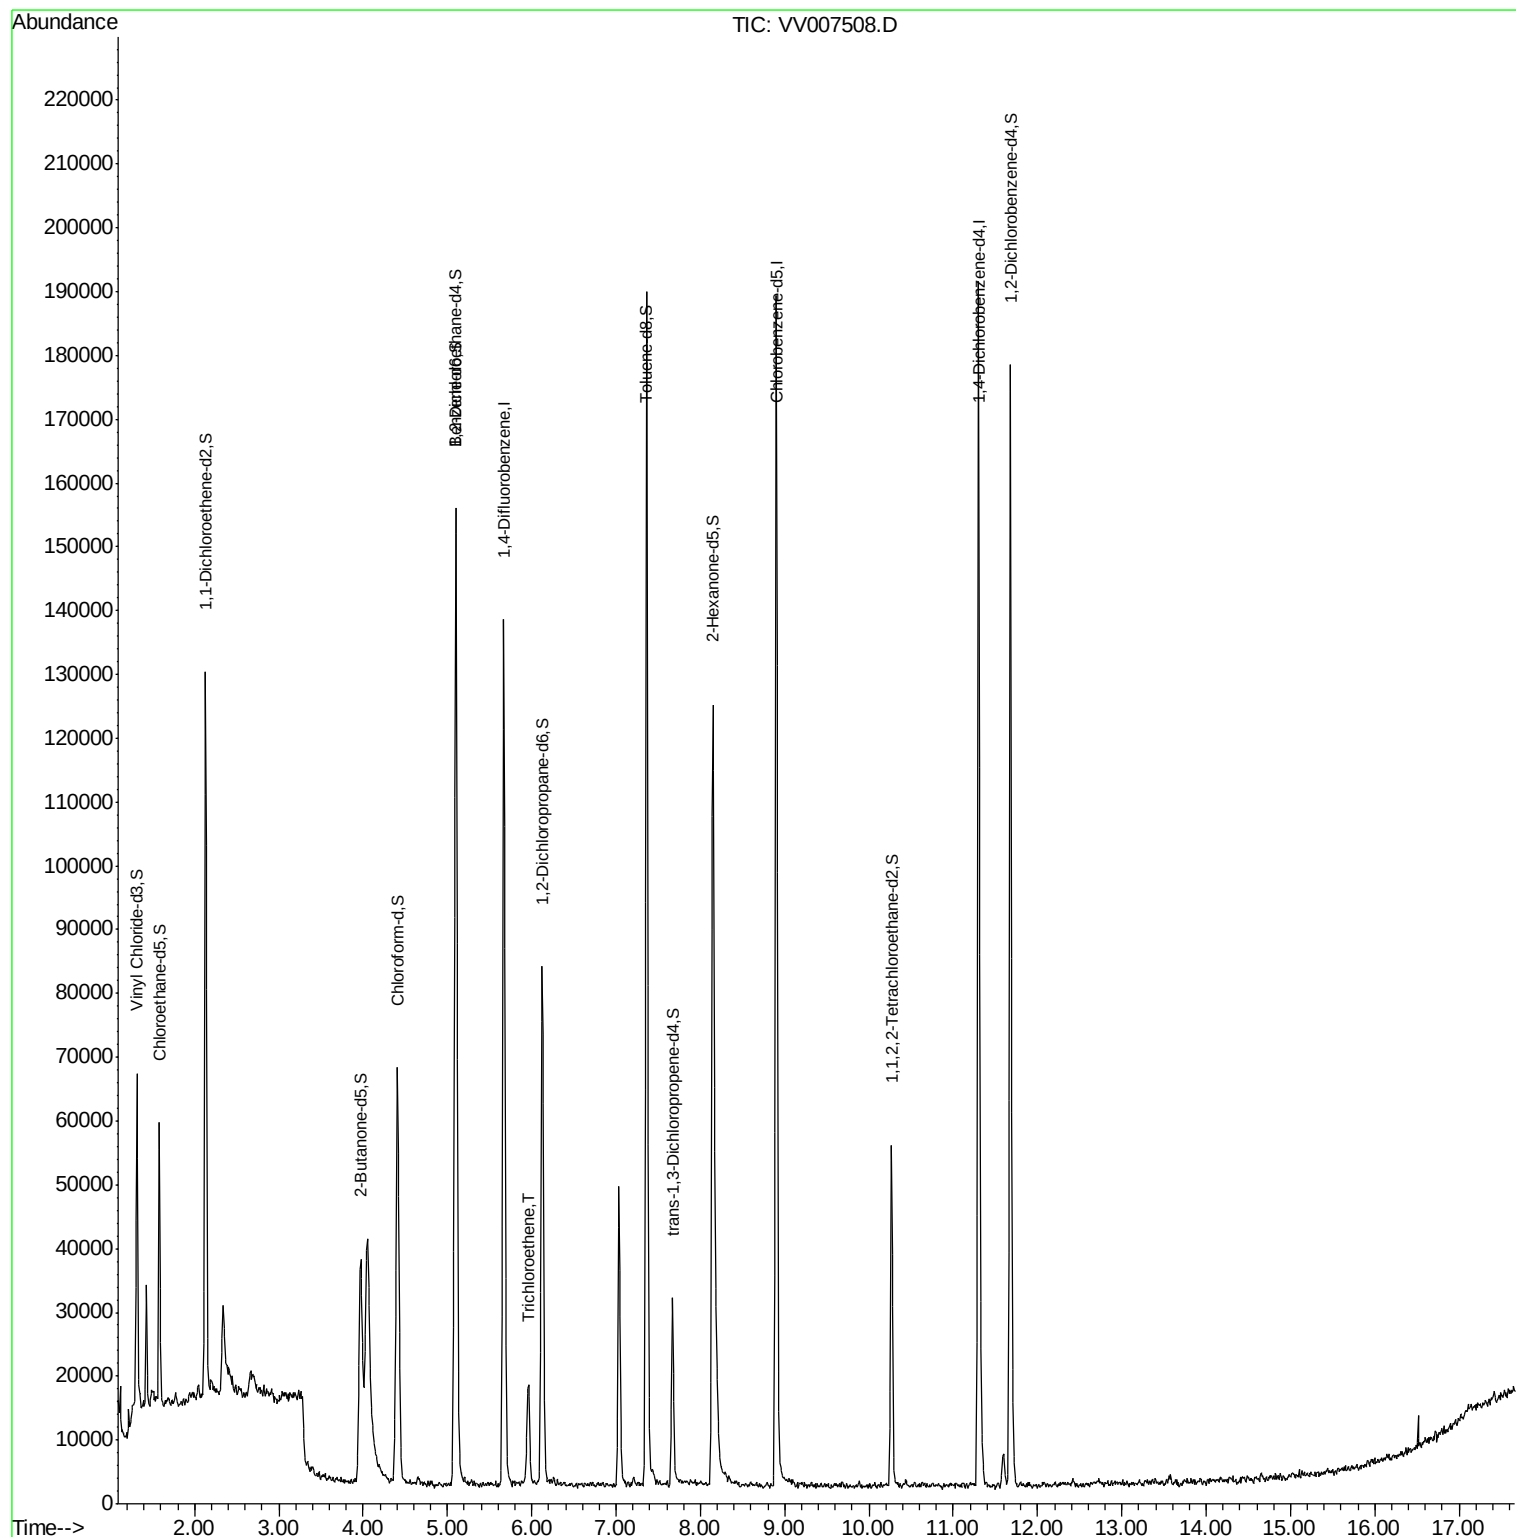

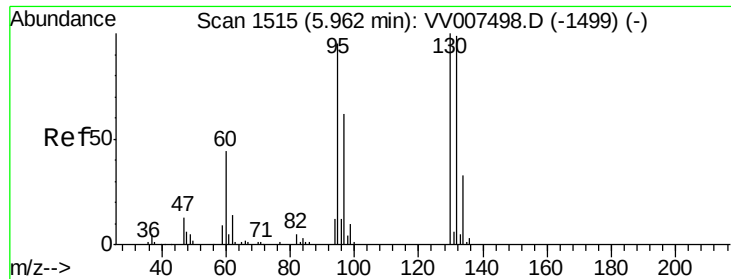

#34

Trichloroethene

Concen: 0.56 ug/L

RT: 5.96 min Scan# 1516

Delta R.T. 0.00 min

Lab File: VV007508.D


Acq: 13 Sep 2018 06:25

Instrument :

MSVOA_V

ClientSampleId :

C0KP7

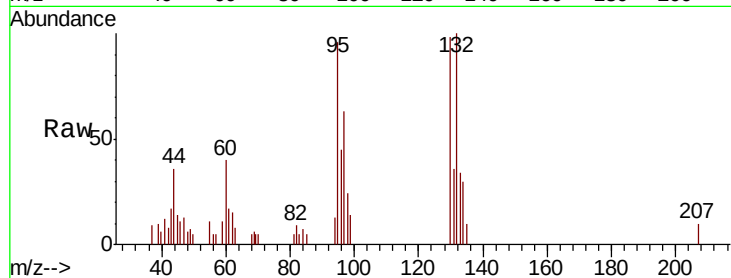

Tot Ion: 95 Resp: 3906

Ion Ratio Lower Upper

95 100

97 65.8 42.8 79.4

132 104.1 67.6 125.6

130 102.1 69.6 129.2

