


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091218\
Data File : VV007470.D
Acq On : 12 Sep 2018 11:11
Operator : SY/MD
Sample : BFB70
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB70

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 13 07:19:10 2018

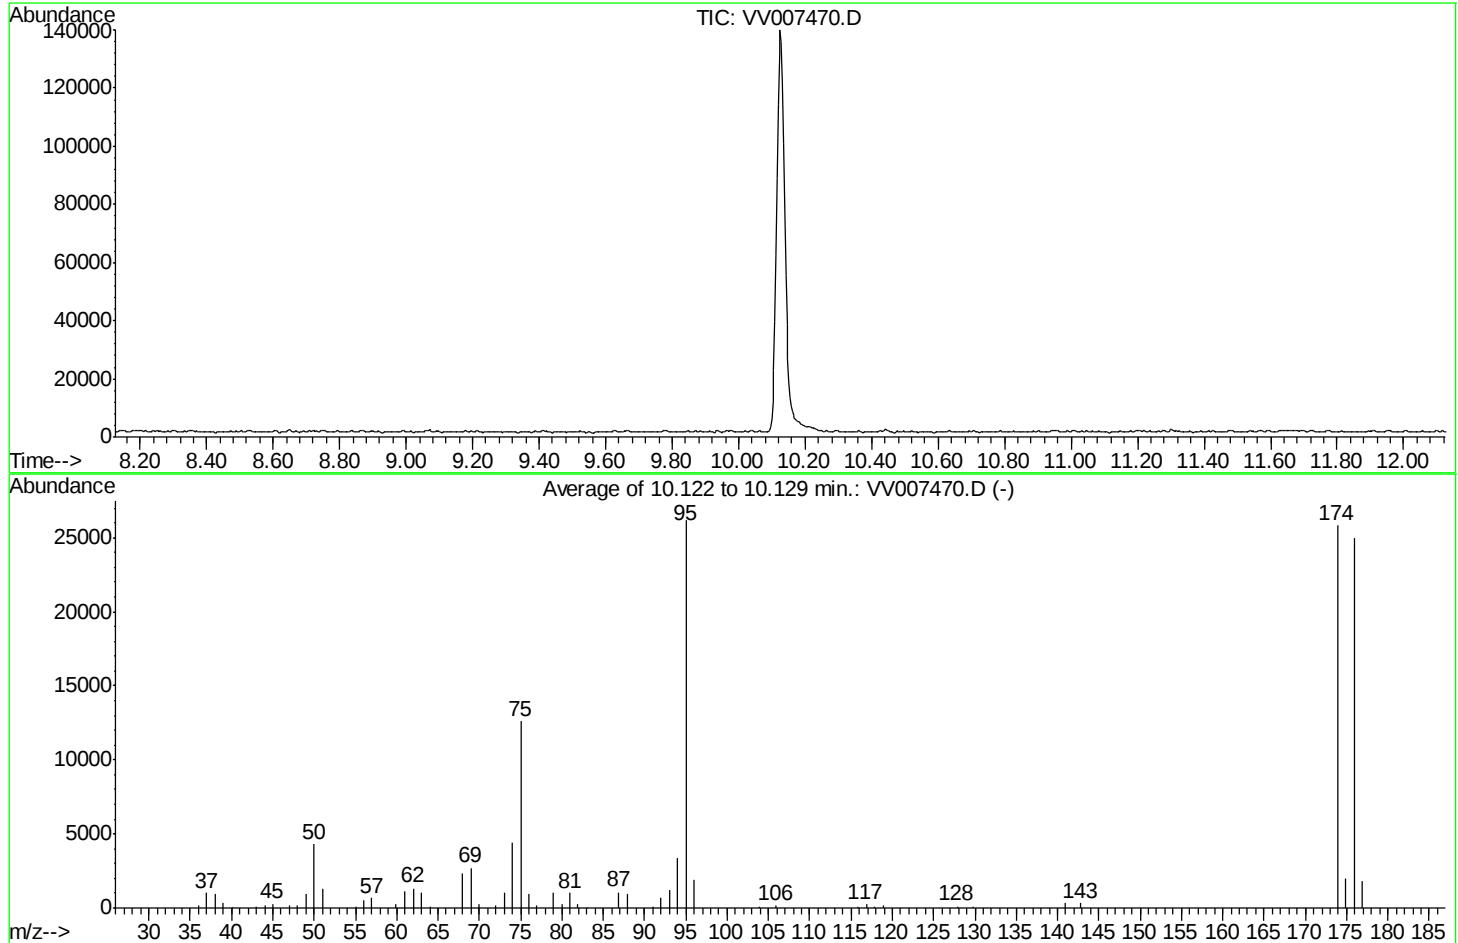

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	4321	PASS
75	95	30	80	48.2	12615	PASS
95	95	100	100	100.0	26173	PASS
96	95	5	9	7.1	1871	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.6	25808	PASS
175	174	5	9	7.9	2031	PASS
176	174	95	101	96.9	25016	PASS
177	176	5	9	7.1	1778	PASS

Scan 2797 (10.084 min): VV007470.D
BFB70

m/z	Abundance
39.00	150.0
41.00	190.0
42.00	140.0
42.90	238.0
44.00	509.0
55.00	161.0
57.00	130.0
207.00	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.00	175.0
37.00	1028.0
38.00	988.0
39.00	527.0
40.00	106.0
41.00	175.0
41.90	131.0
43.00	301.0
44.00	707.0
45.00	268.0
46.90	208.0
47.90	151.0
49.00	927.0
50.00	4185.0
51.00	1245.0
55.00	225.0
56.00	522.0
57.00	804.0
59.90	284.0
61.00	1000.0
62.00	1284.0
63.00	1090.0
64.00	124.0
68.00	2342.0
69.00	2622.0
70.00	252.0
71.90	152.0
73.00	1031.0
74.00	4248.0
75.00	12355.0
76.10	1005.0
76.90	163.0
78.90	1045.0
80.00	305.0
81.00	965.0
81.90	301.0
86.90	1075.0
87.90	977.0
91.00	116.0
92.00	684.0
93.00	1244.0
94.00	3298.0
95.00	25536.0
96.00	1818.0
103.90	129.0
106.00	151.0
115.90	149.0
116.90	238.0
117.80	174.0
118.90	159.0
127.90	136.0
129.80	111.0
140.90	295.0
142.80	312.0
173.90	24520.0
174.90	1895.0
175.90	24072.0
177.00	1680.0
207.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	158.0
37.00	1065.0
38.00	1041.0
39.00	504.0
41.10	186.0
41.90	117.0
43.00	302.0
44.00	725.0
45.00	285.0
47.00	221.0
47.90	177.0
49.00	952.0
50.00	4446.0
51.00	1264.0
55.00	255.0
56.00	541.0
57.00	809.0
60.00	292.0
61.00	1128.0
62.00	1363.0
63.00	1063.0
64.00	105.0
68.00	2424.0
69.00	2783.0
70.00	280.0
71.90	147.0
73.00	1084.0
74.00	4582.0
75.00	12925.0
76.10	956.0
76.90	178.0
78.90	1099.0
80.00	311.0
81.00	1064.0
81.90	288.0
82.90	102.0
86.90	1106.0
87.90	1049.0
90.90	124.0
92.00	747.0
93.00	1214.0
94.00	3457.0
95.00	26928.0
96.00	1917.0
103.90	132.0
106.00	156.0
115.90	125.0
116.90	236.0
117.80	156.0
118.90	162.0
127.80	132.0
129.80	101.0
140.90	309.0
142.90	344.0
173.90	26536.0
174.90	2090.0
175.90	25744.0
177.00	1862.0
207.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	145.0
37.00	1017.0
38.00	958.0
39.00	450.0
41.10	182.0
41.90	107.0
43.00	318.0
44.00	719.0
45.00	296.0
47.00	226.0
48.00	169.0
49.00	902.0
50.00	4334.0
51.00	1259.0
55.00	273.0
56.00	495.0
57.00	731.0
60.00	277.0
61.00	1180.0
62.00	1329.0
63.00	966.0
68.00	2353.0
69.00	2703.0
70.00	293.0
71.90	131.0
73.00	1039.0
74.00	4493.0
75.00	12566.0
76.00	924.0
77.00	184.0
78.90	1049.0
80.00	291.0
81.00	1078.0
81.90	256.0
86.90	1011.0
88.00	962.0
90.90	139.0
92.00	766.0
93.00	1118.0
94.00	3335.0
95.00	26056.0
96.00	1880.0
103.80	133.0
105.90	157.0
115.80	107.0
116.90	185.0
118.90	161.0
127.80	123.0
140.90	326.0
142.90	369.0
173.90	26368.0
174.90	2108.0
175.90	25232.0
176.90	1792.0
207.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70