

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091222\
 Data File : VV027806.D
 Acq On : 12 Sep 2022 13:03
 Operator : SY/MD
 Sample : N4015-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT3-2022-05

Quant Time: Sep 13 03:23:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 10 02:33:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	4170	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.848	117	3689	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	2554	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.295	65	1320	0.511	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 102.000%	
4) 1,2-Dichloroethane-d4	5.018	65	1015	0.522	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	= 104.000%	
7) 1,2-Dichloropropane-d6	6.068	67	656	0.534	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 106.000%	
8) Toluene-d8	7.317	98	3601	0.529	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 106.000%	
10) 1,1,2,2-Tetrachloroeth...	10.216	84	575	0.546	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 110.000%	
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.295	62	41	0.017	ug/L #	1
6) Trichloroethene	5.901	95	56	0.024	ug/L	68
9) 1,2-Dibromoethane	8.353	107	32	0.024	ug/L #	70
12) 1,2,3-Trichloropropane	10.267	75	16	0.019	ug/L #	55
13) 1,2-Dibromo-3-chloropr...	12.392	75	5	0.030	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091222\
Data File : VV027806.D
Acq On : 12 Sep 2022 13:03
Operator : SY/MD
Sample : N4015-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT3-2022-05

Quant Time: Sep 13 03:23:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 10 02:33:14 2022
Response via : Initial Calibration




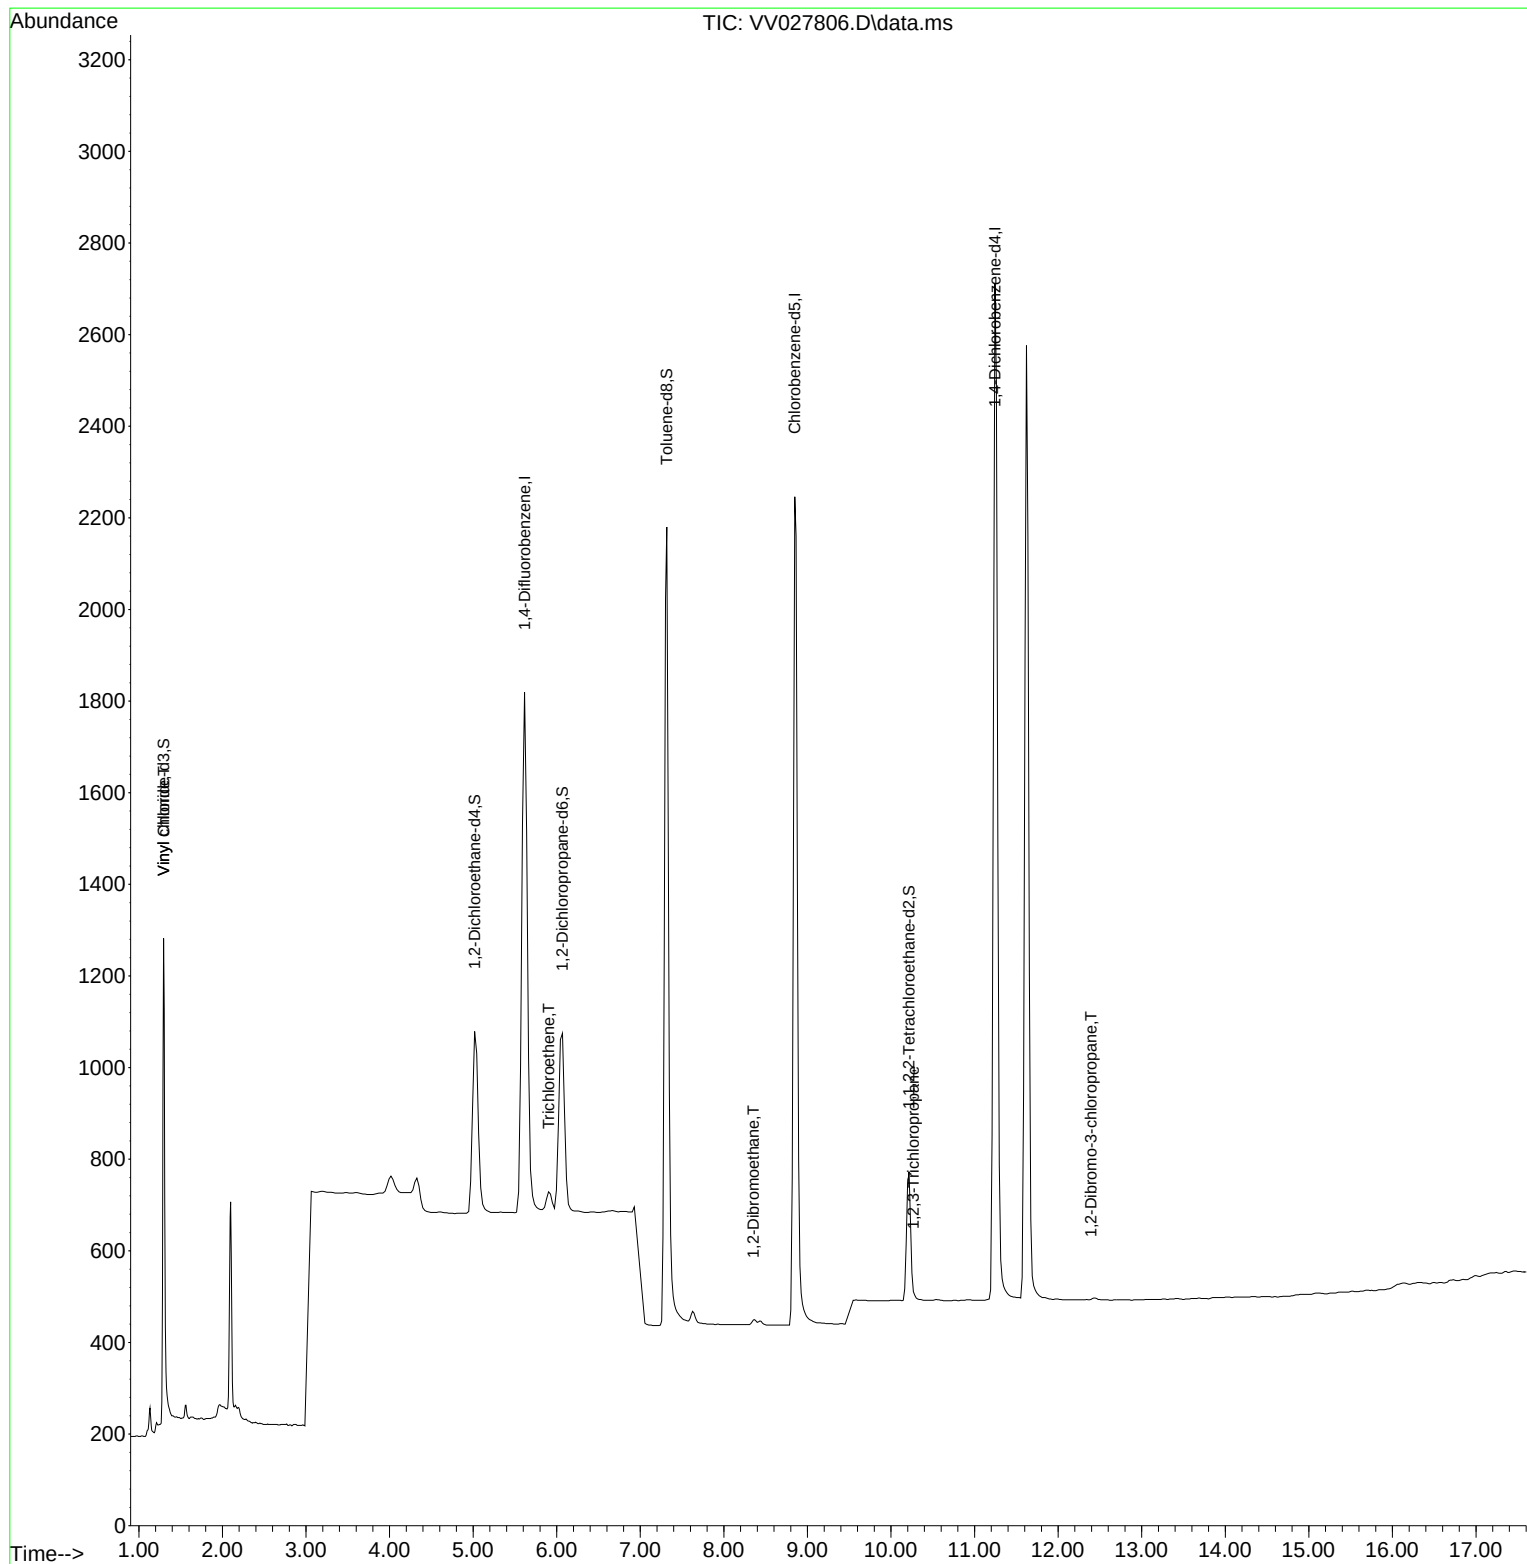


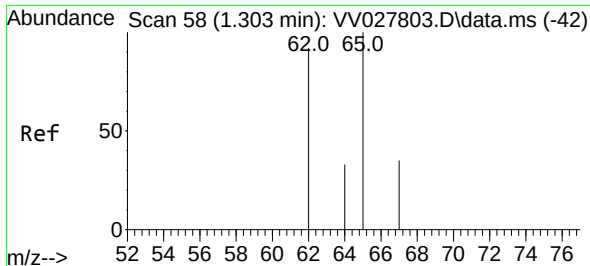

#3
 Vinyl chloride
 Concen: 0.017 ug/L
 RT: 1.295 min Scan# 51
 Delta R.T. -0.007 min
 Lab File: VV027806.D
 Acq: 12 Sep 2022 13:03




Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT3-2022-05


Tgt Ion: 62 Resp: 41
 Ion Ratio Lower Upper
 62 100
 64 106.6 27.8 51.6#

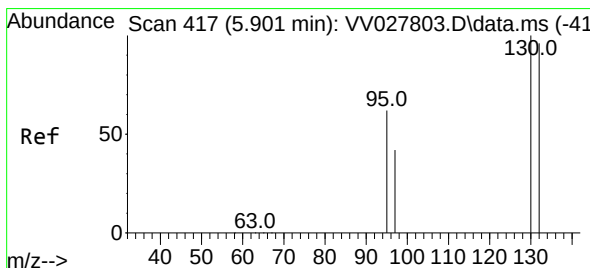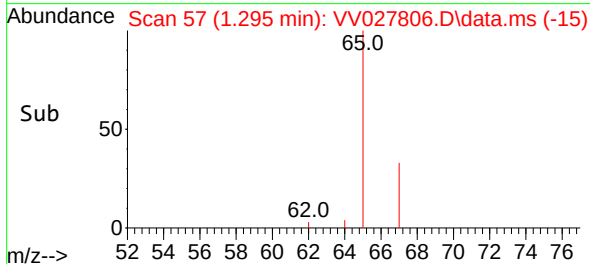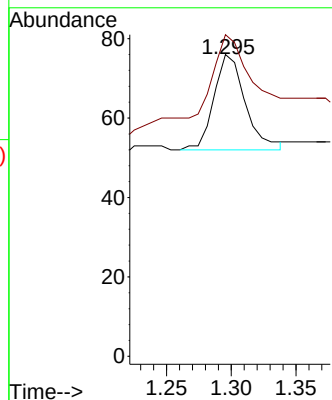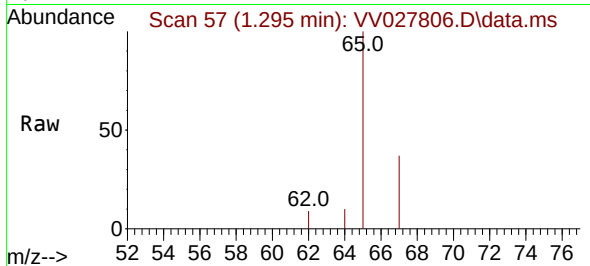

#6
 Trichloroethene
 Concen: 0.024 ug/L
 RT: 5.901 min Scan# 417
 Delta R.T. -0.024 min
 Lab File: VV027806.D
 Acq: 12 Sep 2022 13:03


Tgt Ion: 95 Resp: 56
 Ion Ratio Lower Upper
 95 100
 97 93.1 50.6 94.0
 132 106.9 103.6 192.4
 130 105.2 104.9 194.7

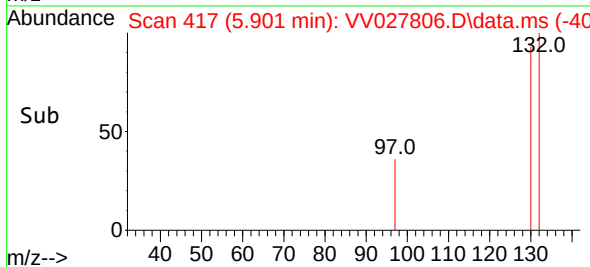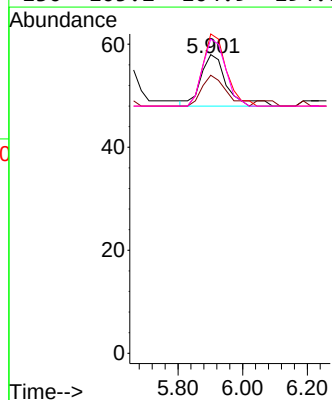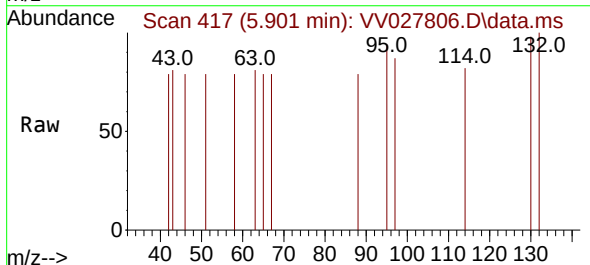



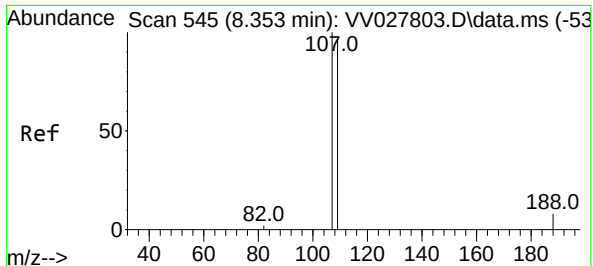


#9
1,2-Dibromoethane
Concen: 0.024 ug/L
RT: 8.353 min Scan# 545
Delta R.T. -0.000 min
Lab File: VV027806.D
Acq: 12 Sep 2022 13:03

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT3-2022-05



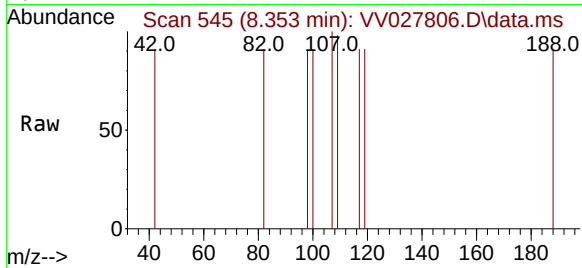



Tgt Ion:107 Resp: 32
Ion Ratio Lower Upper
107 100
109 98.1 66.6 123.8
188 90.7 19.0 28.6#

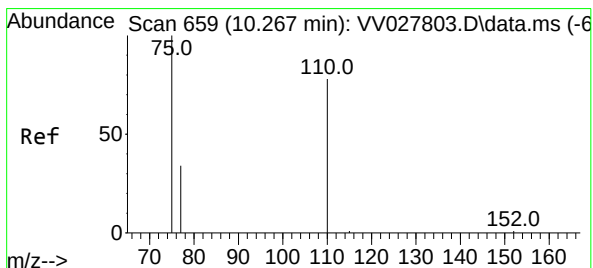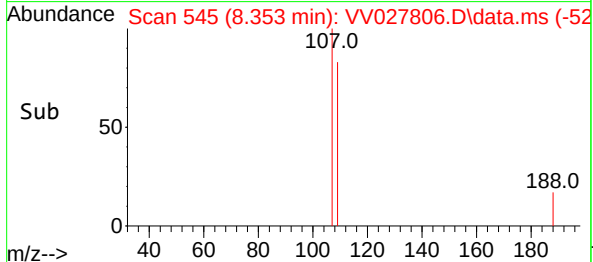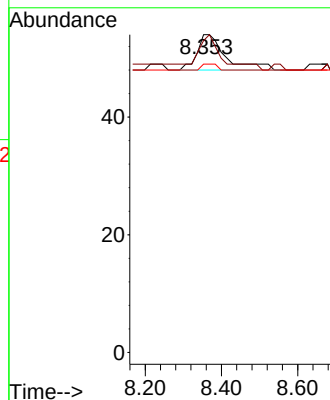

#12
1,2,3-Trichloropropane
Concen: 0.019 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV027806.D
Acq: 12 Sep 2022 13:03


Tgt Ion: 75 Resp: 16
Ion Ratio Lower Upper
75 100
110 37.5 55.5 83.3#
77 0.0 26.2 39.2#

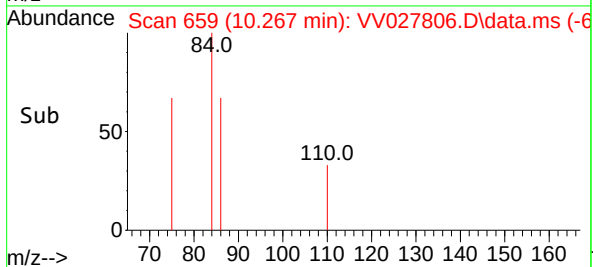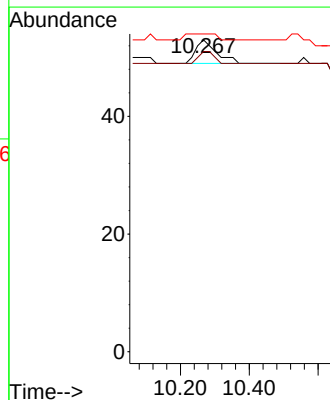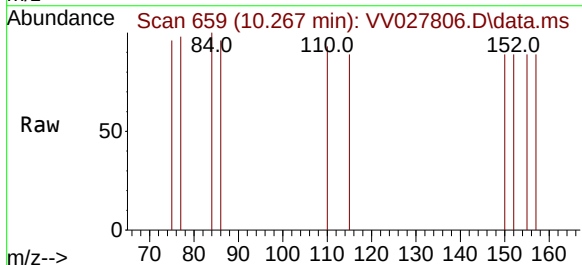

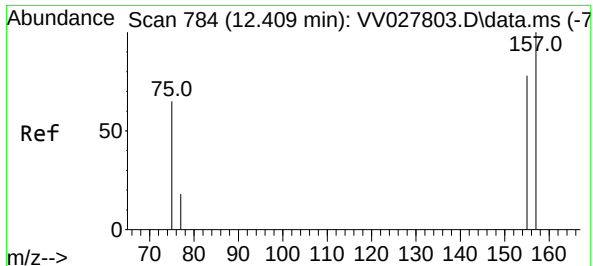

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.030 ug/L
 RT: 12.392 min Scan# 784
 Delta R.T. -0.017 min
 Lab File: VV027806.D
 Acq: 12 Sep 2022 13:03

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT3-2022-05

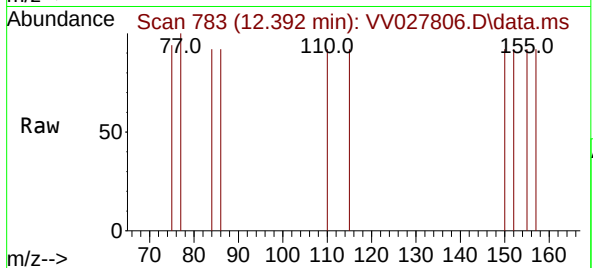

Tgt Ion: 75	Resp: 5
Ion Ratio	Lower Upper
75 100	
157 98.0	94.2 141.2
155 98.0	86.1 129.1

