
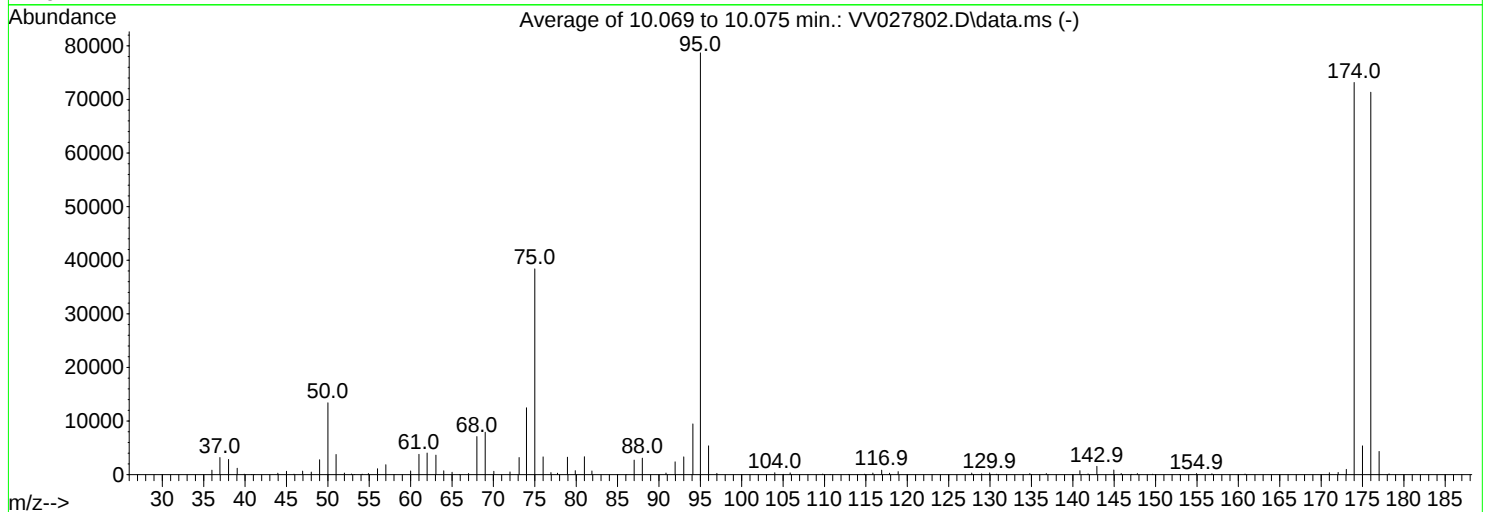


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091222\
 Data File : VV027802.D
 Acq On : 12 Sep 2022 09:54
 Operator : SY/MD
 Sample : BFB205
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Sep 10 02:33:14 2022

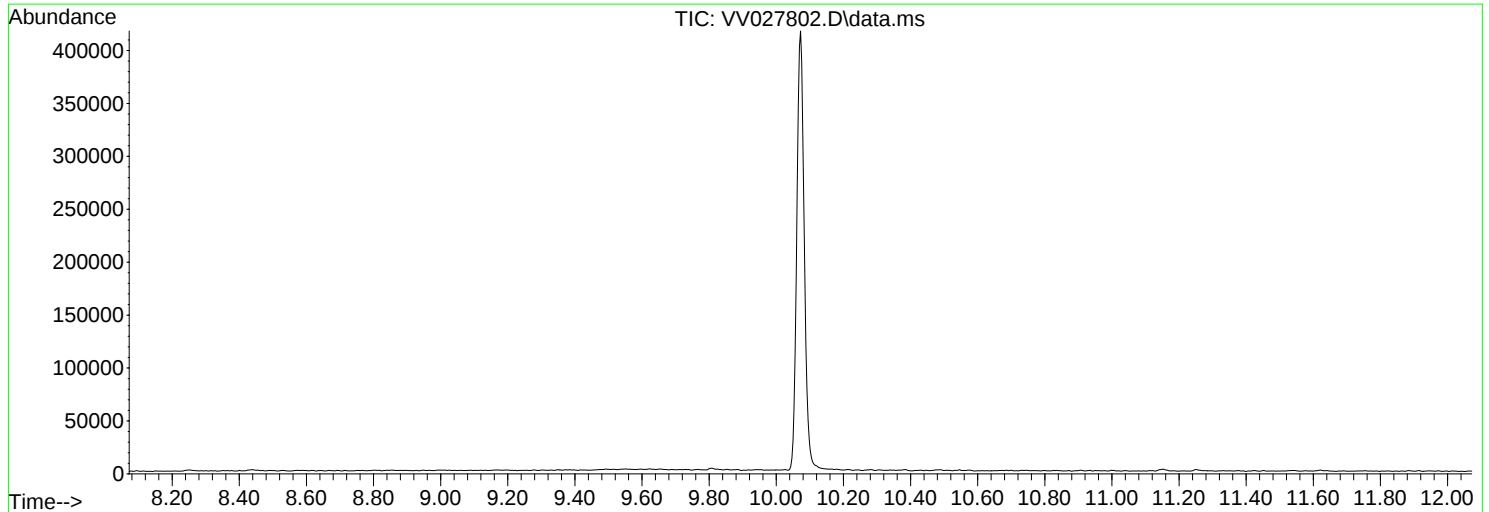

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	13396	PASS
75	95	30	80	48.8	38397	PASS
95	95	100	100	100.0	78688	PASS
96	95	5	9	6.8	5368	PASS
173	174	0.00	2	1.4	1003	PASS
174	95	50	120	93.0	73163	PASS
175	174	5	9	7.3	5366	PASS
176	174	95	101	97.5	71328	PASS
177	176	5	9	6.1	4322	PASS

m/z	Abundance
35.10	292.0
36.00	916.0
36.90	142.0
38.10	439.0
39.90	1813.0
44.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1784.0
37.00	3269.0
38.00	3443.0
39.10	1228.0
39.90	1752.0
41.10	115.0
44.10	457.0
45.00	690.0
45.90	143.0
47.00	645.0
48.00	429.0
49.00	2775.0
50.00	13668.0
51.00	3829.0
52.00	295.0
52.80	130.0
53.20	117.0
54.10	130.0
54.80	204.0
56.00	1130.0
57.00	1788.0
58.00	102.0
60.00	720.0
61.00	3886.0
62.00	4160.0
63.10	3660.0
64.00	732.0
65.00	427.0
65.90	131.0
67.10	175.0
68.00	6943.0
69.00	7976.0
70.00	634.0
72.00	549.0
73.10	2933.0
74.00	12563.0
75.00	38520.0
76.00	3429.0
76.90	352.0
77.90	263.0
78.90	3261.0
79.90	738.0
81.00	3335.0
81.90	671.0
87.00	2762.0
88.00	3190.0
90.90	315.0
91.90	2568.0
93.00	3204.0
94.10	9559.0
95.00	78816.0
96.00	5512.0
97.00	213.0
104.10	374.0
105.80	358.0
109.80	112.0
110.70	116.0
112.90	104.0
114.80	118.0
115.80	269.0
116.90	847.0
117.90	273.0
118.80	547.0
127.80	264.0
129.00	124.0
129.90	320.0
130.80	127.0
134.80	193.0
136.80	245.0
140.90	728.0
141.80	178.0
142.90	1560.0
145.00	763.0
145.90	176.0
147.80	195.0
149.60	104.0
150.00	120.0
155.00	196.0
156.80	210.0
170.90	385.0
172.10	403.0
173.00	995.0
174.00	73152.0
175.00	5303.0
176.00	69704.0
177.00	4305.0
178.20	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1823.0
37.00	3468.0
38.00	3399.0
39.10	1216.0
39.90	1952.0
40.80	118.0
43.90	448.0
45.00	648.0
45.90	123.0
47.00	706.0
48.00	489.0
49.00	2911.0
50.00	13953.0
51.00	3875.0
52.00	301.0
52.80	147.0
54.20	114.0
54.90	202.0
56.00	1152.0
57.00	1903.0
60.00	730.0
61.00	3980.0
62.00	4208.0
63.10	3832.0
64.00	740.0
65.00	485.0
67.00	207.0
68.00	7350.0
69.00	8194.0
70.10	656.0
72.00	543.0
73.10	3297.0
74.00	12999.0
75.00	39824.0
76.00	3481.0
77.00	379.0
77.70	264.0
79.00	3331.0
79.90	775.0
81.00	3510.0
81.90	714.0
87.00	2789.0
88.00	3220.0
90.90	320.0
91.90	2491.0
93.00	3415.0
94.10	9760.0
95.00	81304.0
96.00	5594.0
97.00	246.0
104.00	351.0
105.00	109.0
105.80	350.0
109.80	126.0
113.00	117.0
114.90	122.0
115.90	316.0
116.90	900.0
117.80	276.0
118.90	581.0
127.80	303.0
129.00	146.0
130.00	353.0
130.80	107.0
134.80	211.0
136.80	208.0
140.90	765.0
141.90	153.0
142.90	1620.0
145.00	869.0
145.90	213.0
147.10	115.0
147.80	240.0
149.70	107.0
155.00	206.0
156.80	188.0
160.80	165.0
171.00	384.0
172.10	446.0
173.00	997.0
174.00	75592.0
175.00	5595.0
176.00	73976.0
177.00	4442.0
178.20	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1687.0
37.00	3252.0
38.00	2970.0
39.00	1111.0
40.00	2006.0
43.80	532.0
45.00	591.0
46.90	666.0
48.00	502.0
49.00	2641.0
50.00	12568.0
51.00	3631.0
52.00	277.0
52.90	120.0
55.00	227.0
56.00	1050.0
57.00	1904.0
60.00	658.0
61.00	3541.0
62.00	3733.0
63.00	3483.0
64.00	673.0
65.00	469.0
66.90	223.0
68.00	7058.0
69.00	7529.0
70.10	589.0
72.00	454.0
73.10	3328.0
74.00	11850.0
75.00	36848.0
76.00	3063.0
77.00	408.0
77.70	266.0
79.00	3198.0
79.90	721.0
81.00	3179.0
81.90	647.0
86.10	101.0
87.00	2607.0
88.00	2847.0
90.80	297.0
92.00	2109.0
93.00	3297.0
94.10	9077.0
95.00	75944.0
96.00	4997.0
97.00	275.0
103.90	331.0
105.10	108.0
105.90	326.0
109.80	109.0
115.90	321.0
116.90	774.0
117.90	265.0
119.00	582.0
127.80	326.0
129.00	171.0
130.00	325.0
134.80	183.0
136.80	173.0
140.80	768.0
141.80	125.0
142.90	1455.0
144.90	946.0
145.80	201.0
147.10	106.0
147.80	247.0
149.70	105.0
152.90	107.0
154.90	200.0
156.80	151.0
160.80	191.0
171.10	357.0
172.00	445.0
173.10	1018.0
174.00	70744.0
175.00	5200.0
176.00	70304.0
177.00	4218.0
178.20	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205