

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091223\
 Data File : VW032051.D
 Acq On : 12 Sep 2023 16:15
 Operator : SY/MD
 Sample : 04332-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 13 06:57:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	218810	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	210555	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	106533	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	64617	47.187	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.380%		
7) Chloroethane-d5	1.529	69	54539	45.433	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.860%		
11) 1,1-Dichloroethene-d2	2.060	65	26484	41.303	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.600%		
21) 2-Butanone-d5	3.793	46	116947	108.584	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.580%		
24) Chloroform-d	4.253	84	119539	39.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.880%		
26) 1,2-Dichloroethane-d4	4.947	65	79473	40.010	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.020%		
32) Benzene-d6	4.963	84	249857	43.488	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.980%		
36) 1,2-Dichloropropane-d6	5.992	67	84873	45.896	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.800%		
41) Toluene-d8	7.249	98	220918	41.731	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.460%		
43) trans-1,3-Dichloroprop...	7.558	79	38163	39.816	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.640%		
47) 2-Hexanone-d5	8.031	63	68478	120.817	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	120.820%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	107138	44.834	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.660%		
66) 1,2-Dichlorobenzene-d4	11.564	152	84483	43.502	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.000%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	4603	4.802	ug/L	91
61) 1,2,3-Trichloropropane	11.188	75	14501	7.205	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032051.D
Acq On : 12 Sep 2023 16:15
Operator : SY/MD
Sample : 04332-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 13 06:57:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

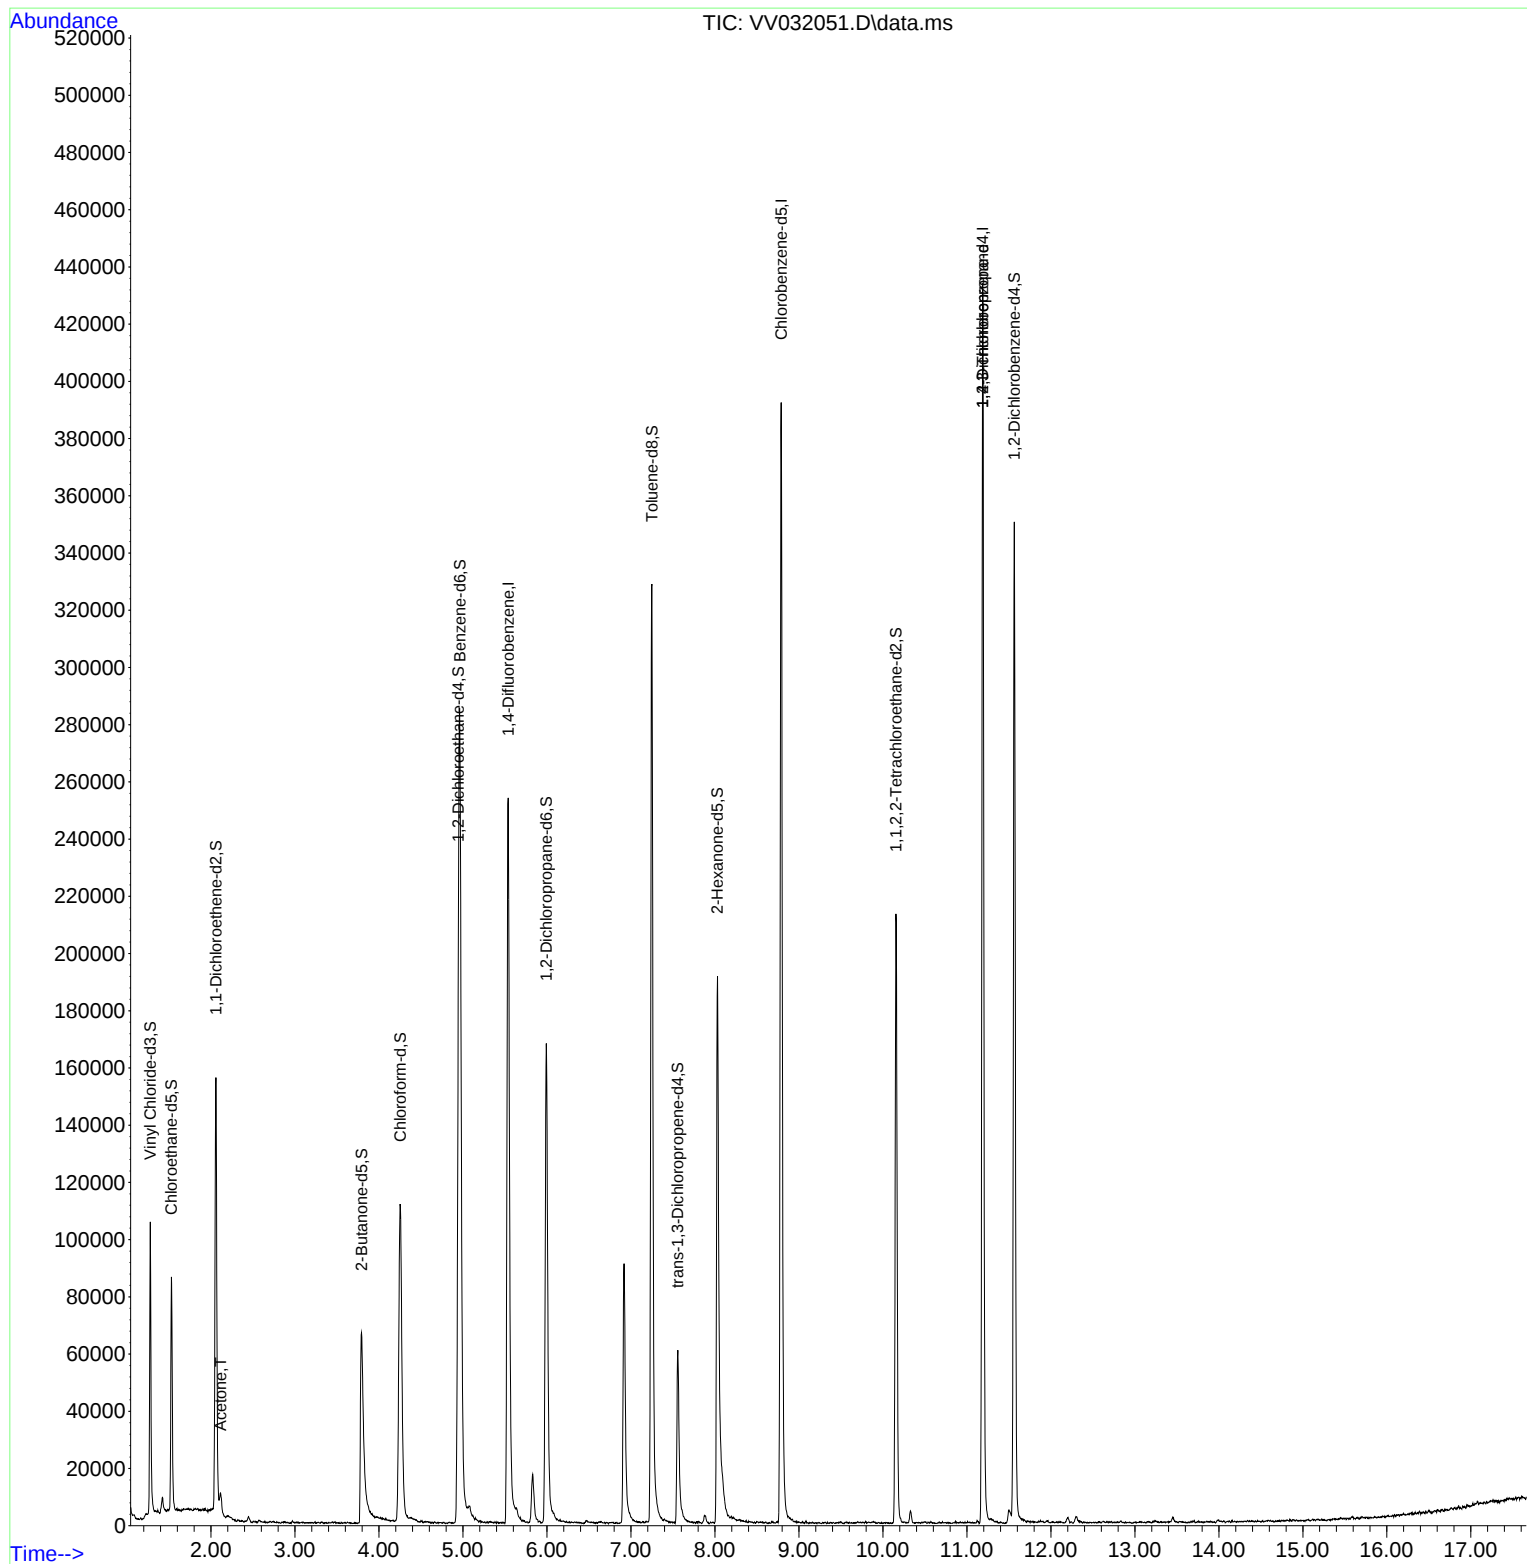

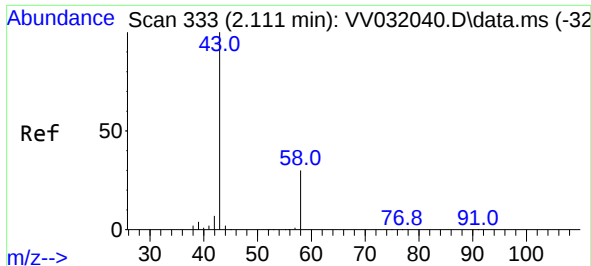

#13

Acetone

Concen: 4.802 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032051.D

Acq: 12 Sep 2023 16:15

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 4603

Ion Ratio Lower Upper

43 100

58 35.3 0.0 61.0

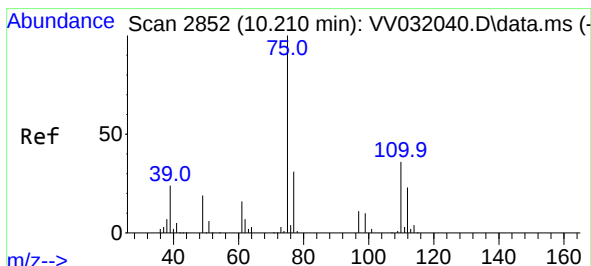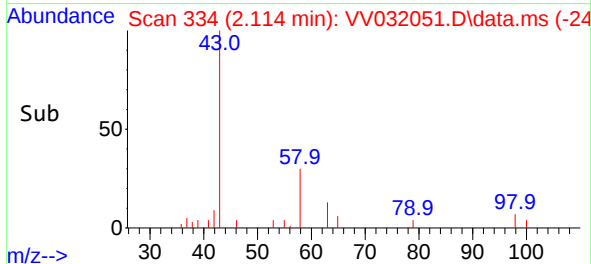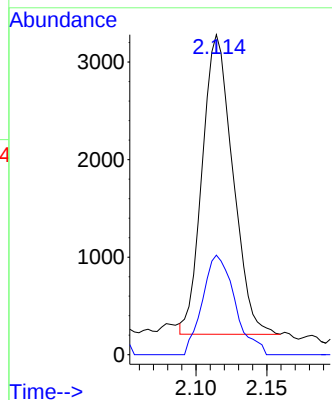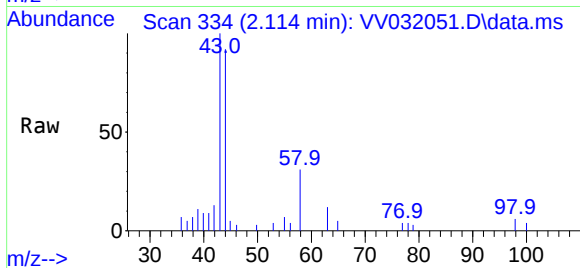

#61

1,2,3-Trichloropropane

Concen: 7.205 ug/L

RT: 11.188 min Scan# 3156

Delta R.T. 0.974 min

Lab File: VV032051.D

Acq: 12 Sep 2023 16:15

Tgt Ion: 75 Resp: 14501

Ion Ratio Lower Upper

75 100

77 33.8 25.7 38.5

110 2.5 30.3 45.5#

