

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032054.D
 Acq On : 12 Sep 2023 17:26
 Operator : SY/MD
 Sample : 04386-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 13 06:57:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	227932	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	225293	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	113436	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	61574	43.165	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.320%	
7) Chloroethane-d5	1.529	69	51747	41.382	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	82.760%	
11) 1,1-Dichloroethene-d2	2.060	65	25274	37.838	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.680%	
21) 2-Butanone-d5	3.790	46	119106	106.162	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.160%	
24) Chloroform-d	4.253	84	118961	38.154	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	76.300%	
26) 1,2-Dichloroethane-d4	4.947	65	78839	38.102	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	76.200%	
32) Benzene-d6	4.963	84	246014	40.018	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	80.040%	
36) 1,2-Dichloropropane-d6	5.995	67	84454	42.681	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.360%	
41) Toluene-d8	7.246	98	217045	38.317	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	76.640%#	
43) trans-1,3-Dichloroprop...	7.558	79	36649	35.735	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.460%	
47) 2-Hexanone-d5	8.031	63	66908	110.324	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	110.320%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	107006	41.849	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	83.700%	
66) 1,2-Dichlorobenzene-d4	11.564	152	82344	39.821	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	79.640%#	
Target Compounds						Qvalue
13) Acetone	2.114	43	5054	5.061	ug/L	96
61) 1,2,3-Trichloropropane	11.188	75	14968	6.984	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032054.D
Acq On : 12 Sep 2023 17:26
Operator : SY/MD
Sample : 04386-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 13 06:57:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

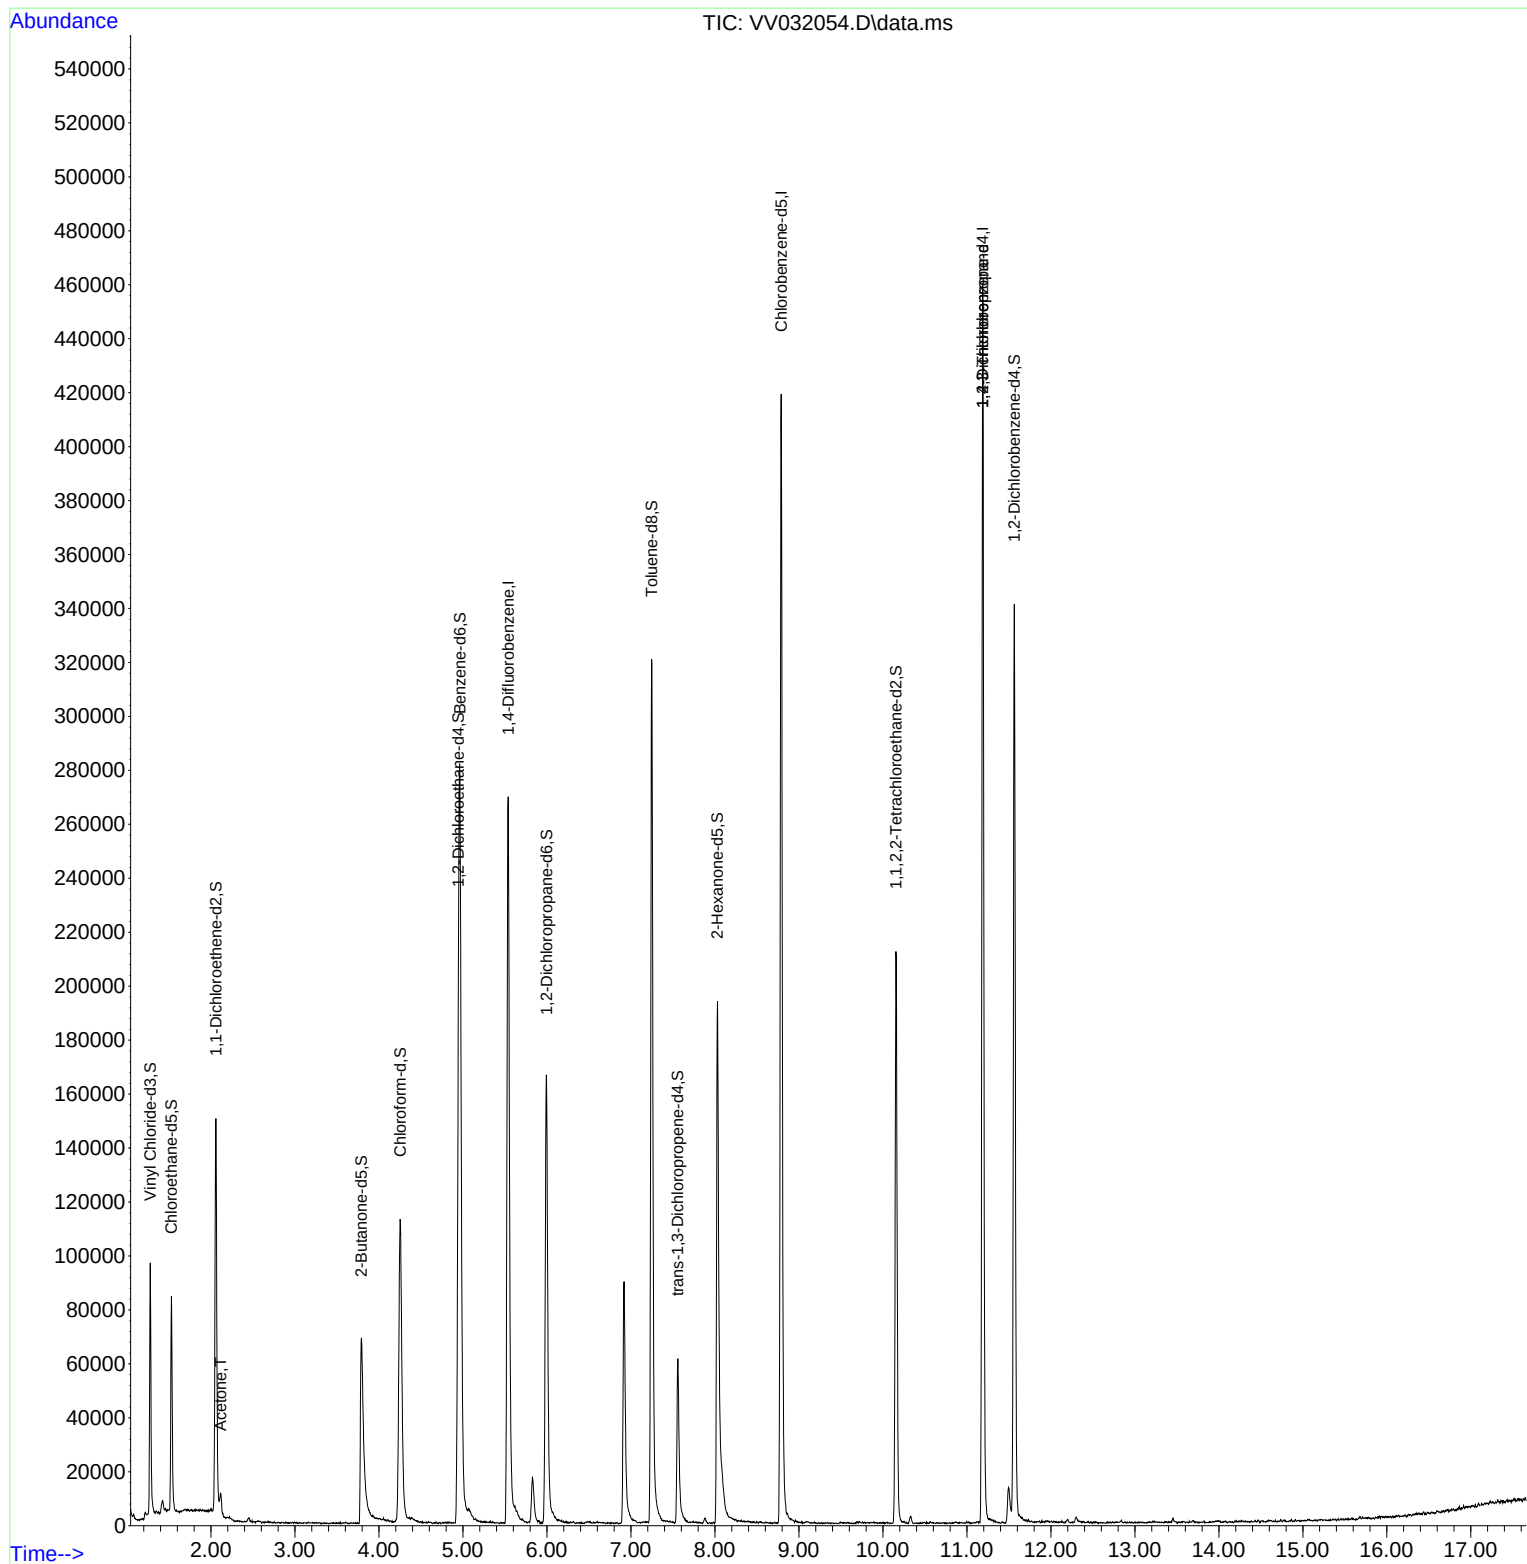

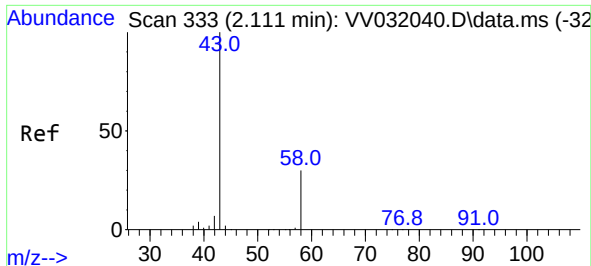

#13

Acetone

Concen: 5.061 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032054.D

Acq: 12 Sep 2023 17:26

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 5054

Ion Ratio Lower Upper

43 100

58 32.7 0.0 61.0

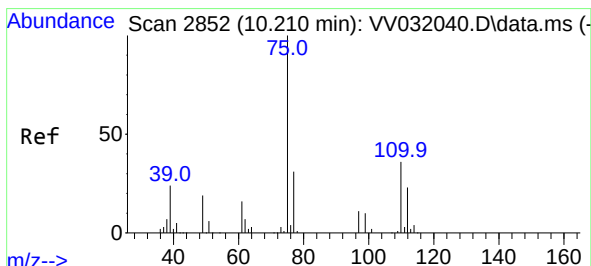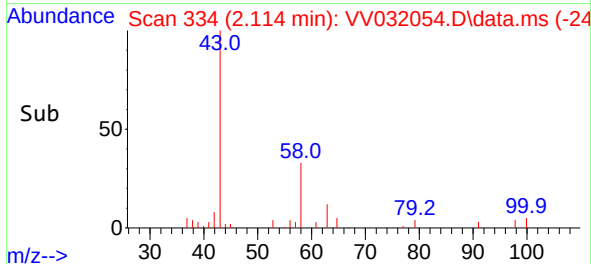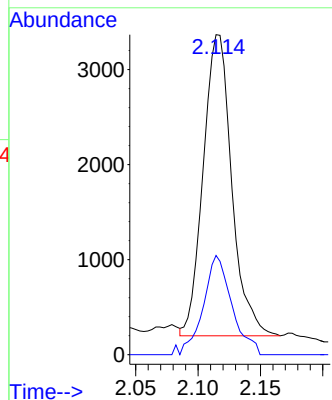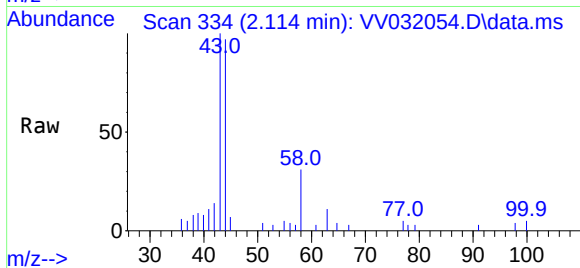

#61

1,2,3-Trichloropropane

Concen: 6.984 ug/L

RT: 11.188 min Scan# 3156

Delta R.T. 0.974 min

Lab File: VV032054.D

Acq: 12 Sep 2023 17:26

Tgt Ion: 75 Resp: 14968

Ion Ratio Lower Upper

75 100

77 32.1 25.7 38.5

110 2.3 30.3 45.5#

