

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032045.D
 Acq On : 12 Sep 2023 13:54
 Operator : SY/MD
 Sample : 04330-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP2

Quant Time: Sep 13 06:56:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	250924	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	245005	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	121660	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	69050	43.970	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.940%
7) Chloroethane-d5	1.532	69	57524	41.787	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.580%
11) 1,1-Dichloroethene-d2	2.059	65	28749	39.097	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.200%
21) 2-Butanone-d5	3.789	46	121181	98.115	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.110%
24) Chloroform-d	4.252	84	127952	37.278	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.560%
26) 1,2-Dichloroethane-d4	4.947	65	84262	36.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.980%
32) Benzene-d6	4.963	84	269363	40.291	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.580%
36) 1,2-Dichloropropane-d6	5.992	67	92199	42.847	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.700%
41) Toluene-d8	7.249	98	239223	38.835	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.660%#
43) trans-1,3-Dichloroprop...	7.558	79	40364	36.191	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.380%
47) 2-Hexanone-d5	8.027	63	71501	108.412	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.410%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	112054	40.298	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	80.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	89356	40.290	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.580%
Target Compounds						
13) Acetone	2.114	43	8858	8.058	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032045.D
Acq On : 12 Sep 2023 13:54
Operator : SY/MD
Sample : 04330-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP2

Quant Time: Sep 13 06:56:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

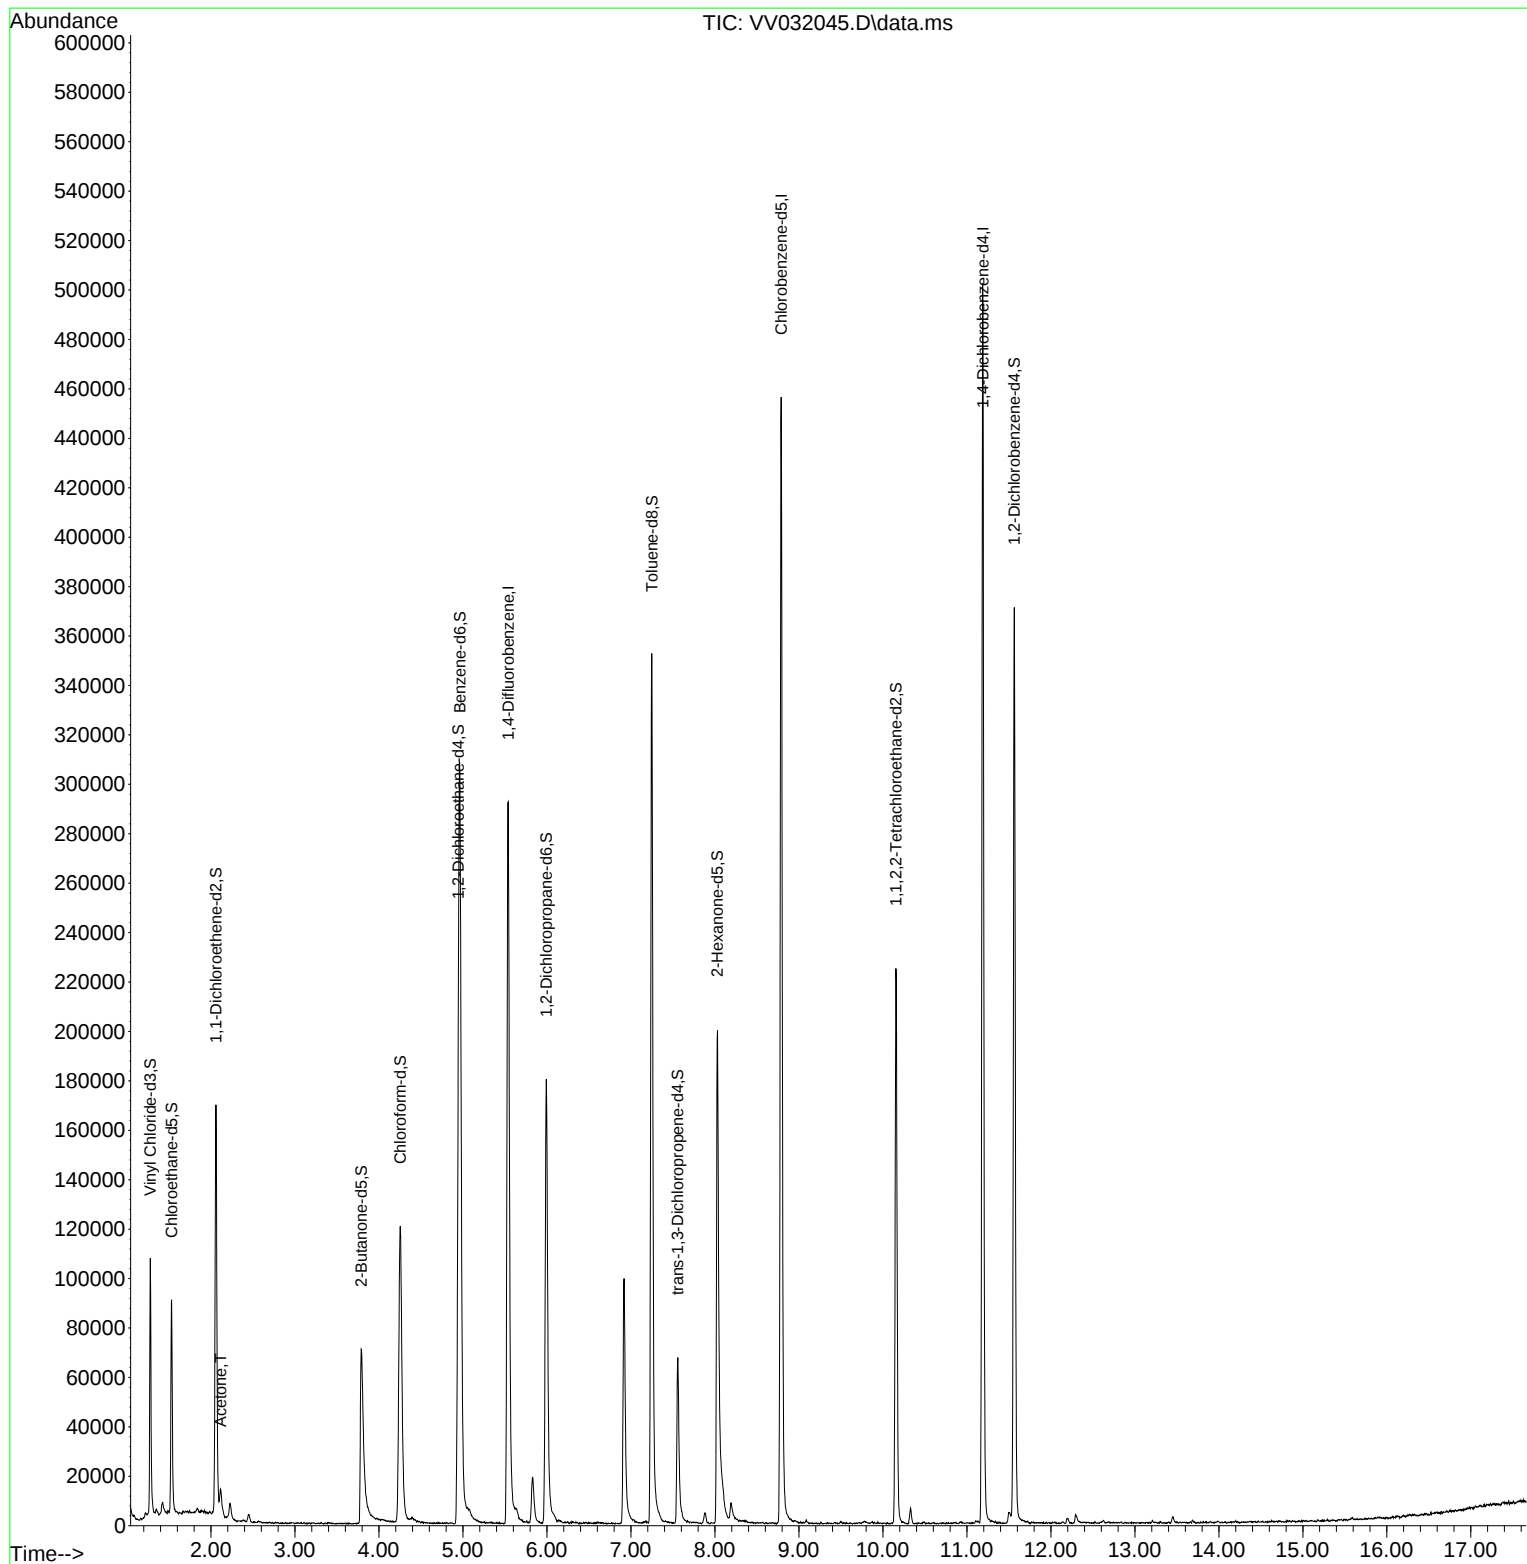

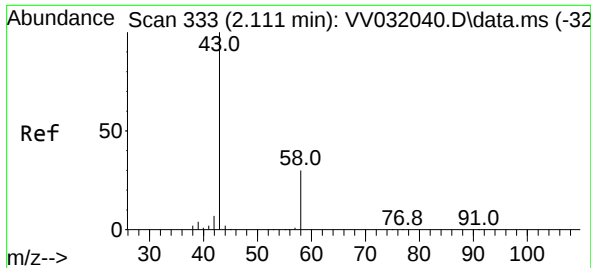

#13

Acetone

Concen: 8.058 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032045.D

Acq: 12 Sep 2023 13:54

Instrument :

MSVOA_V

ClientSampleId :

EZYP2

Tgt Ion: 43 Resp: 8858

Ion Ratio Lower Upper

43 100

58 30.6 0.0 61.0

