

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032046.D
 Acq On : 12 Sep 2023 14:18
 Operator : SY/MD
 Sample : 04330-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR7

Quant Time: Sep 13 06:56:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	244771	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	237357	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	118375	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	70665	46.130	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.260%
7) Chloroethane-d5	1.529	69	58706	43.717	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.440%
11) 1,1-Dichloroethene-d2	2.060	65	29905	41.691	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.380%
21) 2-Butanone-d5	3.790	46	128646	106.777	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.780%
24) Chloroform-d	4.256	84	132638	39.614	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.220%
26) 1,2-Dichloroethane-d4	4.944	65	88320	39.748	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.500%
32) Benzene-d6	4.963	84	276802	42.738	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.480%
36) 1,2-Dichloropropane-d6	5.992	67	94064	45.122	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.240%
41) Toluene-d8	7.246	98	248459	41.634	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.260%
43) trans-1,3-Dichloroprop...	7.558	79	41405	38.320	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.640%
47) 2-Hexanone-d5	8.031	63	74785	117.045	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	117.050%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	115147	42.744	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.480%
66) 1,2-Dichlorobenzene-d4	11.564	152	92465	42.849	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.700%
Target Compounds						
13) Acetone	2.114	43	9746	9.088	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032046.D
Acq On : 12 Sep 2023 14:18
Operator : SY/MD
Sample : 04330-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR7

Quant Time: Sep 13 06:56:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

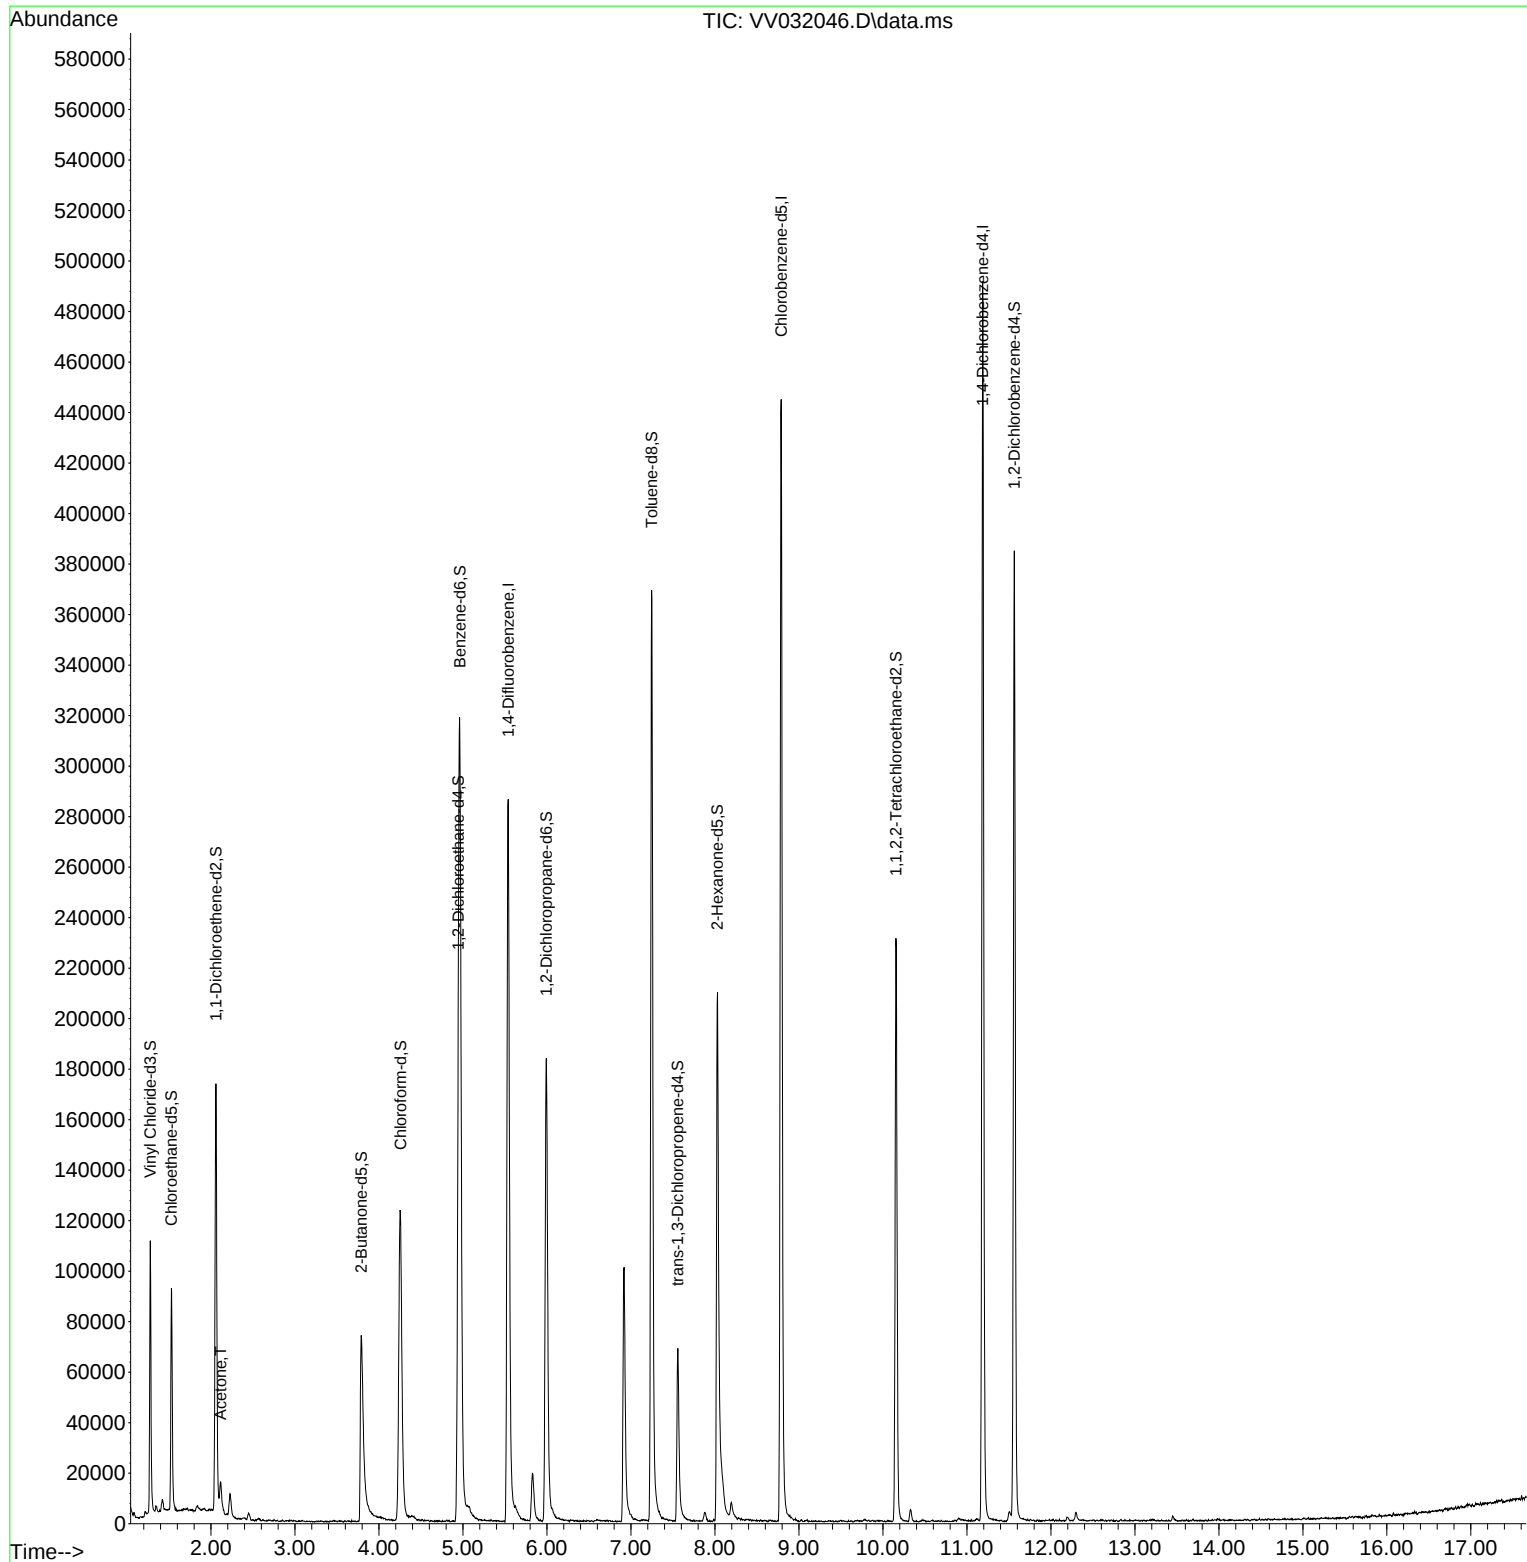

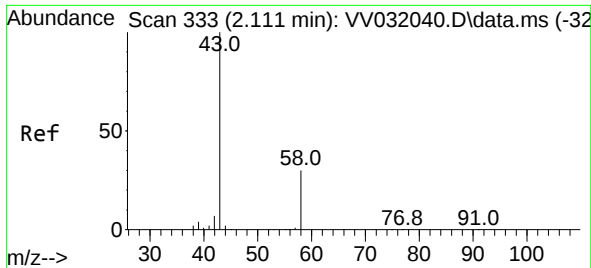

#13

Acetone

Concen: 9.088 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032046.D


Acq: 12 Sep 2023 14:18

Instrument :

MSVOA_V

ClientSampleId :

EZYR7

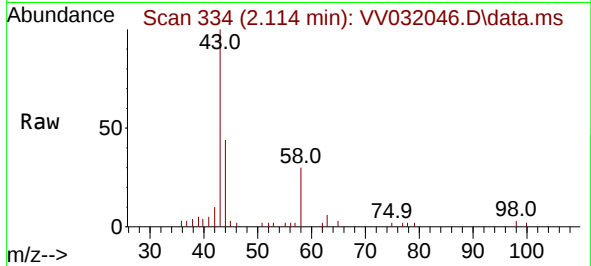

Tgt Ion: 43 Resp: 9746

Ion Ratio Lower Upper

43 100

58 33.6 0.0 61.0

