

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091223\
 Data File : VW032051.D
 Acq On : 12 Sep 2023 16:15
 Operator : SY/MD
 Sample : 04332-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL1

Quant Time: Sep 13 06:57:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	218810	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	210555	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	106533	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	64617	47.187	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.380%
7) Chloroethane-d5	1.529	69	54539	45.433	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.860%
11) 1,1-Dichloroethene-d2	2.060	65	26484	41.303	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.600%
21) 2-Butanone-d5	3.793	46	116947	108.584	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.580%
24) Chloroform-d	4.253	84	119539	39.938	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.880%
26) 1,2-Dichloroethane-d4	4.947	65	79473	40.010	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.020%
32) Benzene-d6	4.963	84	249857	43.488	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.980%
36) 1,2-Dichloropropane-d6	5.992	67	84873	45.896	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.800%
41) Toluene-d8	7.249	98	220918	41.731	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.460%
43) trans-1,3-Dichloroprop...	7.558	79	38163	39.816	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.640%
47) 2-Hexanone-d5	8.031	63	68478	120.817	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	120.820%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	107138	44.834	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.660%
66) 1,2-Dichlorobenzene-d4	11.564	152	84483	43.502	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.000%
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	4603	4.802	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032051.D
Acq On : 12 Sep 2023 16:15
Operator : SY/MD
Sample : 04332-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL1

Quant Time: Sep 13 06:57:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

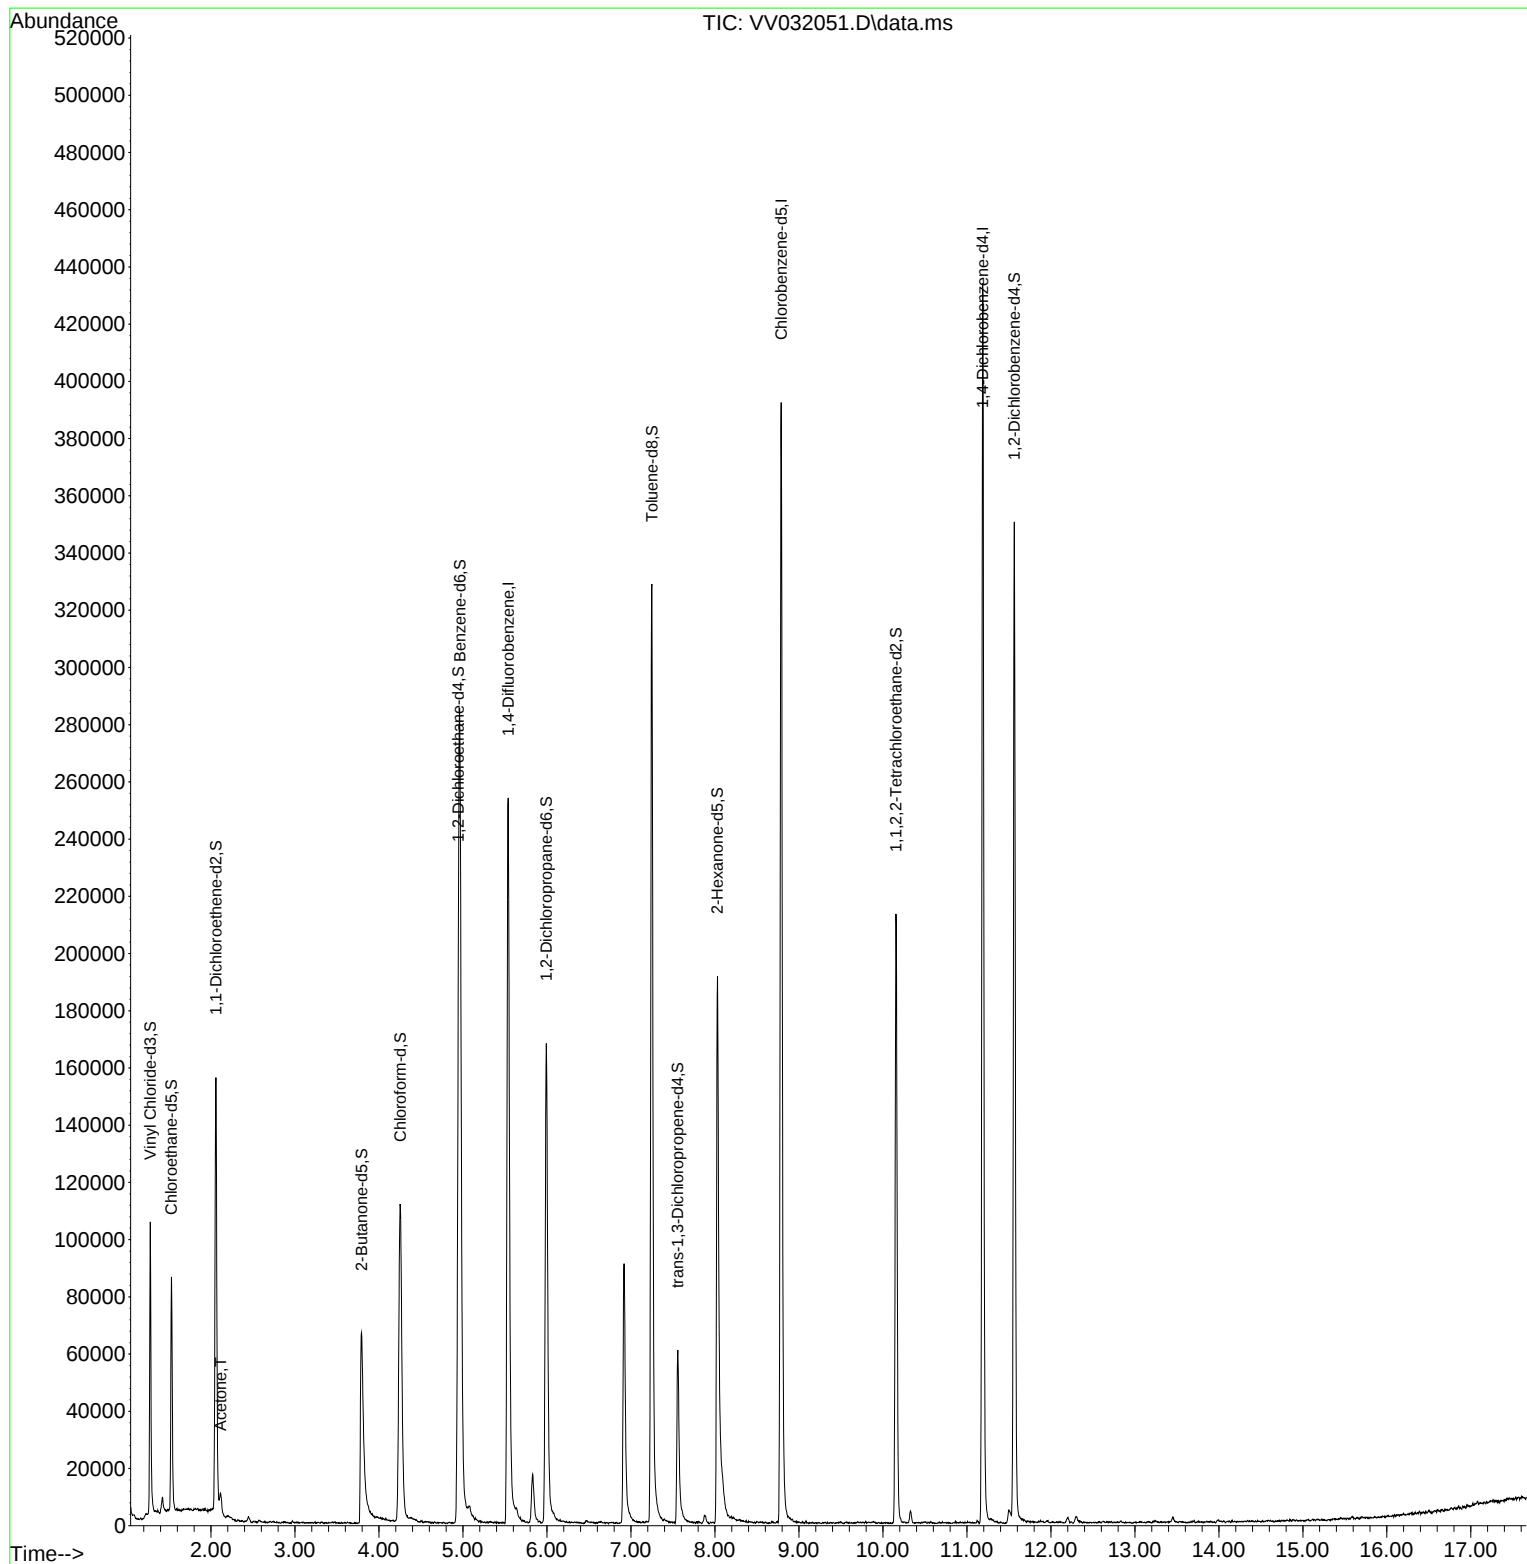

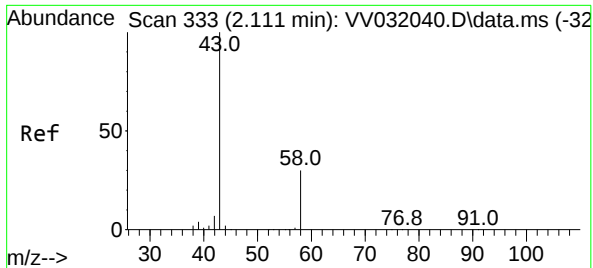

#13
 Acetone
 Concen: 4.802 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV032051.D
 Acq: 12 Sep 2023 16:15

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL1

Tgt Ion: 43 Resp: 4603
 Ion Ratio Lower Upper
 43 100
 58 35.3 0.0 61.0

