

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032054.D
 Acq On : 12 Sep 2023 17:26
 Operator : SY/MD
 Sample : 04386-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAM0

Quant Time: Sep 13 06:57:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	227932	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	225293	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	113436	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	61574	43.165	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.320%
7) Chloroethane-d5	1.529	69	51747	41.382	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.760%
11) 1,1-Dichloroethene-d2	2.060	65	25274	37.838	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.680%
21) 2-Butanone-d5	3.790	46	119106	106.162	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.160%
24) Chloroform-d	4.253	84	118961	38.154	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.300%
26) 1,2-Dichloroethane-d4	4.947	65	78839	38.102	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.200%
32) Benzene-d6	4.963	84	246014	40.018	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.040%
36) 1,2-Dichloropropane-d6	5.995	67	84454	42.681	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.360%
41) Toluene-d8	7.246	98	217045	38.317	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.640%#
43) trans-1,3-Dichloroprop...	7.558	79	36649	35.735	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.460%
47) 2-Hexanone-d5	8.031	63	66908	110.324	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.320%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	107006	41.849	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.700%
66) 1,2-Dichlorobenzene-d4	11.564	152	82344	39.821	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.640%#
Target Compounds						
13) Acetone	2.114	43	5054	5.061	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032054.D
Acq On : 12 Sep 2023 17:26
Operator : SY/MD
Sample : 04386-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAM0

Quant Time: Sep 13 06:57:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

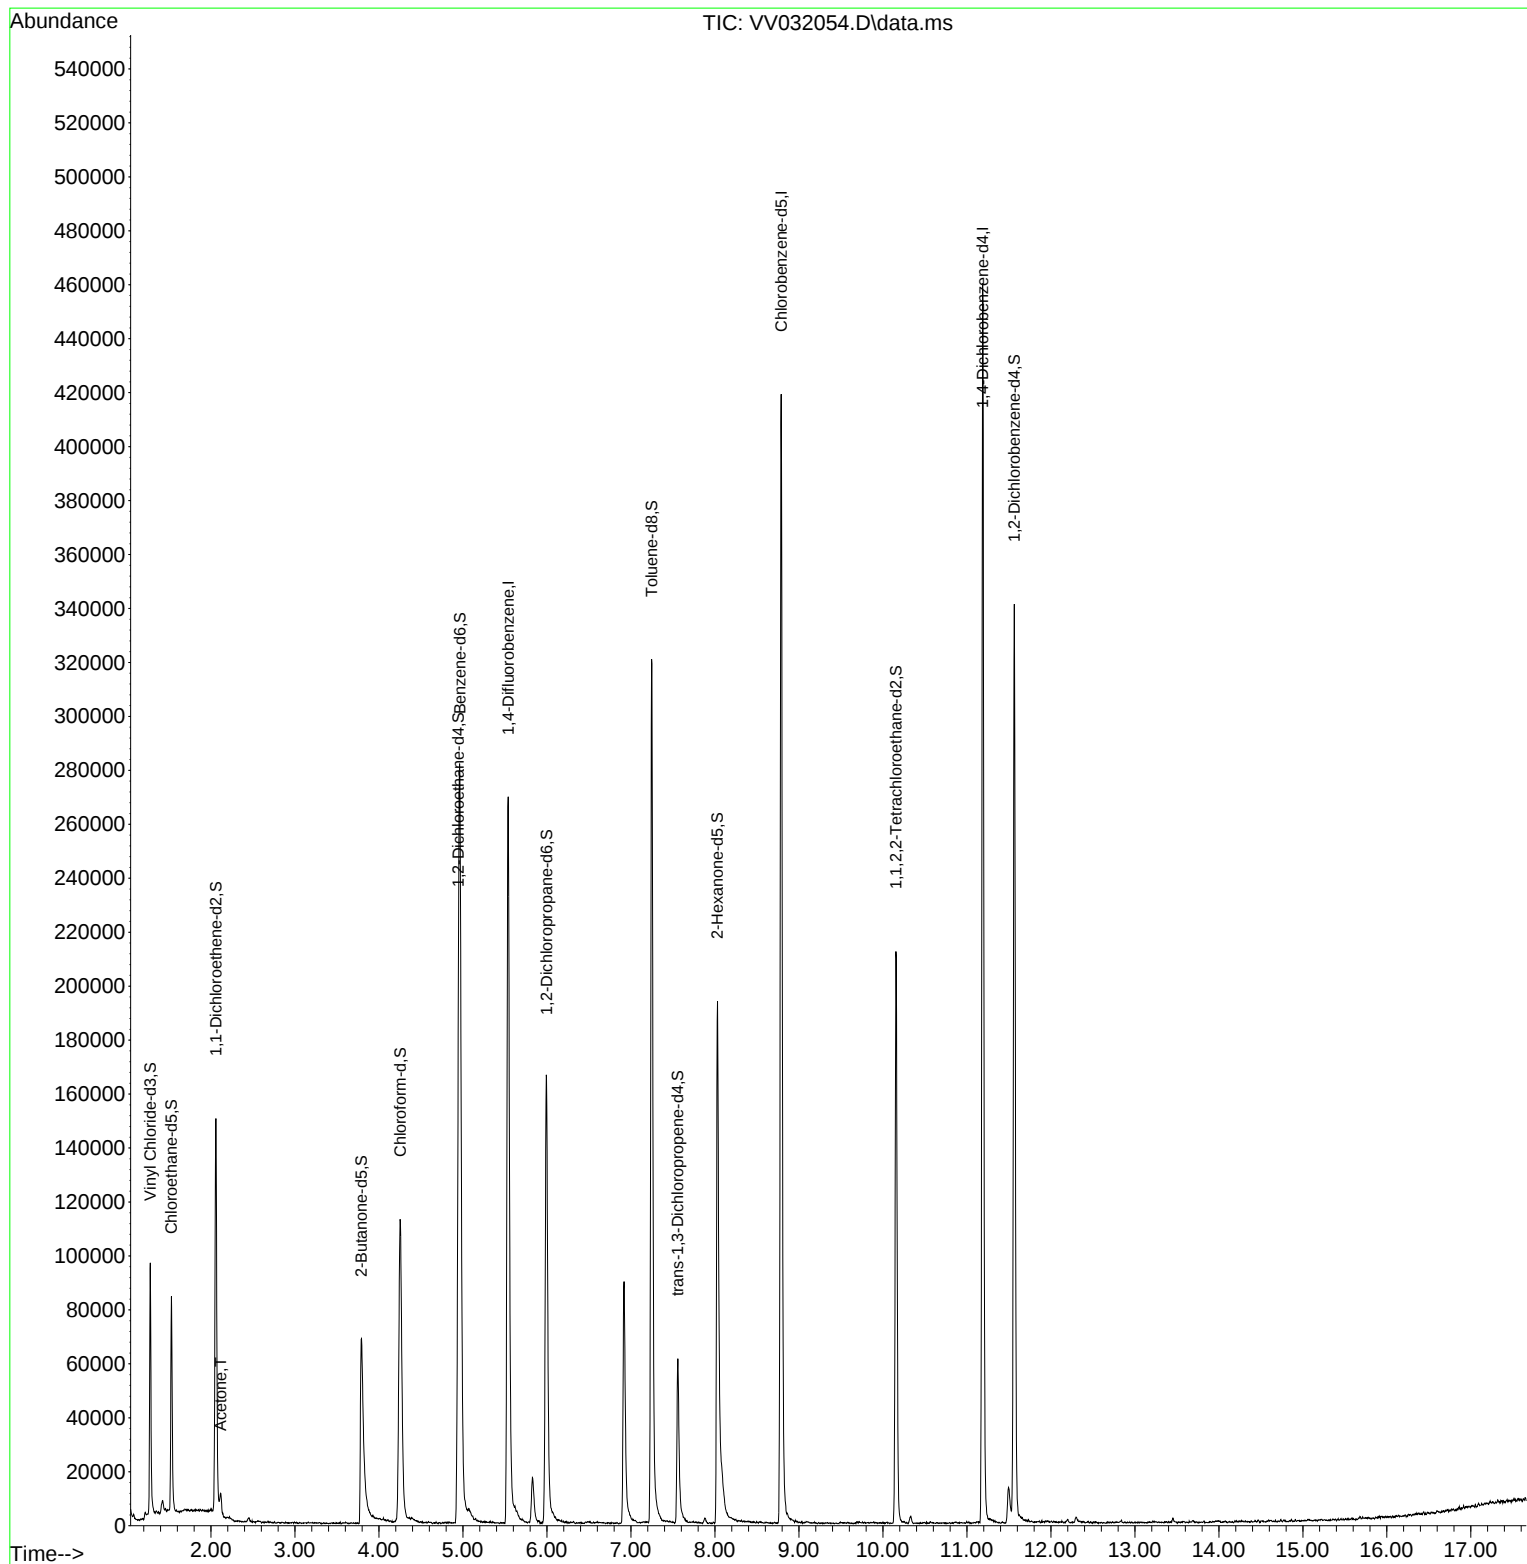

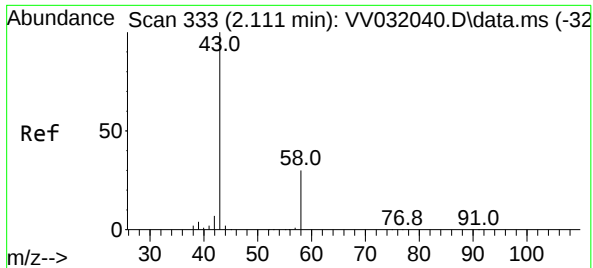

#13
 Acetone
 Concen: 5.061 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV032054.D
 Acq: 12 Sep 2023 17:26

Instrument :
 MSVOA_V
 ClientSampleId :
 COAM0

Tgt Ion: 43 Resp: 5054
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 61.0

