

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032055.D
 Acq On : 12 Sep 2023 17:49
 Operator : SY/MD
 Sample : 04386-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL2

Quant Time: Sep 13 06:57:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	240604	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	233560	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	115942	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	67244	44.657	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.320%
7) Chloroethane-d5	1.529	69	54255	41.102	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.200%
11) 1,1-Dichloroethene-d2	2.059	65	27440	38.917	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.840%
21) 2-Butanone-d5	3.793	46	119639	101.021	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.020%
24) Chloroform-d	4.252	84	123525	37.531	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.060%
26) 1,2-Dichloroethane-d4	4.947	65	82049	37.565	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.140%
32) Benzene-d6	4.963	84	257993	40.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.960%
36) 1,2-Dichloropropane-d6	5.992	67	89702	43.729	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.460%
41) Toluene-d8	7.246	98	225644	38.425	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.860%#
43) trans-1,3-Dichloroprop...	7.558	79	38739	36.436	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.880%
47) 2-Hexanone-d5	8.030	63	68397	108.788	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.790%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	109151	41.177	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.360%
66) 1,2-Dichlorobenzene-d4	11.564	152	85427	40.418	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.840%
Target Compounds						
13) Acetone	2.114	43	8033	7.621	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032055.D
Acq On : 12 Sep 2023 17:49
Operator : SY/MD
Sample : 04386-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL2

Quant Time: Sep 13 06:57:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

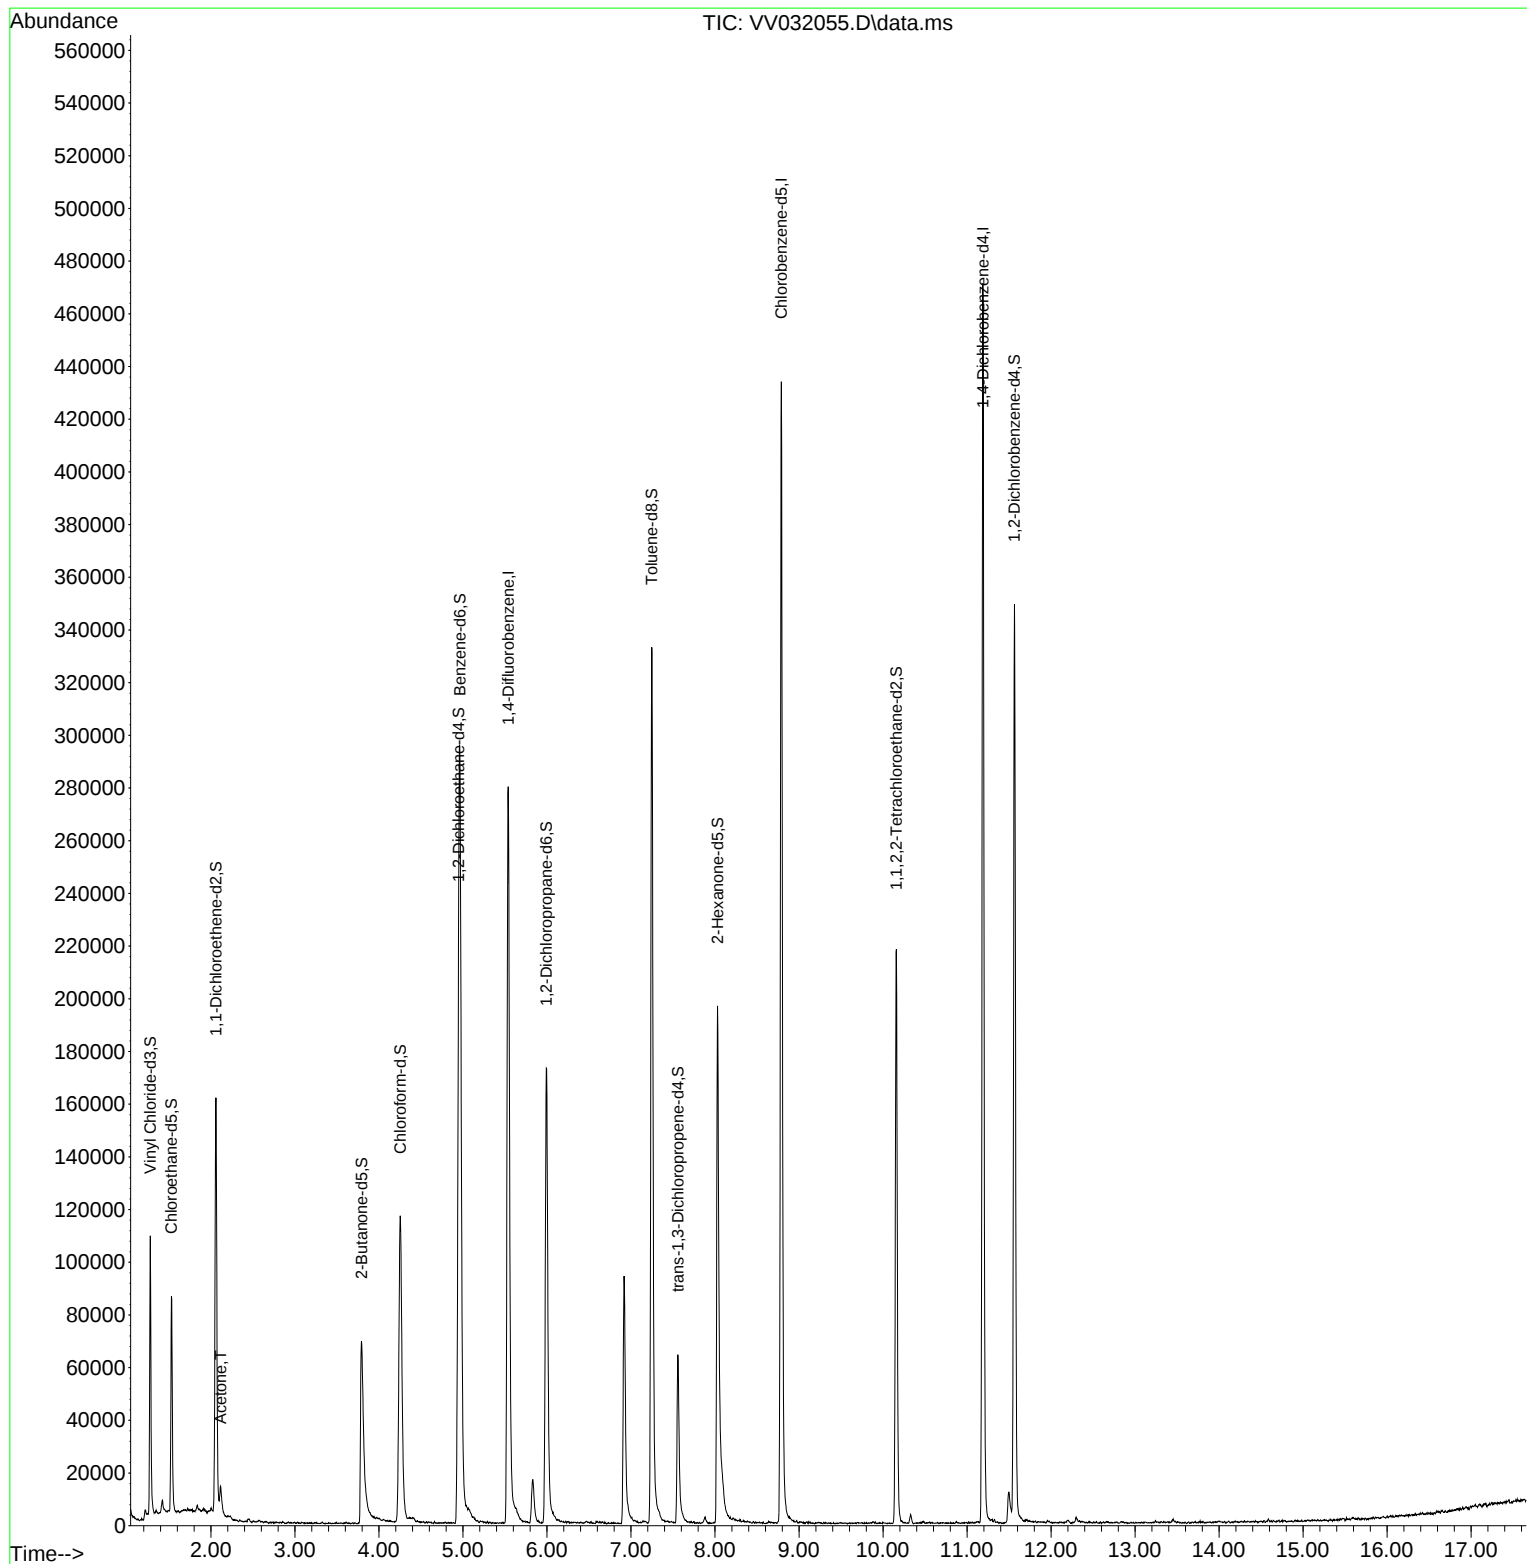

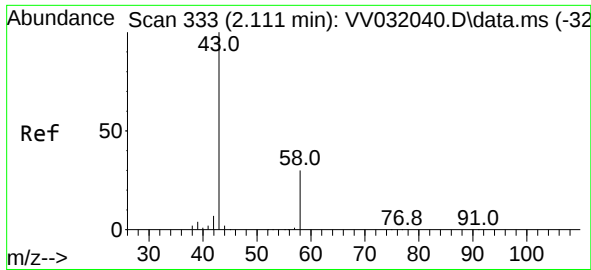

#13
 Acetone
 Concen: 7.621 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV032055.D
 Acq: 12 Sep 2023 17:49

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL2

Tgt Ion: 43 Resp: 8033
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 61.0

