

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032050.D
 Acq On : 12 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04385-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	98041	105543	13.20%	1.606%
2	1.529	146	152	168	rVB	83304	100261	12.54%	1.525%
3	2.060	308	317	328	rBV	156624	225427	28.20%	3.429%
4	2.642	496	498	500	rBV3	357	185	0.02%	0.003%
5	2.883	566	573	574	rBV4	475	477	0.06%	0.007%
6	3.011	610	613	616	rBV	301	219	0.03%	0.003%
7	3.066	625	630	632	rBV2	390	260	0.03%	0.004%
8	3.240	681	684	686	rVV	525	273	0.03%	0.004%
9	3.269	690	693	697	rBV2	494	493	0.06%	0.007%
10	3.500	764	765	769	rVB2	513	234	0.03%	0.004%
11	3.519	769	771	775	rBV2	375	221	0.03%	0.003%
12	3.545	775	779	783	rVV2	322	324	0.04%	0.005%
13	3.561	783	784	787	rVB	368	189	0.02%	0.003%
14	3.719	829	833	837	rVB4	502	364	0.05%	0.006%
15	3.790	847	855	889	rBV	73210	200657	25.10%	3.052%
16	4.253	986	999	1029	rVB	118116	301716	37.75%	4.590%
17	4.600	1105	1107	1110	rBV3	492	322	0.04%	0.005%
18	4.667	1126	1128	1130	rBV	341	182	0.02%	0.003%
19	4.738	1147	1150	1153	rBV2	367	253	0.03%	0.004%
20	4.773	1159	1161	1166	rBV4	299	228	0.03%	0.003%
21	4.828	1173	1178	1179	rBV2	368	275	0.03%	0.004%
22	4.960	1198	1219	1246	rBV2	301497	799315	100.00%	12.159%
23	5.320	1330	1331	1333	rBV	534	162	0.02%	0.002%
24	5.397	1353	1355	1357	rBV2	541	226	0.03%	0.003%
25	5.426	1362	1364	1367	rBV	334	185	0.02%	0.003%
26	5.452	1371	1372	1374	rBV2	552	273	0.03%	0.004%
27	5.494	1382	1385	1387	rBV	493	294	0.04%	0.004%
28	5.539	1387	1399	1423	rBV	284150	588453	73.62%	8.952%
29	5.828	1478	1489	1504	rBV3	17182	38016	4.76%	0.578%
30	5.992	1527	1540	1563	rBV	179363	379336	47.46%	5.771%
31	6.240	1614	1617	1618	rBV2	628	328	0.04%	0.005%
32	6.339	1644	1648	1649	rBV2	522	308	0.04%	0.005%
33	6.400	1661	1667	1672	rVB4	620	569	0.07%	0.009%
34	6.429	1672	1676	1678	rBV3	458	366	0.05%	0.006%
35	6.526	1703	1706	1707	rBV	373	204	0.03%	0.003%
36	6.558	1714	1716	1721	rBV3	369	382	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032050.D
 Acq On : 12 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04385-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.683	1751	1755	1756	rBV	512	362	0.05%	0.006%
38	6.748	1773	1775	1778	rVB4	531	241	0.03%	0.004%
39	6.767	1778	1781	1783	rBV3	515	281	0.04%	0.004%
40	6.812	1788	1795	1797	rBV3	325	336	0.04%	0.005%
41	6.841	1802	1804	1808	rVB2	311	224	0.03%	0.003%
42	6.918	1814	1828	1853	rBV2	95591	188071	23.53%	2.861%
43	7.246	1919	1930	1963	rBV	348353	634651	79.40%	9.654%
44	7.558	2018	2027	2048	rVV	65267	121269	15.17%	1.845%
45	7.783	2094	2097	2101	rVB3	420	273	0.03%	0.004%
46	7.841	2111	2115	2120	rVB2	498	324	0.04%	0.005%
47	7.886	2120	2129	2139	rBV3	2667	5218	0.65%	0.079%
48	7.953	2146	2150	2154	rBV4	453	391	0.05%	0.006%
49	7.979	2154	2158	2164	rBV5	406	512	0.06%	0.008%
50	8.031	2164	2174	2215	rBV	207364	425051	53.18%	6.466%
51	8.468	2309	2310	2313	rBV2	356	249	0.03%	0.004%
52	8.574	2341	2343	2346	rVV	367	172	0.02%	0.003%
53	8.789	2399	2410	2434	rBV	436844	731446	91.51%	11.127%
54	9.159	2522	2525	2527	rVV	372	220	0.03%	0.003%
55	9.185	2530	2533	2539	rVB5	560	481	0.06%	0.007%
56	9.284	2561	2564	2565	rBV2	315	194	0.02%	0.003%
57	9.410	2600	2603	2605	rVB	523	197	0.02%	0.003%
58	9.423	2605	2607	2608	rBV	311	160	0.02%	0.002%
59	9.474	2619	2623	2624	rBV2	394	249	0.03%	0.004%
60	9.590	2653	2659	2663	rBV4	525	542	0.07%	0.008%
61	9.635	2672	2673	2675	rBV4	462	162	0.02%	0.002%
62	9.699	2689	2693	2696	rBV4	337	297	0.04%	0.005%
63	9.760	2706	2712	2713	rBV3	417	427	0.05%	0.006%
64	9.911	2757	2759	2762	rBV2	361	191	0.02%	0.003%
65	9.931	2763	2765	2769	rVV2	410	222	0.03%	0.003%
66	9.985	2779	2782	2785	rVB3	671	360	0.05%	0.005%
67	10.021	2789	2793	2796	rBV3	448	299	0.04%	0.005%
68	10.040	2796	2799	2801	rBV2	322	194	0.02%	0.003%
69	10.156	2821	2835	2855	rBV	228805	363472	45.47%	5.529%
70	10.329	2882	2889	2901	rBV2	4697	7377	0.92%	0.112%
71	10.455	2924	2928	2929	rBV2	335	239	0.03%	0.004%
72	10.484	2934	2937	2945	rVB5	960	853	0.11%	0.013%
73	10.519	2945	2948	2949	rBV5	372	177	0.02%	0.003%
74	10.548	2953	2957	2959	rBV3	414	365	0.05%	0.006%
75	10.587	2968	2969	2972	rVB	508	177	0.02%	0.003%
76	10.612	2972	2977	2978	rBV2	287	224	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032050.D
 Acq On : 12 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04385-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.725	3010	3012	3015	rBV2	373	181	0.02%	0.003%
78	10.899	3060	3066	3070	rBV6	1231	1685	0.21%	0.026%
79	10.966	3086	3087	3092	rVB4	629	400	0.05%	0.006%
80	11.027	3104	3106	3109	rVB4	503	291	0.04%	0.004%
81	11.072	3116	3120	3122	rBV2	474	462	0.06%	0.007%
82	11.188	3145	3156	3177	rBV	489629	754763	94.43%	11.482%
83	11.358	3207	3209	3212	rVB2	642	298	0.04%	0.005%
84	11.426	3228	3230	3233	rBV3	287	185	0.02%	0.003%
85	11.503	3248	3254	3256	rBV4	3694	4086	0.51%	0.062%
86	11.564	3263	3273	3295	rVB	364990	574813	71.91%	8.744%
87	11.985	3401	3404	3405	rBV	656	406	0.05%	0.006%
88	12.111	3441	3443	3444	rBV3	479	174	0.02%	0.003%
89	12.429	3539	3542	3545	rBV3	522	403	0.05%	0.006%
90	12.583	3587	3590	3592	rBV2	440	258	0.03%	0.004%
91	12.763	3644	3646	3648	rBV	474	226	0.03%	0.003%
92	12.825	3663	3665	3666	rBV	533	284	0.04%	0.004%
93	12.882	3681	3683	3684	rBV	463	214	0.03%	0.003%
94	12.960	3704	3707	3708	rBV	409	182	0.02%	0.003%
95	13.107	3750	3753	3754	rBV	404	183	0.02%	0.003%
96	13.188	3774	3778	3781	rBV4	596	572	0.07%	0.009%
97	13.336	3822	3824	3828	rBV3	341	192	0.02%	0.003%
98	13.567	3894	3896	3897	rBV	452	194	0.02%	0.003%
99	13.805	3968	3970	3972	rBV2	584	276	0.03%	0.004%
100	14.345	4136	4138	4141	rBV2	606	291	0.04%	0.004%




Sum of corrected areas: 6573689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032050.D
Acq On : 12 Sep 2023 15:52
Operator : SY/MD
Sample : 04385-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

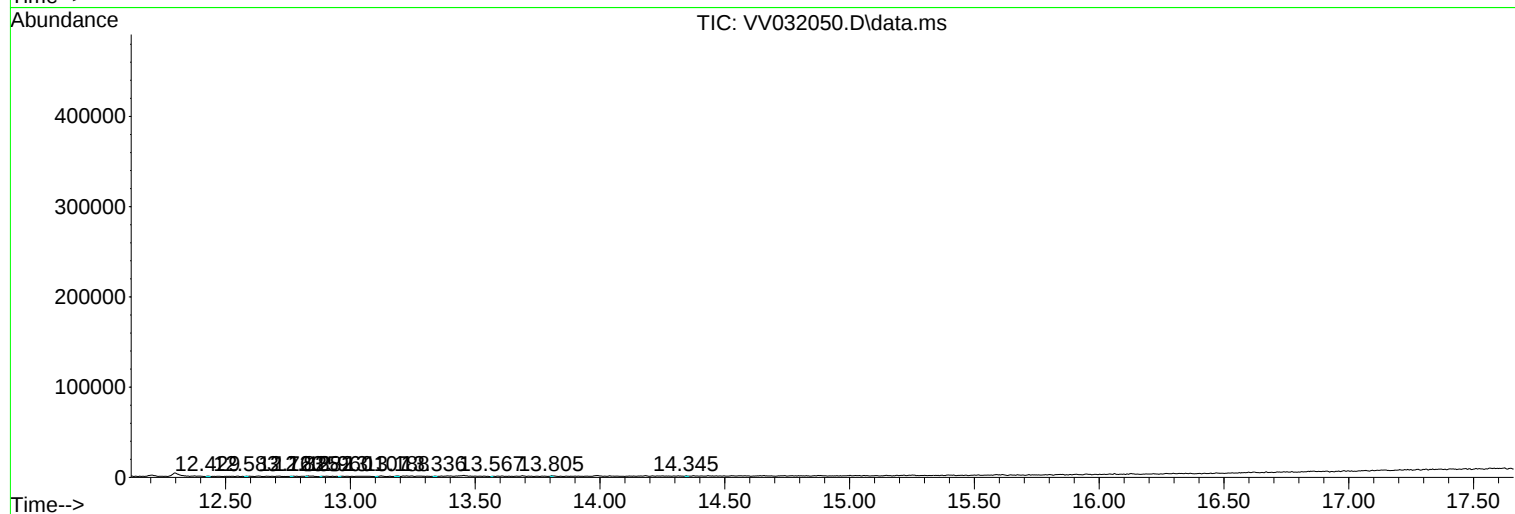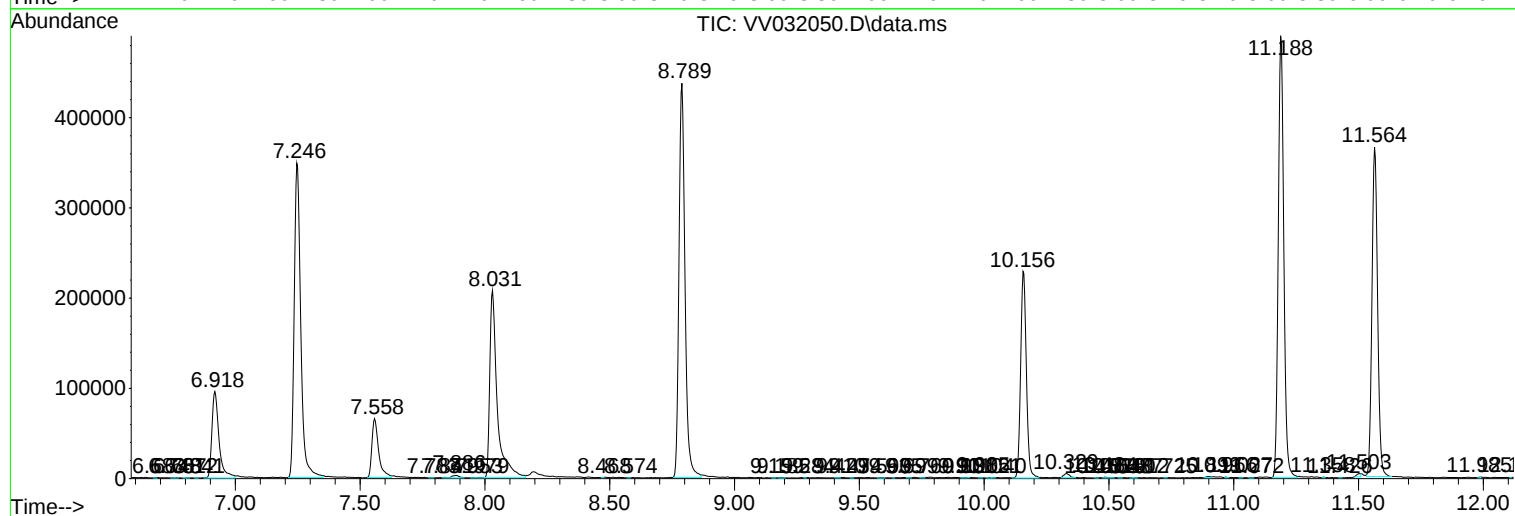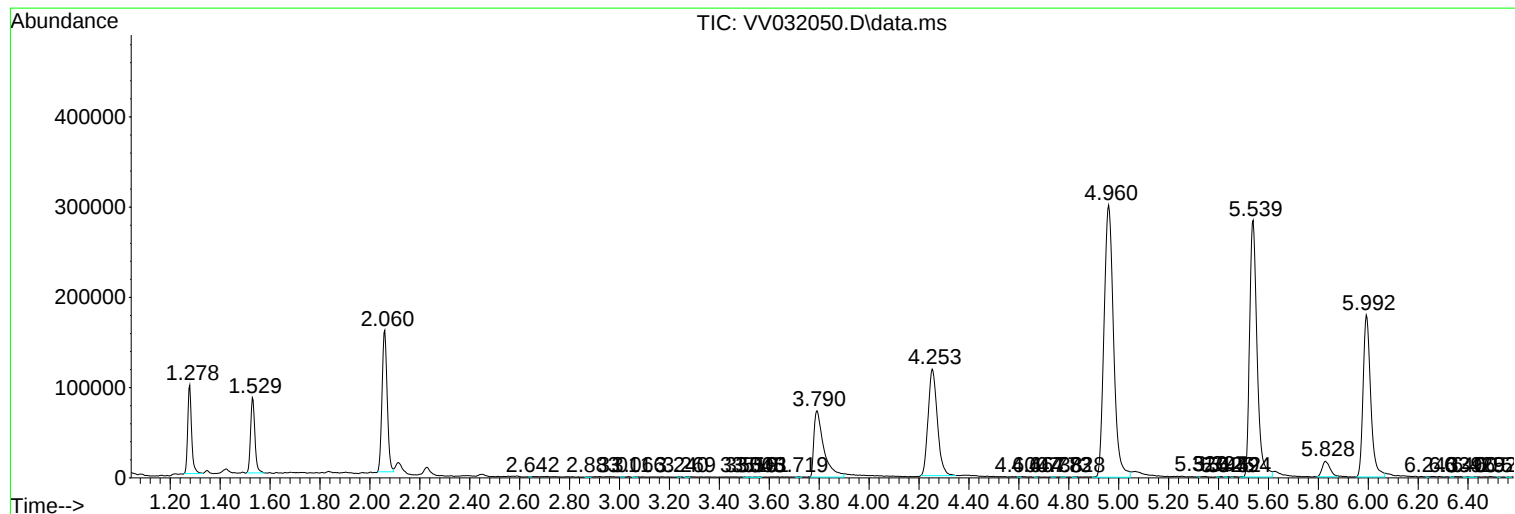

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032050.D
Acq On : 12 Sep 2023 15:52
Operator : SY/MD
Sample : 04385-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032050.D
Acq On : 12 Sep 2023 15:52
Operator : SY/MD
Sample : 04385-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc