

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032058.D
 Acq On : 12 Sep 2023 19:00
 Operator : SY/MD
 Sample : 04330-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	99823	105286	13.20%	1.631%
2	1.529	146	152	164	rBV	82007	96264	12.07%	1.492%
3	2.060	309	317	336	rVB	155156	224809	28.18%	3.484%
4	2.552	467	470	473	rBV4	738	591	0.07%	0.009%
5	2.587	479	481	483	rBV3	316	178	0.02%	0.003%
6	2.622	488	492	494	rBV3	467	329	0.04%	0.005%
7	2.687	508	512	514	rBV2	451	380	0.05%	0.006%
8	2.857	561	565	568	rBV4	383	348	0.04%	0.005%
9	3.011	610	613	617	rVB2	486	320	0.04%	0.005%
10	3.060	625	628	631	rBV2	511	363	0.05%	0.006%
11	3.166	659	661	665	rBV3	570	391	0.05%	0.006%
12	3.220	674	678	681	rBV2	444	340	0.04%	0.005%
13	3.253	684	688	690	rBV3	434	345	0.04%	0.005%
14	3.288	697	699	701	rVB	492	193	0.02%	0.003%
15	3.301	701	703	706	rBV2	407	279	0.03%	0.004%
16	3.471	752	756	757	rBV	449	237	0.03%	0.004%
17	3.574	784	788	791	rBV2	259	264	0.03%	0.004%
18	3.616	796	801	803	rBV	386	270	0.03%	0.004%
19	3.648	808	811	814	rBV2	431	254	0.03%	0.004%
20	3.793	847	856	887	rBV	69620	194931	24.44%	3.021%
21	4.253	983	999	1022	rBV	117349	305260	38.27%	4.730%
22	4.597	1104	1106	1109	rVB3	495	241	0.03%	0.004%
23	4.613	1109	1111	1113	rBV3	455	180	0.02%	0.003%
24	4.671	1126	1129	1134	rVB2	690	494	0.06%	0.008%
25	4.844	1180	1183	1186	rBV2	267	206	0.03%	0.003%
26	4.960	1203	1219	1245	rBV2	303946	797633	100.00%	12.360%
27	5.204	1293	1295	1301	rVB2	713	425	0.05%	0.007%
28	5.285	1316	1320	1323	rVB3	578	474	0.06%	0.007%
29	5.413	1357	1360	1364	rBV3	539	368	0.05%	0.006%
30	5.436	1364	1367	1369	rVB	485	343	0.04%	0.005%
31	5.539	1387	1399	1422	rBV	273227	568593	71.29%	8.811%
32	5.834	1477	1491	1507	rBV3	11144	25645	3.22%	0.397%
33	5.992	1527	1540	1561	rBV	176389	373198	46.79%	5.783%
34	6.217	1608	1610	1613	rBV2	747	436	0.05%	0.007%
35	6.281	1626	1630	1631	rBV2	262	218	0.03%	0.003%
36	6.323	1641	1643	1650	rBV5	633	776	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032058.D
 Acq On : 12 Sep 2023 19:00
 Operator : SY/MD
 Sample : 04330-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.368	1655	1657	1662	rVV4	738	600	0.08%	0.009%
38	6.468	1686	1688	1692	rVV2	287	257	0.03%	0.004%
39	6.487	1692	1694	1696	rVV2	309	181	0.02%	0.003%
40	6.513	1700	1702	1706	rVV2	499	297	0.04%	0.005%
41	6.532	1706	1708	1711	rVV2	428	257	0.03%	0.004%
42	6.561	1714	1717	1720	rBV2	381	265	0.03%	0.004%
43	6.638	1739	1741	1744	rVB2	519	224	0.03%	0.003%
44	6.683	1752	1755	1757	rVB2	455	266	0.03%	0.004%
45	6.748	1766	1775	1777	rBV2	629	658	0.08%	0.010%
46	6.805	1789	1793	1796	rVB2	297	265	0.03%	0.004%
47	6.867	1810	1812	1816	rBV2	418	275	0.03%	0.004%
48	6.918	1817	1828	1853	rBV	93470	184311	23.11%	2.856%
49	7.246	1918	1930	1967	rBV	345622	631976	79.23%	9.793%
50	7.558	2017	2027	2049	rBV	64237	119052	14.93%	1.845%
51	7.854	2116	2119	2122	rBV2	378	272	0.03%	0.004%
52	7.876	2122	2126	2128	rVV2	492	405	0.05%	0.006%
53	7.921	2138	2140	2143	rVB3	467	292	0.04%	0.005%
54	7.979	2155	2158	2163	rBV3	325	302	0.04%	0.005%
55	8.030	2163	2174	2211	rBV	201813	409693	51.36%	6.348%
56	8.728	2389	2391	2398	rBV2	360	339	0.04%	0.005%
57	8.789	2398	2410	2443	rBV	428559	713983	89.51%	11.064%
58	9.014	2475	2480	2482	rBV2	357	329	0.04%	0.005%
59	9.069	2492	2497	2499	rBV3	640	559	0.07%	0.009%
60	9.098	2504	2506	2510	rVB2	321	182	0.02%	0.003%
61	9.278	2559	2562	2564	rBV2	466	294	0.04%	0.005%
62	9.374	2587	2592	2595	rBV3	361	301	0.04%	0.005%
63	9.420	2603	2606	2610	rBV3	495	413	0.05%	0.006%
64	9.500	2629	2631	2635	rBV2	353	187	0.02%	0.003%
65	9.519	2635	2637	2641	rVV2	442	273	0.03%	0.004%
66	9.629	2668	2671	2676	rBV3	289	247	0.03%	0.004%
67	9.731	2701	2703	2707	rVB2	486	270	0.03%	0.004%
68	9.754	2707	2710	2712	rBV2	333	223	0.03%	0.003%
69	9.773	2712	2716	2717	rVV	340	190	0.02%	0.003%
70	9.821	2727	2731	2733	rBV	320	188	0.02%	0.003%
71	9.944	2766	2769	2771	rBV	450	192	0.02%	0.003%
72	10.018	2788	2792	2795	rBV3	408	326	0.04%	0.005%
73	10.101	2814	2818	2822	rVB3	560	421	0.05%	0.007%
74	10.156	2822	2835	2861	rBV	236002	378997	47.52%	5.873%
75	10.519	2946	2948	2952	rVB	373	249	0.03%	0.004%
76	10.583	2963	2968	2972	rBV3	358	356	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032058.D
 Acq On : 12 Sep 2023 19:00
 Operator : SY/MD
 Sample : 04330-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.616	2975	2978	2982	rBV2	433	290	0.04%	0.004%
78	10.796	3030	3034	3037	rVB2	482	342	0.04%	0.005%
79	10.863	3051	3055	3056	rBV3	488	265	0.03%	0.004%
80	11.143	3139	3142	3145	rBV3	559	362	0.05%	0.006%
81	11.188	3145	3156	3174	rBV	467882	724582	90.84%	11.228%
82	11.484	3245	3248	3251	rBV2	265	190	0.02%	0.003%
83	11.564	3262	3273	3295	rBV	366541	572121	71.73%	8.865%
84	11.860	3362	3365	3367	rBV2	323	239	0.03%	0.004%
85	12.271	3490	3493	3495	rVB2	457	206	0.03%	0.003%
86	12.374	3521	3525	3527	rBV2	480	354	0.04%	0.005%
87	12.426	3537	3541	3545	rBV3	316	307	0.04%	0.005%
88	12.516	3567	3569	3571	rBV2	402	217	0.03%	0.003%
89	12.677	3618	3619	3622	rBV	290	186	0.02%	0.003%
90	12.828	3663	3666	3667	rBV	515	308	0.04%	0.005%
91	13.201	3779	3782	3787	rVB3	491	311	0.04%	0.005%
92	13.243	3792	3795	3796	rBV	676	371	0.05%	0.006%
93	13.551	3888	3891	3895	rBV2	521	367	0.05%	0.006%
94	13.612	3907	3910	3914	rBV3	567	363	0.05%	0.006%
95	13.683	3928	3932	3934	rBV2	487	373	0.05%	0.006%
96	13.995	4023	4029	4034	rBV4	1061	1096	0.14%	0.017%
97	14.069	4049	4052	4054	rBV2	491	335	0.04%	0.005%
98	14.111	4063	4065	4069	rBV2	460	305	0.04%	0.005%
99	14.130	4069	4071	4074	rBV2	417	290	0.04%	0.004%
100	14.400	4152	4155	4157	rBV2	620	431	0.05%	0.007%




Sum of corrected areas: 6453440

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032058.D
Acq On : 12 Sep 2023 19:00
Operator : SY/MD
Sample : 04330-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

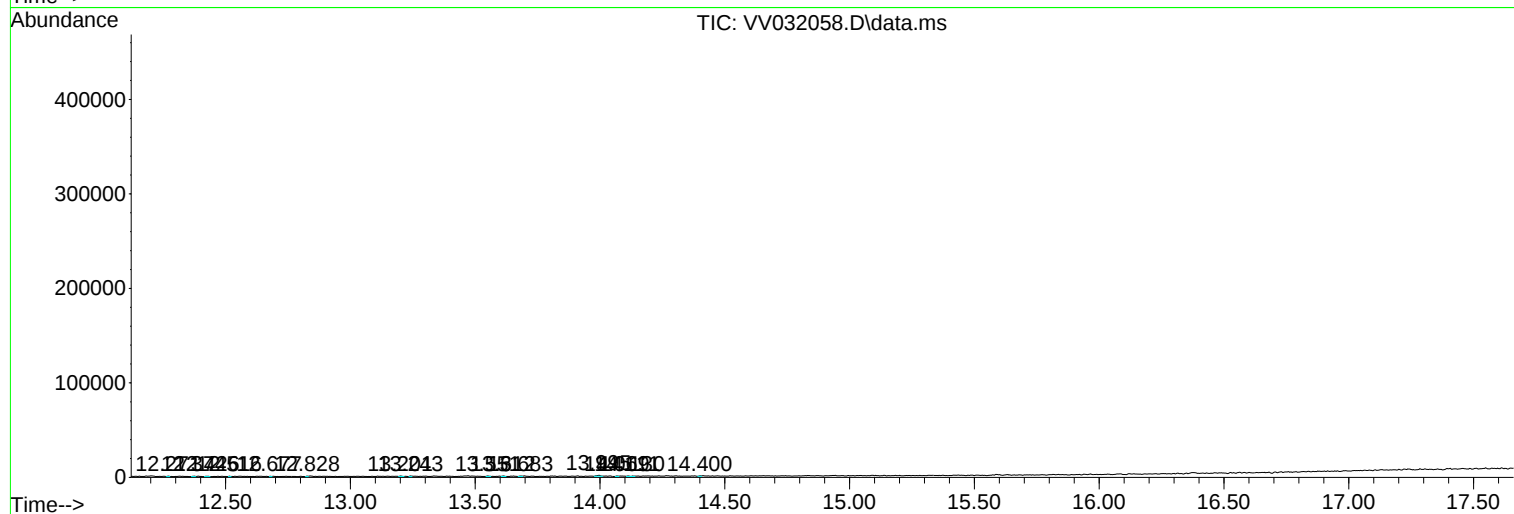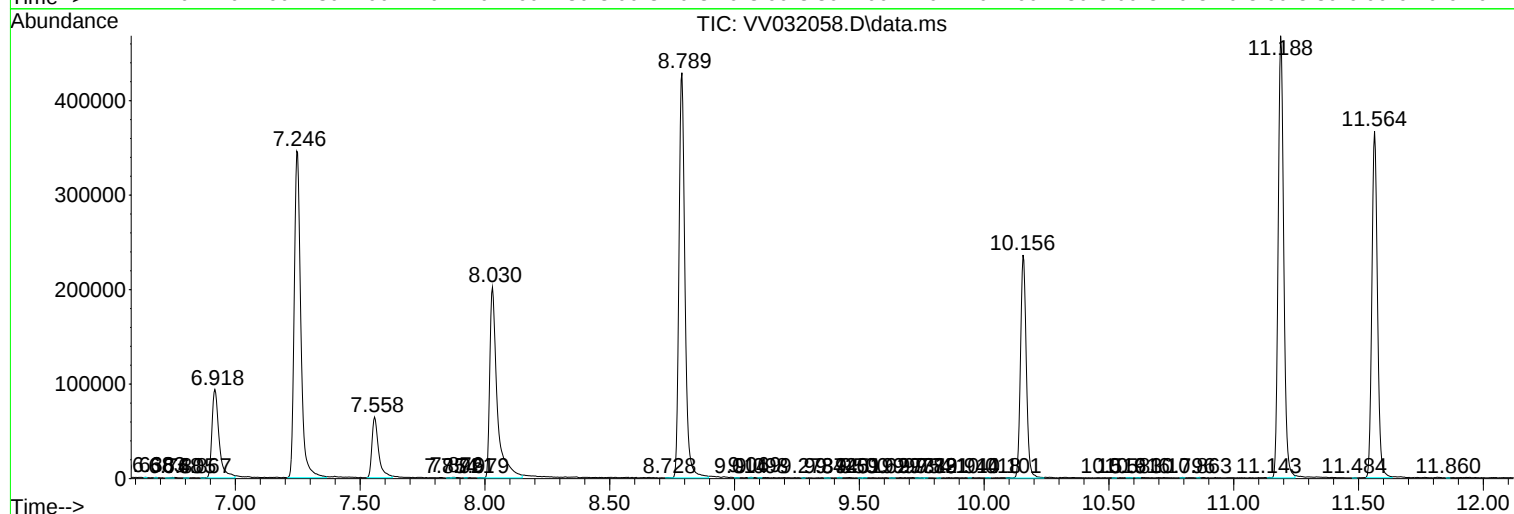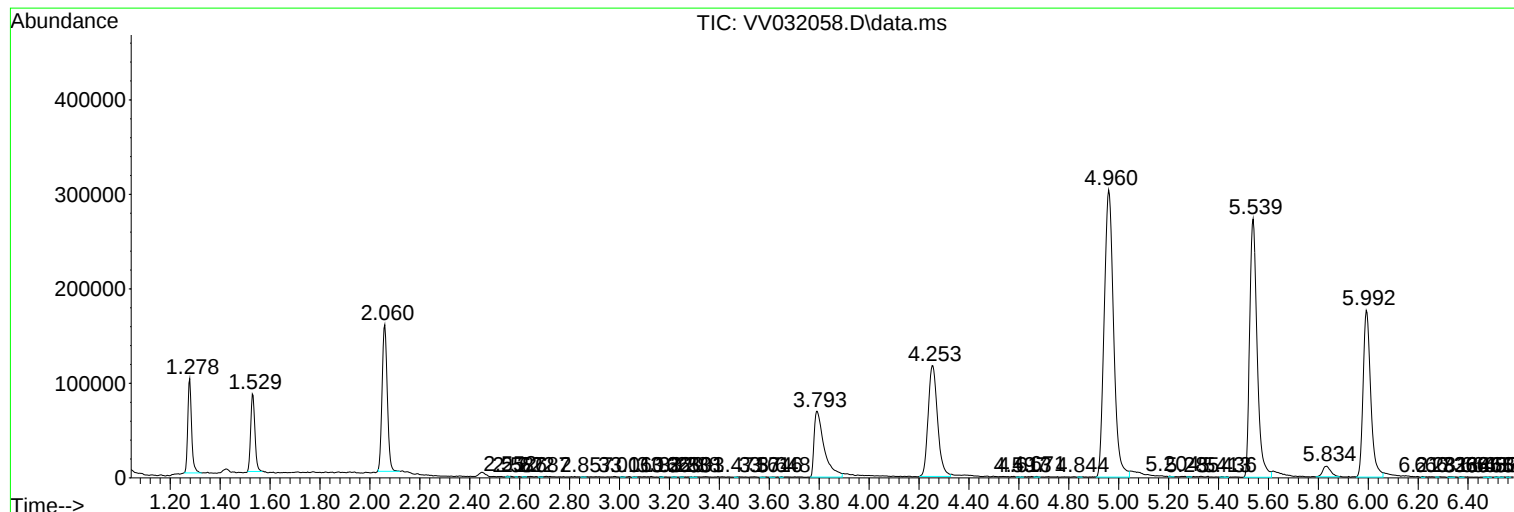

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032058.D
Acq On : 12 Sep 2023 19:00
Operator : SY/MD
Sample : 04330-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032058.D
Acq On : 12 Sep 2023 19:00
Operator : SY/MD
Sample : 04330-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------