

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032059.D
 Acq On : 12 Sep 2023 19:24
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	94787	97381	12.82%	1.583%
2	1.529	146	152	169	rVB	78398	94245	12.41%	1.532%
3	2.060	308	317	333	rBV	145167	208284	27.42%	3.386%
4	2.909	578	581	584	rBV2	545	435	0.06%	0.007%
5	2.941	589	591	596	rBV3	453	280	0.04%	0.005%
6	2.970	596	600	605	rVB4	399	384	0.05%	0.006%
7	3.011	610	613	615	rBV2	550	349	0.05%	0.006%
8	3.085	633	636	639	rBV3	501	331	0.04%	0.005%
9	3.262	688	691	696	rVB3	375	300	0.04%	0.005%
10	3.484	757	760	763	rBV3	253	207	0.03%	0.003%
11	3.503	765	766	770	rVB2	592	253	0.03%	0.004%
12	3.526	770	773	776	rBV	306	244	0.03%	0.004%
13	3.732	834	837	843	rVB2	499	301	0.04%	0.005%
14	3.793	847	856	894	rBV	70247	200865	26.44%	3.266%
15	4.253	986	999	1027	rVB	111044	280694	36.95%	4.564%
16	4.564	1093	1096	1098	rBV2	479	317	0.04%	0.005%
17	4.677	1129	1131	1133	rVB3	484	212	0.03%	0.003%
18	4.793	1165	1167	1170	rVB2	566	283	0.04%	0.005%
19	4.828	1176	1178	1180	rVB2	462	186	0.02%	0.003%
20	4.960	1203	1219	1247	rBV2	287039	759729	100.00%	12.352%
21	5.365	1342	1345	1350	rVB2	582	396	0.05%	0.006%
22	5.388	1350	1352	1355	rBV2	419	198	0.03%	0.003%
23	5.416	1359	1361	1365	rVB	450	250	0.03%	0.004%
24	5.452	1369	1372	1375	rVB2	708	394	0.05%	0.006%
25	5.539	1385	1399	1424	rBV	258263	539948	71.07%	8.779%
26	5.831	1480	1490	1508	rBV2	11354	24500	3.22%	0.398%
27	5.937	1520	1523	1527	rBV3	438	406	0.05%	0.007%
28	5.992	1527	1540	1561	rBV	169605	358721	47.22%	5.832%
29	6.307	1635	1638	1641	rBV	495	339	0.04%	0.006%
30	6.339	1646	1648	1651	rBV	280	176	0.02%	0.003%
31	6.535	1703	1709	1711	rBV3	404	416	0.05%	0.007%
32	6.593	1724	1727	1729	rBV2	448	296	0.04%	0.005%
33	6.606	1729	1731	1737	rVB3	566	546	0.07%	0.009%
34	6.651	1743	1745	1748	rVV4	456	212	0.03%	0.003%
35	6.703	1757	1761	1763	rVB	525	268	0.04%	0.004%
36	6.719	1763	1766	1767	rBV2	433	262	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032059.D
 Acq On : 12 Sep 2023 19:24
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.767	1775	1781	1783	rBV2	649	444	0.06%	0.007%
38	6.863	1809	1811	1815	rVB	352	171	0.02%	0.003%
39	6.918	1815	1828	1865	rBV	89889	179183	23.59%	2.913%
40	7.246	1919	1930	1960	rBV	327590	592801	78.03%	9.638%
41	7.558	2017	2027	2054	rBV2	61583	116696	15.36%	1.897%
42	7.738	2081	2083	2085	rBV	527	228	0.03%	0.004%
43	7.793	2099	2100	2103	rBV2	352	207	0.03%	0.003%
44	7.815	2105	2107	2109	rVV	425	205	0.03%	0.003%
45	7.838	2112	2114	2121	rVV3	299	381	0.05%	0.006%
46	7.883	2125	2128	2130	rVV	666	408	0.05%	0.007%
47	7.966	2151	2154	2156	rBV3	319	212	0.03%	0.003%
48	7.992	2158	2162	2164	rBV2	454	304	0.04%	0.005%
49	8.031	2164	2174	2205	rBV	200982	395928	52.11%	6.437%
50	8.513	2322	2324	2327	rBV2	509	187	0.02%	0.003%
51	8.593	2346	2349	2353	rVB3	641	491	0.06%	0.008%
52	8.619	2353	2357	2360	rBV3	340	303	0.04%	0.005%
53	8.789	2397	2410	2440	rBV	400976	679928	89.50%	11.055%
54	9.069	2494	2497	2500	rBV3	368	328	0.04%	0.005%
55	9.127	2512	2515	2517	rBV3	377	174	0.02%	0.003%
56	9.143	2517	2520	2524	rVB2	421	352	0.05%	0.006%
57	9.166	2524	2527	2529	rBV	280	190	0.03%	0.003%
58	9.223	2543	2545	2548	rVV	306	199	0.03%	0.003%
59	9.310	2569	2572	2575	rVV2	252	184	0.02%	0.003%
60	9.339	2579	2581	2585	rBV	297	173	0.02%	0.003%
61	9.358	2585	2587	2590	rBV2	342	228	0.03%	0.004%
62	9.448	2612	2615	2618	rVB	398	216	0.03%	0.004%
63	9.574	2652	2654	2658	rVB2	408	205	0.03%	0.003%
64	9.632	2670	2672	2674	rBV	365	173	0.02%	0.003%
65	9.805	2723	2726	2729	rVB	335	216	0.03%	0.004%
66	9.834	2729	2735	2738	rBV2	543	359	0.05%	0.006%
67	9.931	2762	2765	2767	rBV	289	195	0.03%	0.003%
68	10.008	2786	2789	2790	rBV	361	205	0.03%	0.003%
69	10.156	2824	2835	2858	rBV	231120	366848	48.29%	5.964%
70	10.265	2867	2869	2874	rVB3	617	490	0.06%	0.008%
71	10.288	2874	2876	2878	rBV2	535	254	0.03%	0.004%
72	10.384	2904	2906	2909	rVB2	490	194	0.03%	0.003%
73	10.403	2909	2912	2915	rBV	377	209	0.03%	0.003%
74	10.487	2935	2938	2940	rVV2	376	265	0.03%	0.004%
75	10.526	2947	2950	2954	rBV2	336	285	0.04%	0.005%
76	10.545	2954	2956	2959	rVB3	370	187	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
 Data File : VV032059.D
 Acq On : 12 Sep 2023 19:24
 Operator : SY/MD
 Sample : 04385-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.564	2959	2962	2965	rBV2	279	207	0.03%	0.003%
78	10.651	2985	2989	2993	rVB2	614	403	0.05%	0.007%
79	10.674	2994	2996	2999	rVV2	261	181	0.02%	0.003%
80	10.699	3001	3004	3007	rVB2	329	219	0.03%	0.004%
81	10.757	3019	3022	3024	rBV2	383	232	0.03%	0.004%
82	10.799	3033	3035	3039	rVB	419	299	0.04%	0.005%
83	10.828	3039	3044	3045	rBV	348	284	0.04%	0.005%
84	10.892	3062	3064	3067	rVB	386	195	0.03%	0.003%
85	10.915	3067	3071	3075	rBV	448	363	0.05%	0.006%
86	10.960	3083	3085	3089	rVB4	335	186	0.02%	0.003%
87	10.982	3089	3092	3099	rBV3	323	377	0.05%	0.006%
88	11.066	3115	3118	3122	rBV2	291	221	0.03%	0.004%
89	11.188	3145	3156	3178	rBV	440020	685165	90.19%	11.140%
90	11.445	3234	3236	3240	rVB2	401	245	0.03%	0.004%
91	11.564	3261	3273	3295	rBV	344749	546536	71.94%	8.886%
92	11.741	3326	3328	3332	rBV2	398	251	0.03%	0.004%
93	11.760	3332	3334	3337	rVV2	371	208	0.03%	0.003%
94	11.972	3398	3400	3404	rVV2	389	239	0.03%	0.004%
95	12.021	3413	3415	3416	rBV	675	250	0.03%	0.004%
96	12.349	3514	3517	3520	rBV	293	212	0.03%	0.003%
97	13.368	3832	3834	3836	rVB2	553	232	0.03%	0.004%
98	13.448	3855	3859	3862	rBV2	662	573	0.08%	0.009%
99	13.976	4018	4023	4024	rBV2	876	602	0.08%	0.010%
100	14.062	4048	4050	4051	rBV	435	184	0.02%	0.003%




Sum of corrected areas: 6150678

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032059.D
Acq On : 12 Sep 2023 19:24
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

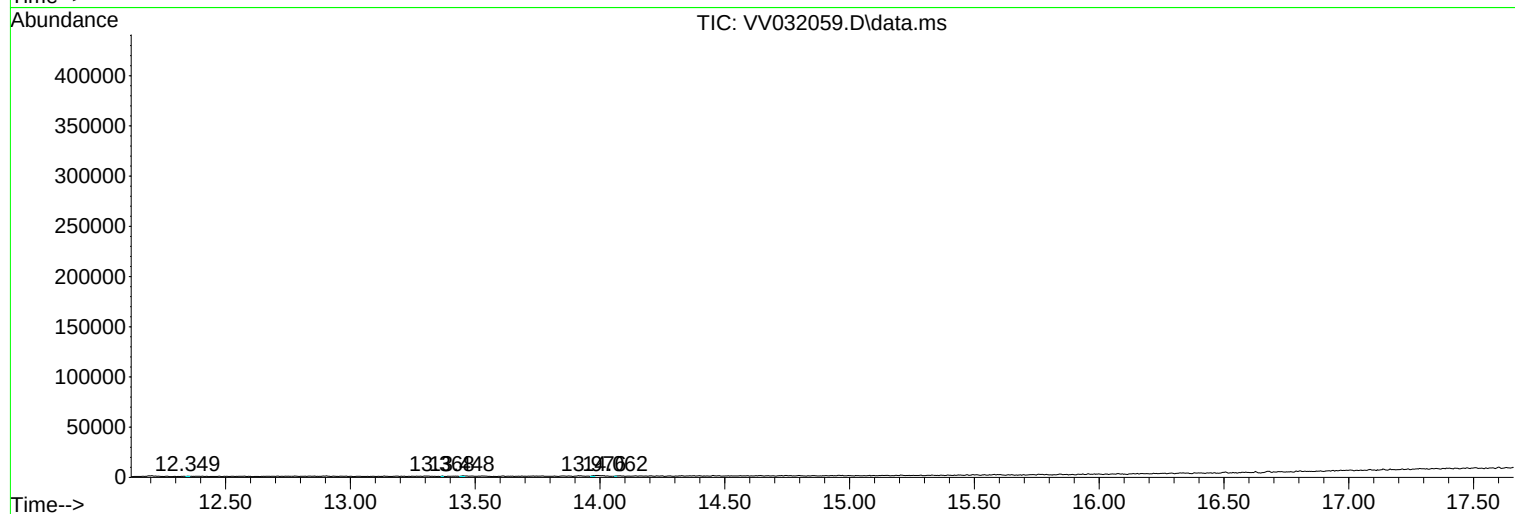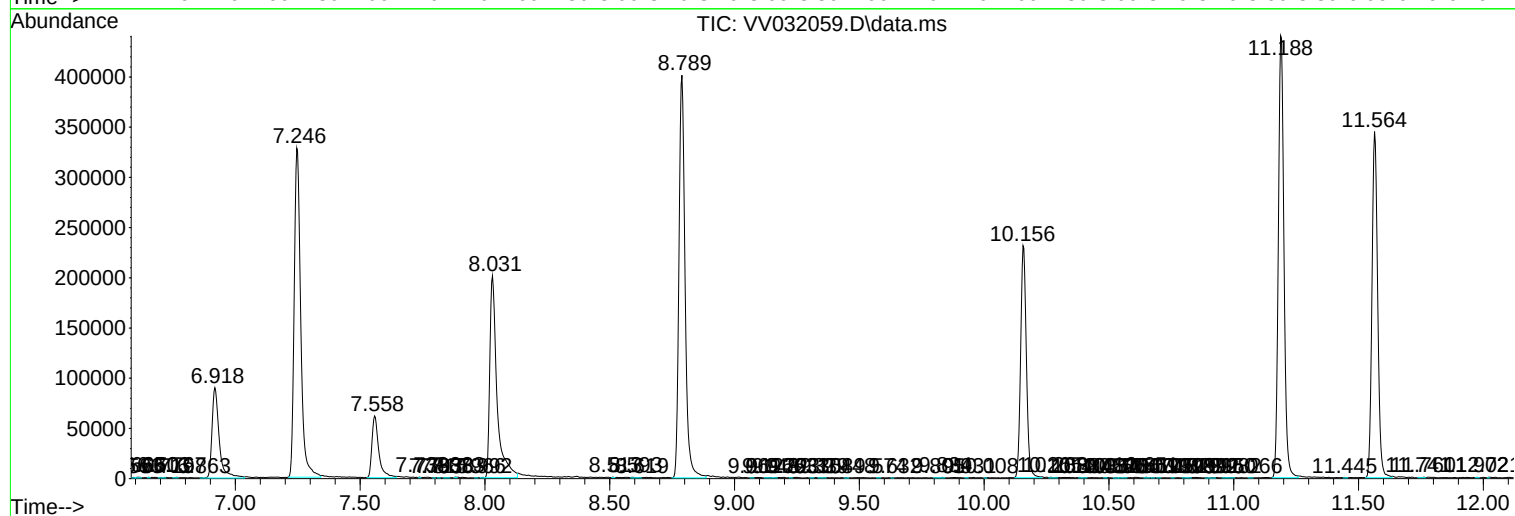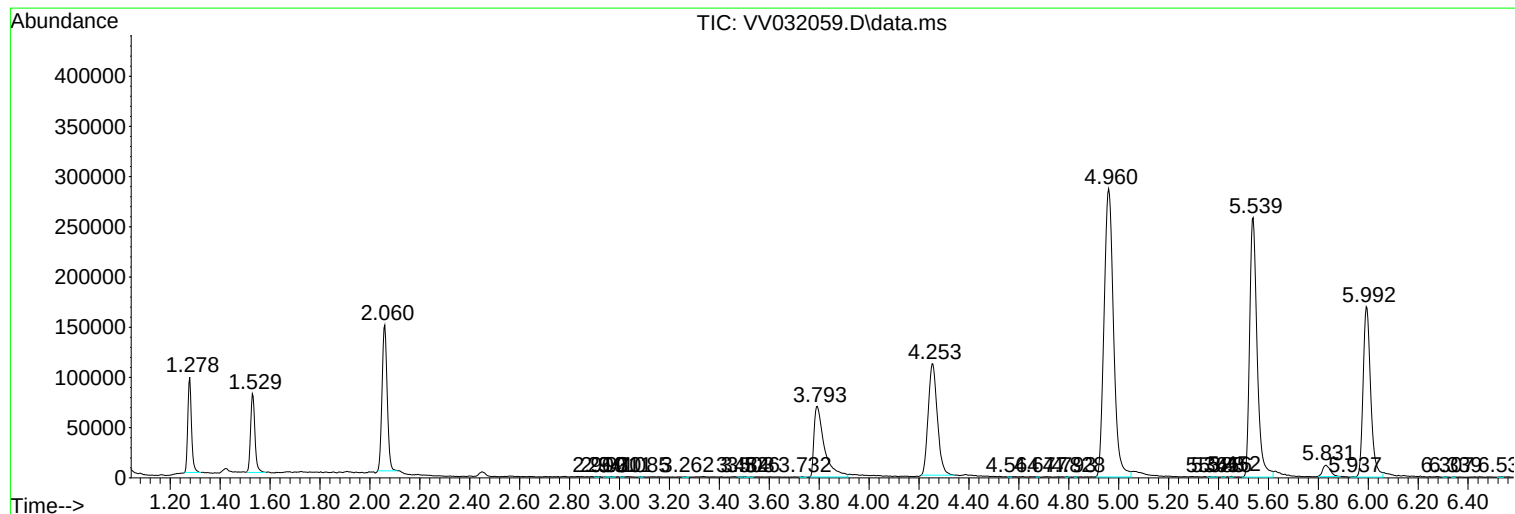

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032059.D
Acq On : 12 Sep 2023 19:24
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032059.D
Acq On : 12 Sep 2023 19:24
Operator : SY/MD
Sample : 04385-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------