


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091223\
Data File : VV032039.D
Acq On : 12 Sep 2023 10:49
Operator : SY/MD
Sample : BFB210
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB210

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Fri Sep 15 08:00:54 2023

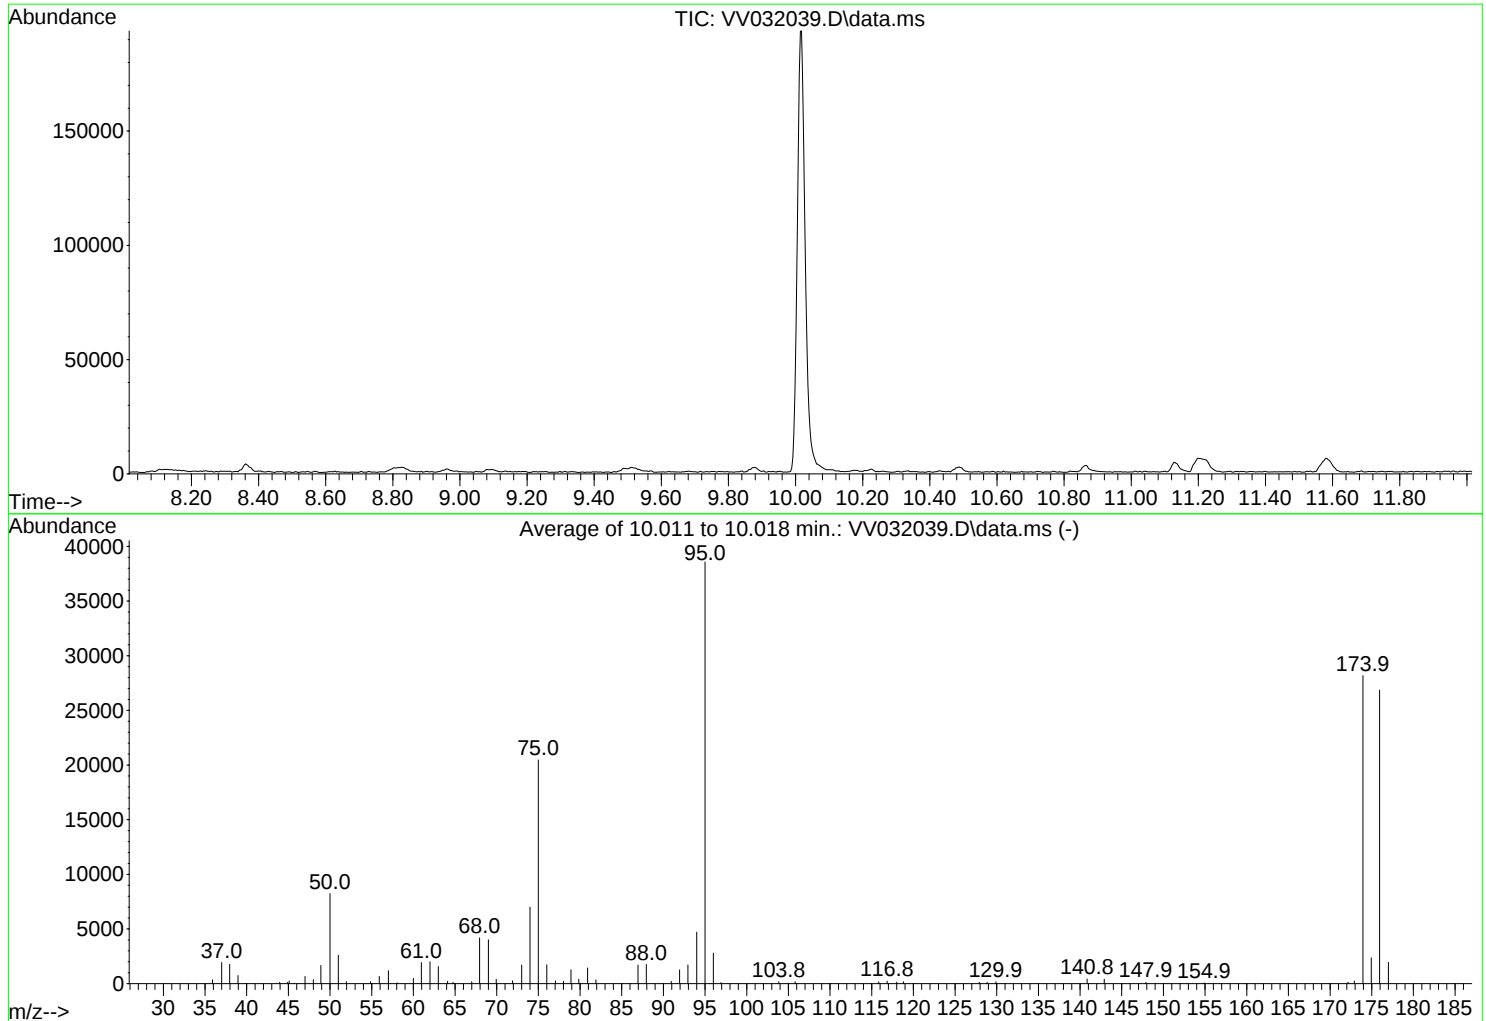

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	8242	PASS
75	95	30	80	53.0	20467	PASS
95	95	100	100	100.0	38589	PASS
96	95	5	9	7.3	2799	PASS
173	174	0.00	2	0.8	234	PASS
174	95	50	120	73.0	28173	PASS
175	174	5	9	8.4	2353	PASS
176	174	95	105	95.3	26861	PASS
177	176	5	10	7.2	1940	PASS

m/z	Abundance
36.00	110.0
39.90	184.0
44.00	626.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	451.0
37.00	1927.0
38.00	1646.0
38.90	718.0
39.90	203.0
43.90	761.0
44.90	341.0
45.70	128.0
47.00	545.0
48.00	317.0
48.90	1579.0
50.00	7708.0
51.00	2456.0
52.00	169.0
54.80	141.0
55.90	621.0
57.00	1155.0
60.00	457.0
61.00	1820.0
62.00	1859.0
63.00	1451.0
64.10	210.0
64.70	138.0
67.10	183.0
67.90	3975.0
69.00	3853.0
69.90	389.0
71.90	230.0
73.00	1622.0
74.00	6726.0
75.00	19240.0
76.00	1630.0
77.00	264.0
78.00	201.0
78.90	1207.0
79.80	385.0
80.90	1360.0
81.90	345.0
86.10	101.0
87.00	1617.0
88.00	1554.0
90.90	199.0
92.00	1169.0
92.90	1596.0
94.00	4329.0
95.00	36464.0
96.00	2760.0
103.90	148.0
104.90	103.0
105.80	183.0
115.80	123.0
116.80	243.0
118.00	104.0
118.80	159.0
127.90	130.0
128.90	104.0
129.90	155.0
140.80	365.0
142.90	374.0
147.90	123.0
154.90	116.0
172.20	118.0
174.00	25728.0
174.90	2275.0
176.00	24336.0
177.00	1775.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	479.0
37.00	1964.0
37.90	1810.0
38.90	753.0
40.00	216.0
43.90	757.0
45.10	382.0
47.00	651.0
48.00	396.0
48.90	1727.0
50.00	8464.0
51.00	2654.0
52.00	209.0
54.90	174.0
55.90	663.0
57.00	1222.0
58.10	117.0
60.00	517.0
61.00	1965.0
62.00	2047.0
63.00	1656.0
64.10	235.0
64.80	145.0
67.00	177.0
68.00	4312.0
69.00	4091.0
70.00	418.0
71.90	277.0
73.00	1756.0
74.00	7191.0
75.00	21192.0
76.00	1789.0
77.10	267.0
78.00	220.0
78.90	1332.0
79.80	425.0
80.90	1494.0
81.90	357.0
87.00	1734.0
87.90	1826.0
90.90	210.0
91.90	1305.0
93.00	1797.0
94.00	4906.0
95.00	39912.0
96.00	2949.0
96.90	117.0
103.80	183.0
105.80	178.0
115.90	160.0
116.80	221.0
118.00	136.0
118.80	191.0
127.90	137.0
128.90	130.0
129.90	175.0
140.90	437.0
142.90	429.0
147.90	127.0
154.90	106.0
172.10	137.0
172.90	367.0
173.90	29144.0
174.90	2454.0
176.00	27736.0
177.00	2021.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
35.90	472.0
37.00	1926.0
37.90	1863.0
39.00	769.0
40.00	230.0
44.00	729.0
45.10	384.0
47.00	761.0
48.00	384.0
48.90	1709.0
50.00	8555.0
51.00	2674.0
51.90	220.0
54.90	194.0
55.90	694.0
57.00	1201.0
58.00	109.0
60.00	493.0
60.90	2001.0
62.00	2098.0
63.00	1619.0
64.10	215.0
64.80	133.0
66.90	151.0
68.00	4294.0
69.00	4095.0
70.00	379.0
71.90	268.0
73.00	1719.0
74.00	7094.0
75.00	20968.0
76.00	1769.0
77.10	237.0
78.00	230.0
78.90	1287.0
79.90	427.0
80.90	1439.0
81.90	335.0
86.90	1746.0
87.90	1892.0
91.00	228.0
91.90	1314.0
93.00	1735.0
94.00	4889.0
95.00	39392.0
96.00	2687.0
96.90	133.0
103.80	211.0
105.80	180.0
115.90	194.0
116.90	238.0
118.00	147.0
118.80	198.0
127.90	142.0
128.80	122.0
129.90	179.0
140.90	477.0
142.90	422.0
147.90	104.0
172.10	163.0
172.90	334.0
173.90	29648.0
175.00	2331.0
175.90	28512.0
177.00	2024.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210