

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091225\
 Data File : VV039051.D
 Acq On : 12 Sep 2025 10:09
 Operator : SY/MD
 Sample : VV0912MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Quant Time: Sep 13 00:26:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM091125WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 12 01:49:00 2025
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.529	114	816489	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.773	117	853334	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.172	152	343996	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.291	65	385049	51.337	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.680%	
7) Chloroethane-d5		1.542	69	322663	54.385	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.780%	
11) 1,1-Dichloroethene-d2		2.069	65	170211	52.614	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	105.220%	
21) 2-Butanone-d5		3.780	46	418026	142.024	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	142.020%#	
24) Chloroform-d		4.246	84	682853	55.204	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.400%	
26) 1,2-Dichloroethane-d4		4.934	65	420147	57.678	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.360%	
32) Benzene-d6		4.953	84	1295196	52.355	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.720%	
36) 1,2-Dichloropropane-d6		5.979	67	417364	51.564	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.120%	
41) Toluene-d8		7.233	98	1049714	45.452	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.900%	
43) trans-1,3-Dichloroprop...		7.545	79	176146	46.047	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.100%	
47) 2-Hexanone-d5		8.011	63	288200	125.078	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	125.080%	
56) 1,1,2,2-Tetrachloroeth...		10.140	84	554963	48.147	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.300%	
66) 1,2-Dichlorobenzene-d4		11.548	152	364076	56.352	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.700%	
Target Compounds						Qvalue	
10) 1,1,2-Trichloro-1,2,2-...		2.069	101	5405	0.764	ug/L	# 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091225\
Data File : VV039051.D
Acq On : 12 Sep 2025 10:09
Operator : SY/MD
Sample : VV0912MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Time: Sep 13 00:26:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM091125WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 12 01:49:00 2025
Response via : Initial Calibration

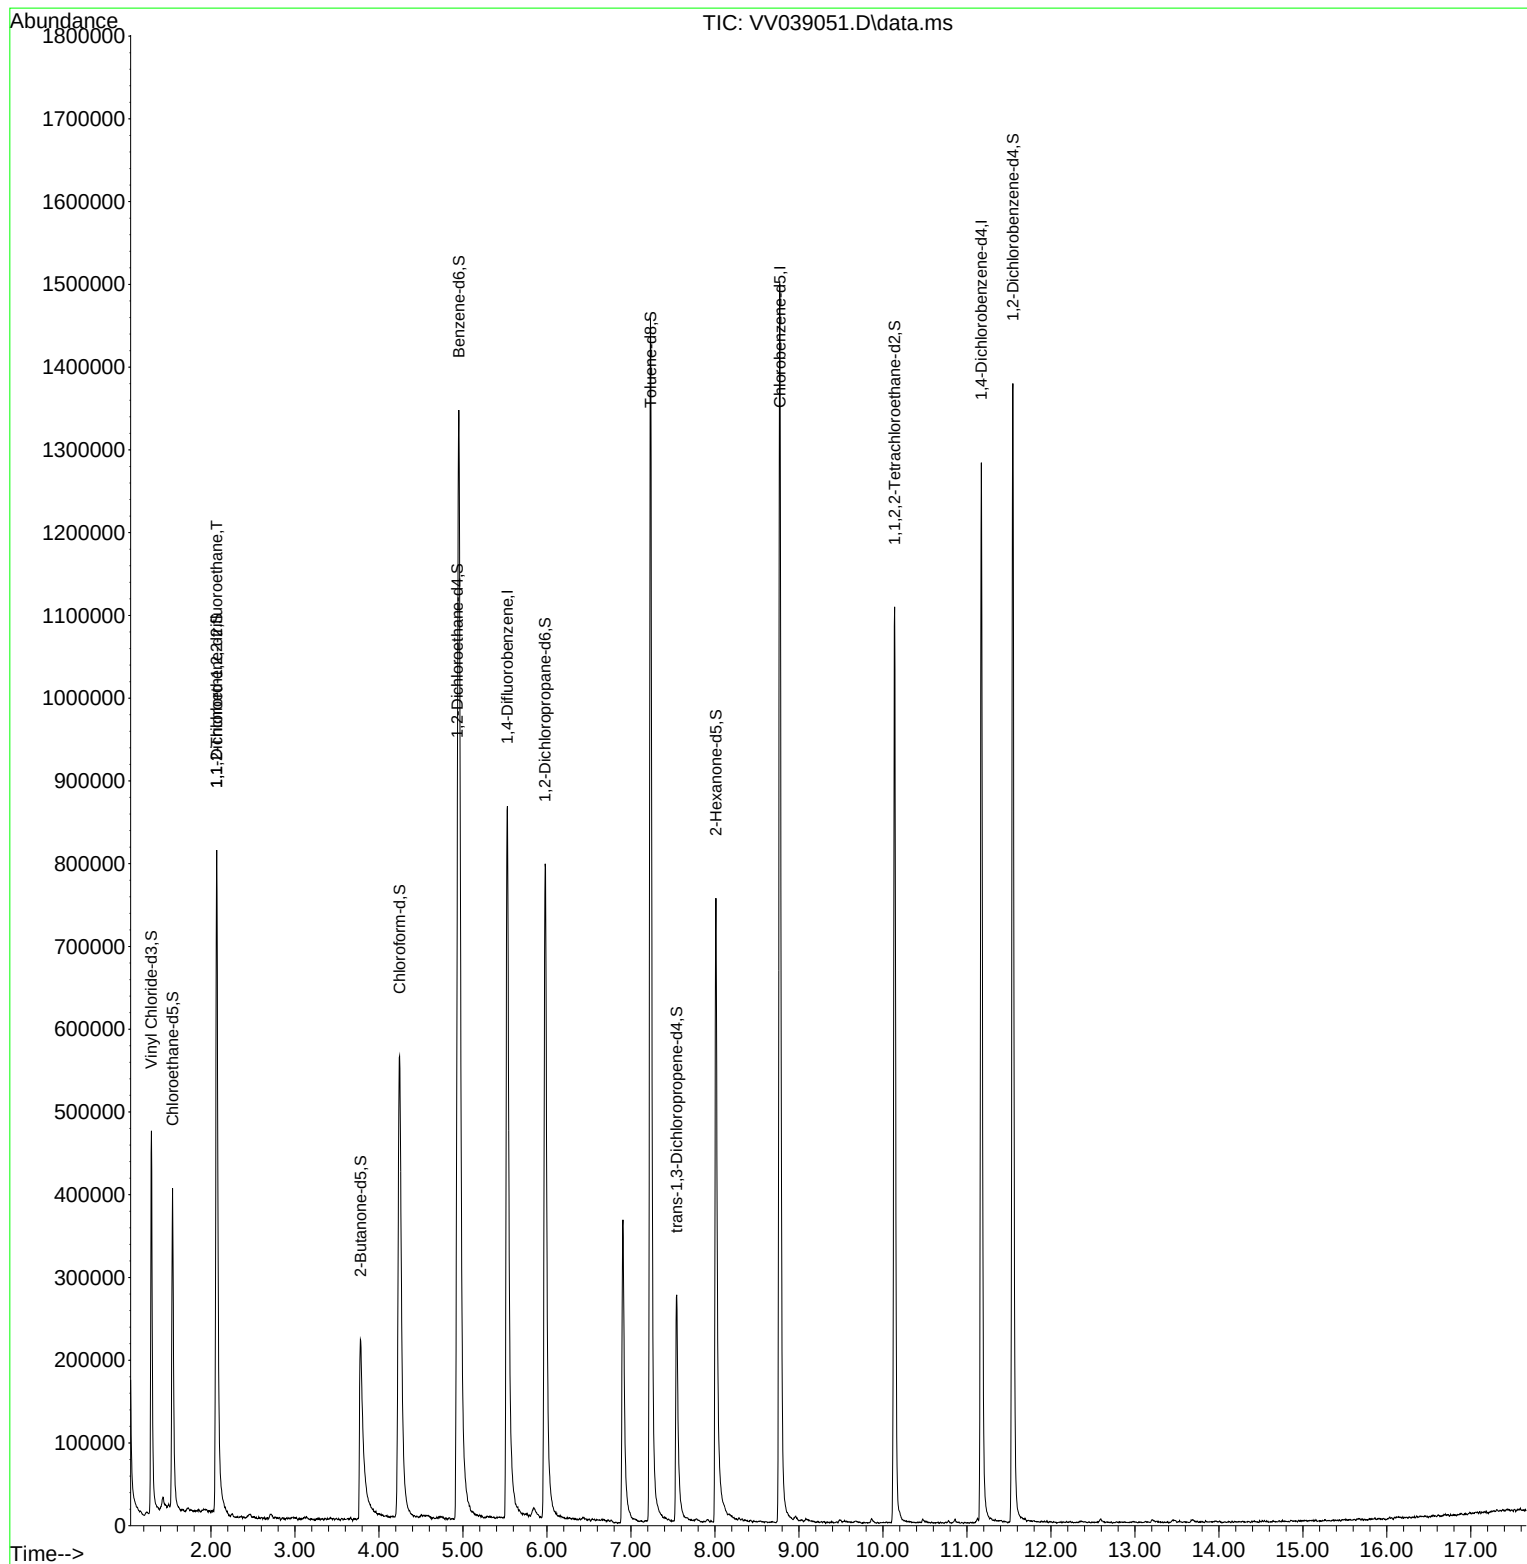

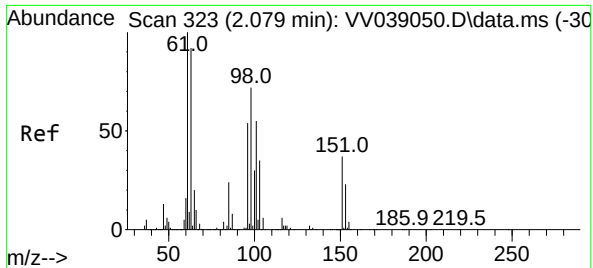

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.764 ug/L
 RT: 2.069 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV039051.D
 Acq: 12 Sep 2025 10:09

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Tgt Ion:	101	Resp:	5405
Ion	Ratio	Lower	Upper
101	100		
85	6.0	34.7	52.1#
151	15.6	54.6	81.8#

