


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091225\
Data File : VV039049.D
Acq On : 12 Sep 2025 08:46
Operator : SY/MD
Sample : BFB206
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB206

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM091125WMA.M
Title : VOC Analysis
Last Update : Fri Sep 12 01:49:00 2025

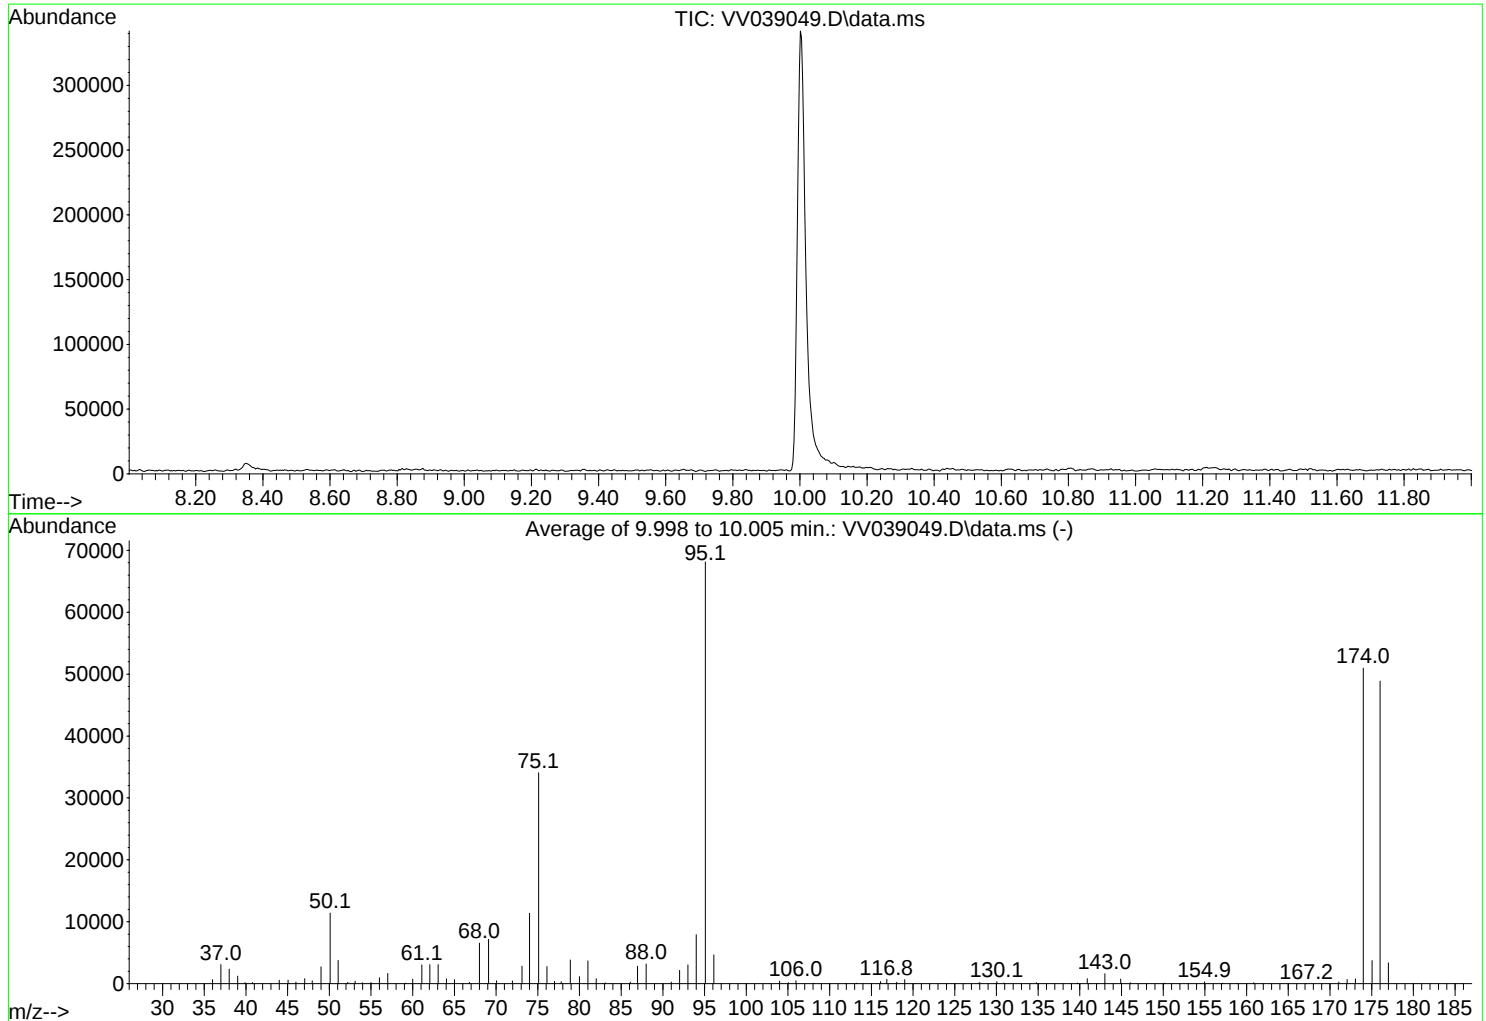

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	11388	PASS
75	95	30	80	50.0	34080	PASS
95	95	100	100	100.0	68144	PASS
96	95	5	9	6.8	4649	PASS
173	174	0.00	2	1.5	767	PASS
174	95	50	120	74.8	50971	PASS
175	174	5	9	7.3	3725	PASS
176	174	95	105	95.9	48880	PASS
177	176	5	10	6.9	3374	PASS

m/z	Abundance
36.60	107.0
40.00	910.0
41.20	122.0
44.00	771.0
53.50	114.0
57.30	101.0
77.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	609.0
37.00	3358.0
38.00	2238.0
39.00	1177.0
39.90	1008.0
40.80	127.0
44.00	1320.0
45.10	644.0
46.00	163.0
47.10	882.0
48.00	486.0
49.00	2536.0
50.10	11140.0
51.00	3520.0
52.20	206.0
53.10	326.0
54.00	169.0
55.00	195.0
56.00	931.0
57.00	1489.0
59.10	110.0
60.00	696.0
61.10	2941.0
62.00	2678.0
63.10	2929.0
64.00	747.0
65.00	593.0
66.80	214.0
68.00	6732.0
69.10	6888.0
70.10	458.0
72.00	385.0
73.10	2463.0
74.00	10692.0
75.10	32640.0
76.10	2580.0
77.00	519.0
77.70	365.0
78.90	3430.0
80.00	1026.0
81.00	3376.0
82.00	837.0
82.80	132.0
83.10	113.0
86.00	197.0
86.90	2477.0
88.00	2825.0
91.10	218.0
92.00	2085.0
93.00	2784.0
94.00	7679.0
95.10	65808.0
96.10	4593.0
102.80	107.0
104.00	344.0
105.00	162.0
106.00	452.0
111.90	104.0
113.20	109.0
116.10	380.0
116.90	632.0
118.10	210.0
119.00	596.0
120.30	144.0
126.20	100.0
127.80	226.0
130.10	282.0
130.90	111.0
134.80	141.0
139.70	156.0
140.90	748.0
142.10	107.0
143.00	1565.0
144.90	651.0
146.00	164.0
154.90	214.0
157.10	140.0
160.90	147.0
171.10	208.0
172.00	513.0
173.00	761.0
174.00	46576.0
175.00	3680.0
176.00	45240.0
177.00	3192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	693.0
37.00	3198.0
38.00	2439.0
39.00	1259.0
39.90	1085.0
40.80	196.0
44.10	1295.0
45.10	571.0
46.00	228.0
47.10	822.0
48.00	466.0
49.00	2837.0
50.10	11798.0
51.10	3812.0
52.20	225.0
53.10	415.0
54.00	161.0
55.00	184.0
56.00	1004.0
57.00	1708.0
59.20	115.0
60.00	768.0
61.10	3193.0
62.10	3111.0
63.00	3221.0
64.00	766.0
65.00	668.0
66.00	101.0
66.80	196.0
68.00	6844.0
69.10	7539.0
70.00	472.0
71.90	444.0
73.10	2957.0
74.00	11892.0
75.10	35320.0
76.10	2817.0
77.00	549.0
77.80	292.0
78.90	4043.0
80.00	1186.0
81.00	3772.0
82.00	827.0
83.10	114.0
86.10	257.0
87.00	2926.0
88.00	3368.0
91.00	284.0
92.00	2293.0
93.00	3128.0
94.00	8085.0
95.10	70432.0
96.10	4767.0
104.00	432.0
105.00	155.0
106.00	511.0
108.10	118.0
113.30	117.0
116.10	352.0
116.90	739.0
118.10	246.0
119.00	702.0
128.00	272.0
130.00	315.0
130.90	128.0
134.80	170.0
139.70	145.0
140.90	795.0
143.00	1711.0
144.90	761.0
146.00	154.0
150.20	114.0
154.90	290.0
157.10	103.0
160.90	158.0
171.00	245.0
172.10	676.0
173.10	774.0
174.00	52760.0
175.10	3852.0
176.00	50544.0
177.00	3480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	672.0
37.00	2690.0
38.00	2372.0
39.00	1176.0
39.90	1163.0
40.80	252.0
44.10	1307.0
45.00	515.0
46.00	405.0
47.00	672.0
47.90	431.0
49.00	2753.0
50.10	11226.0
51.10	3948.0
52.20	236.0
53.10	419.0
53.90	131.0
55.00	171.0
56.00	947.0
57.00	1770.0
60.00	688.0
61.10	2954.0
62.10	3456.0
63.00	3047.0
64.10	828.0
65.00	702.0
66.80	180.0
68.00	6074.0
69.10	7072.0
70.00	444.0
71.90	488.0
73.10	3025.0
74.00	11563.0
75.10	34280.0
76.10	2870.0
77.00	562.0
77.90	262.0
78.90	4021.0
80.00	1239.0
81.00	3850.0
82.00	733.0
83.10	133.0
86.20	340.0
87.00	3081.0
88.00	3357.0
90.90	296.0
92.00	2097.0
93.00	3149.0
94.00	7969.0
95.10	68192.0
96.10	4586.0
97.00	179.0
104.00	458.0
105.10	150.0
105.90	474.0
108.10	136.0
110.00	107.0
116.10	241.0
116.80	697.0
118.00	232.0
119.00	668.0
128.00	294.0
130.00	382.0
130.90	101.0
134.80	133.0
140.90	853.0
143.00	1506.0
144.90	833.0
146.10	121.0
150.20	104.0
153.00	107.0
155.00	346.0
158.80	120.0
160.80	142.0
167.20	102.0
171.00	351.0
172.00	791.0
173.10	766.0
174.00	53576.0
175.00	3643.0
176.00	50856.0
177.00	3450.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206