

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091318\
 Data File : VV007521.D
 Acq On : 13 Sep 2018 20:37
 Operator : SY/MD
 Sample : J4864-06
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D12

Quant Time: Sep 14 05:39:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 14 05:10:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	128581	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	115220	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59444	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27784	4.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.80%
7) Chloroethane-d5	1.59	69	23968	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.13	63	47125	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	3.97	46	45262	48.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.62%
24) Chloroform-d	4.41	84	57985	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	5.09	65	28774	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
32) Benzene-d6	5.10	84	113396	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
36) 1,2-Dichloropropane-d6	6.12	67	34393	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.20%
41) Toluene-d8	7.36	98	114552	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.67	79	14491	4.02	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.40%
46) 2-Hexanone-d5	8.14	63	23782	41.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.64%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	19465	3.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	71.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	46742	4.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.00%


Target Compounds					Qvalue
13) Acetone	2.21	43	9975	16.303 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091318\
Data File : VV007521.D
Acq On : 13 Sep 2018 20:37
Operator : SY/MD
Sample : J4864-06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D12

Quant Time: Sep 14 05:39:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 14 05:10:24 2018
Response via : Initial Calibration

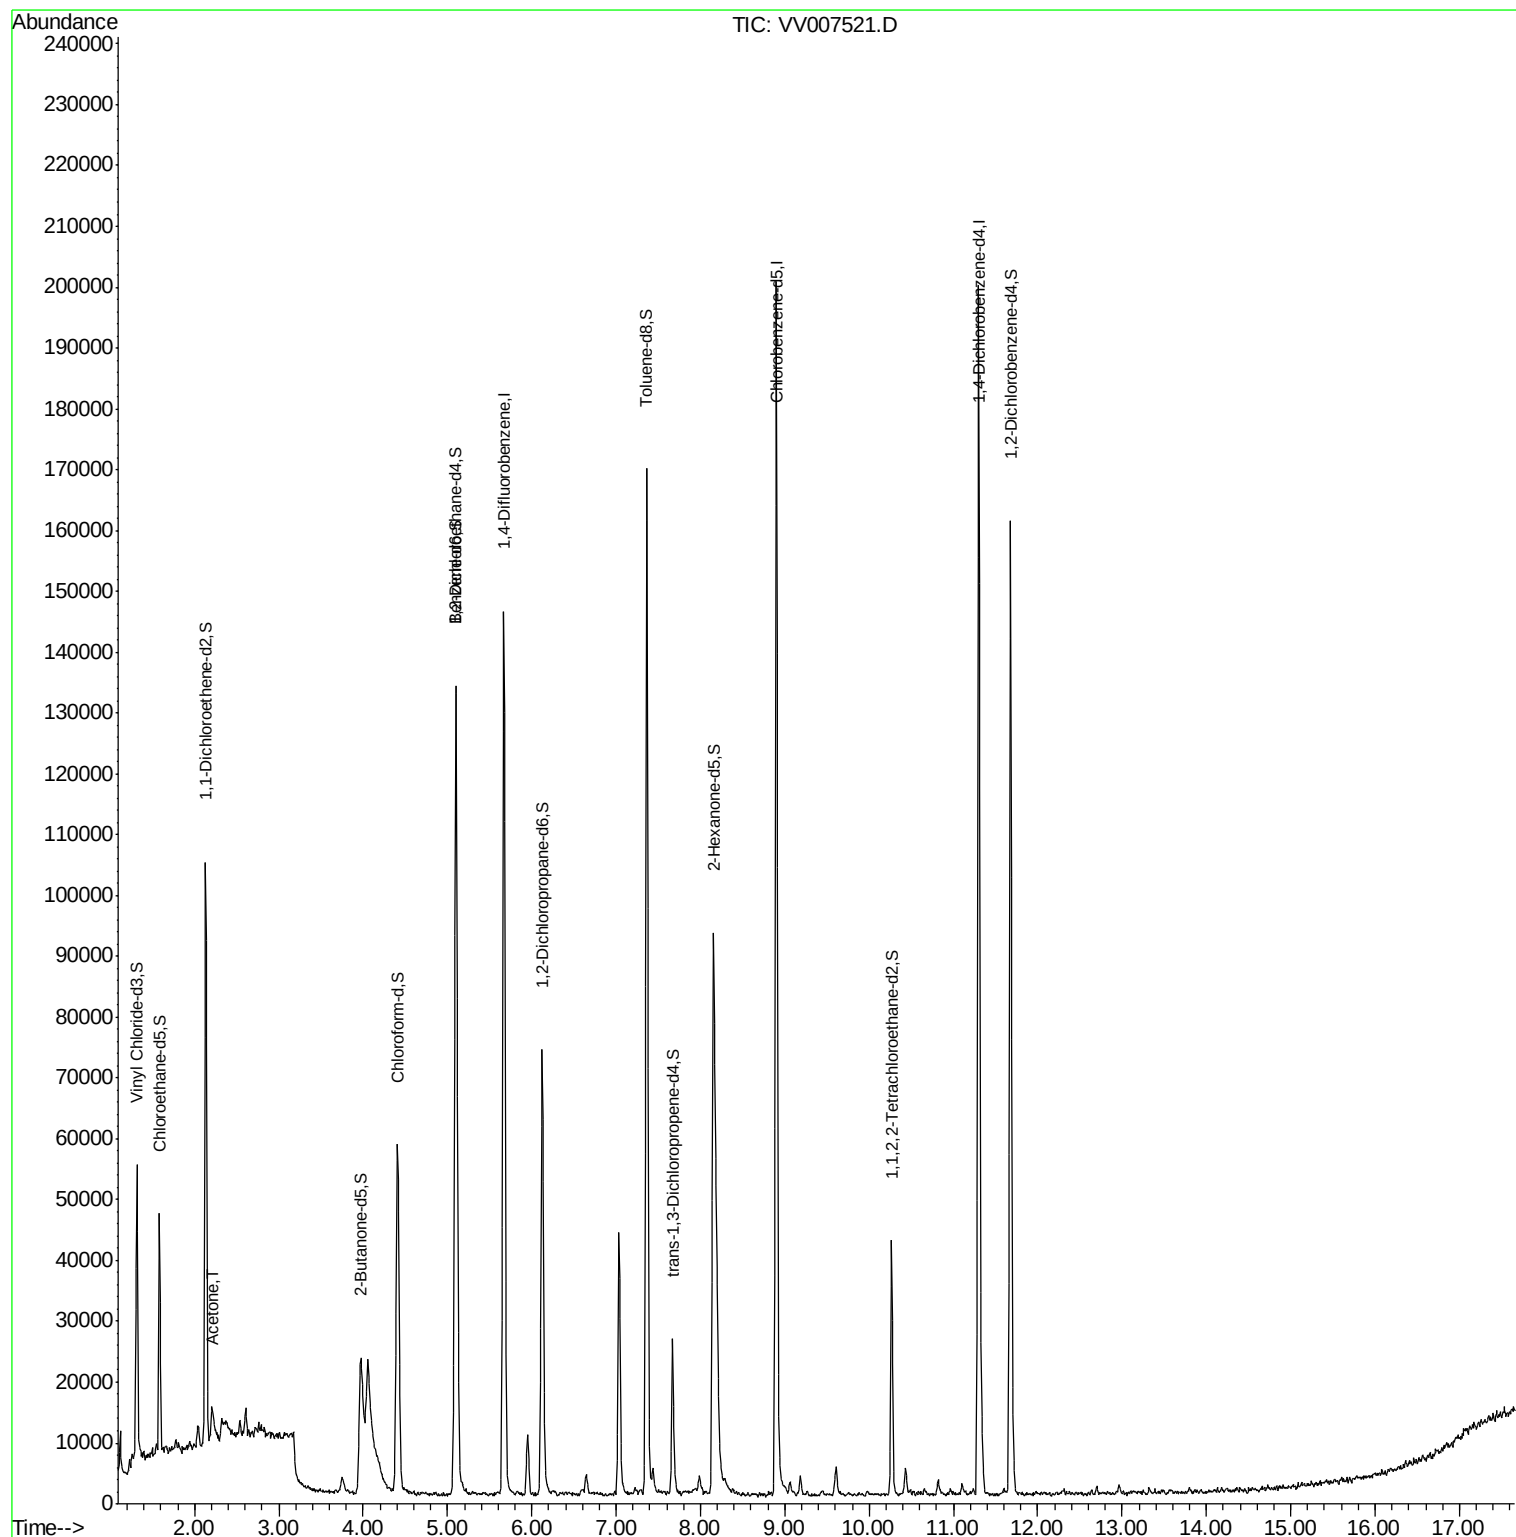

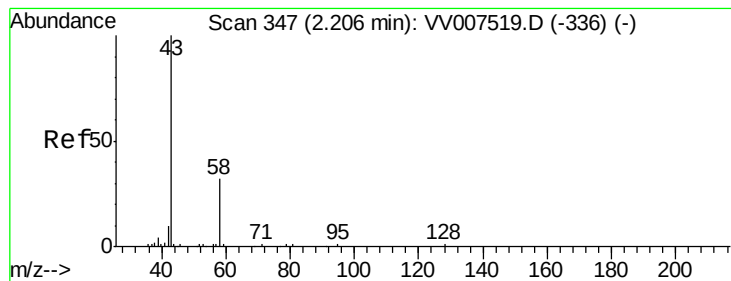

#13
 Acetone
 Concen: 16.303 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. 0.00 min
 Lab File: VV007521.D
 Acq: 13 Sep 2018 20:37

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D12

Tgt Ion: 43 Resp: 9975
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 63.4

