


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091318\
Data File : VV007510.D
Acq On : 13 Sep 2018 12:37
Operator : SY/MD
Sample : BFB71
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 17 12:17:05 2018

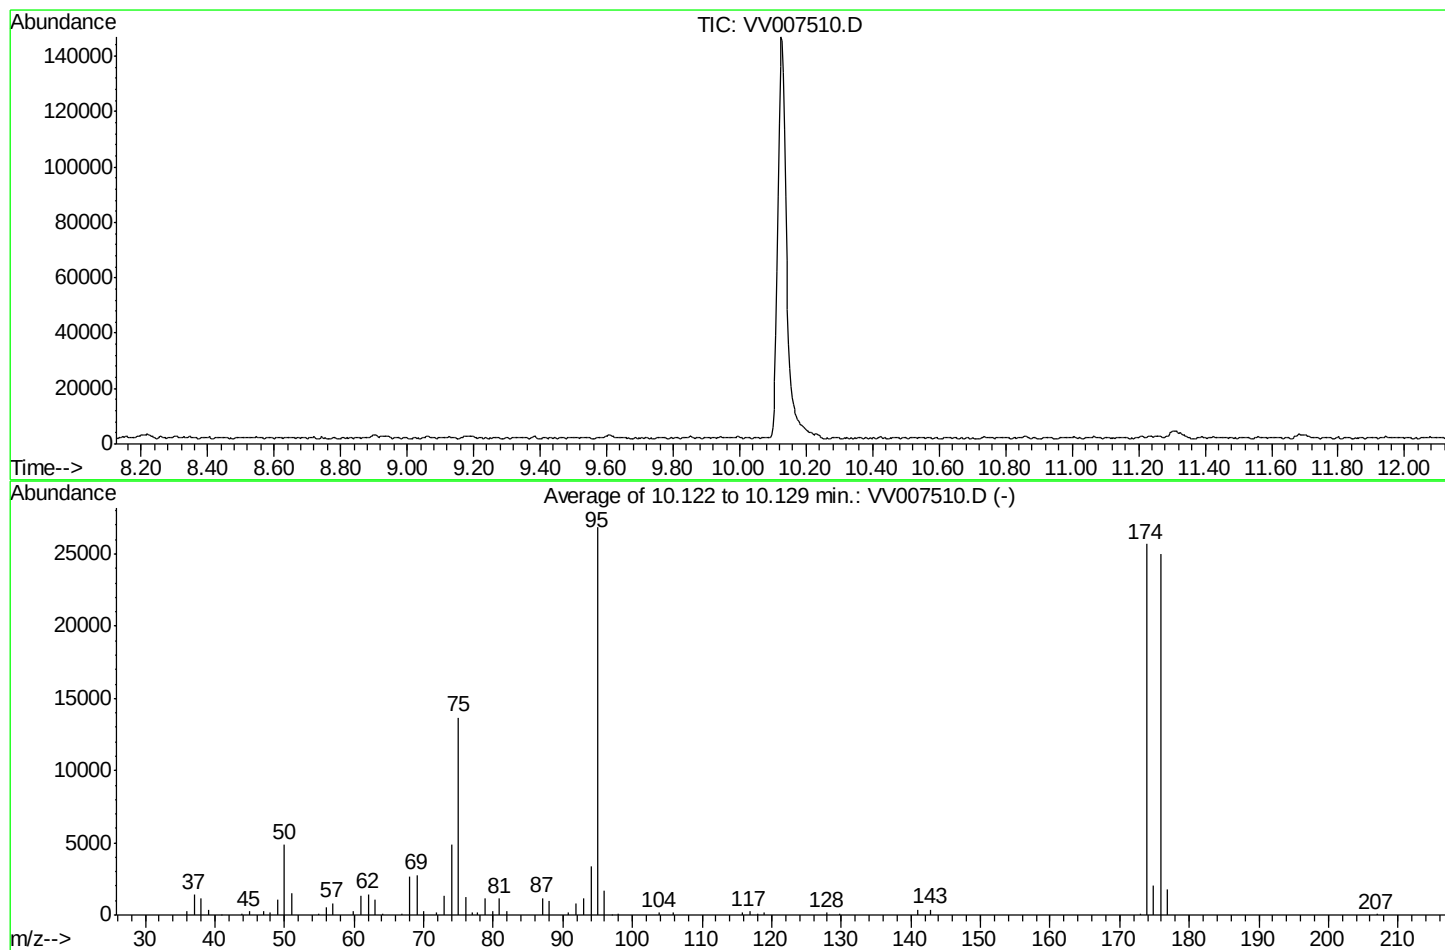

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4851	PASS
75	95	30	80	50.9	13658	PASS
95	95	100	100	100.0	26850	PASS
96	95	5	9	6.3	1688	PASS
173	174	0.00	2	0.5	127	PASS
174	95	50	120	95.7	25698	PASS
175	174	5	9	8.0	2053	PASS
176	174	95	101	97.5	25048	PASS
177	176	5	9	7.2	1801	PASS

m/z	Abundance
39.00	170.0
39.90	106.0
40.90	213.0
41.90	186.0
42.90	304.0
43.90	665.0
44.90	101.0
54.90	226.0
56.90	111.0
69.00	133.0
206.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	278.0
37.00	1349.0
38.00	1078.0
39.00	566.0
40.90	242.0
41.80	155.0
42.90	240.0
43.90	783.0
44.90	310.0
46.90	292.0
47.90	170.0
49.00	1022.0
50.00	4759.0
51.00	1477.0
55.00	288.0
56.00	504.0
57.00	929.0
59.90	301.0
61.00	1266.0
62.00	1388.0
63.00	967.0
64.10	144.0
67.00	126.0
68.00	2674.0
69.00	2754.0
69.90	260.0
71.90	171.0
73.00	1354.0
74.00	4733.0
75.00	13301.0
76.00	1157.0
77.10	175.0
77.80	183.0
78.90	1158.0
79.90	297.0
80.90	1108.0
81.90	253.0
87.00	1097.0
88.00	949.0
90.90	197.0
91.90	767.0
93.00	1215.0
94.00	3236.0
95.00	25504.0
96.00	1631.0
97.90	157.0
103.90	184.0
105.80	145.0
115.80	172.0
116.80	242.0
118.00	129.0
118.90	264.0
127.90	187.0
129.80	132.0
140.90	321.0
142.90	349.0
173.00	381.0
173.90	23824.0
174.90	1931.0
175.90	23512.0
176.90	1611.0
207.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	283.0
37.00	1483.0
38.00	1185.0
39.00	575.0
40.90	230.0
41.80	129.0
42.90	257.0
43.90	776.0
44.90	380.0
47.00	291.0
47.90	161.0
49.00	1077.0
50.00	4956.0
51.00	1524.0
55.00	301.0
56.00	561.0
57.00	995.0
59.90	305.0
61.00	1426.0
62.00	1425.0
63.00	1124.0
64.00	104.0
67.00	135.0
68.00	2671.0
69.00	3016.0
70.00	267.0
71.90	199.0
73.00	1432.0
74.00	5022.0
75.00	13991.0
76.00	1331.0
76.90	170.0
77.80	178.0
78.90	1213.0
79.90	311.0
80.90	1167.0
81.90	277.0
87.00	1218.0
87.90	973.0
90.80	203.0
92.00	824.0
93.00	1223.0
94.00	3472.0
95.00	27544.0
96.00	1732.0
97.90	127.0
103.90	173.0
105.80	161.0
115.80	205.0
116.80	261.0
118.00	127.0
118.90	231.0
127.90	174.0
129.90	128.0
140.90	359.0
142.90	391.0
173.90	26456.0
174.90	2122.0
175.90	25872.0
176.90	1855.0
207.00	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	244.0
37.00	1413.0
38.00	1199.0
39.00	544.0
40.00	126.0
41.00	191.0
42.90	265.0
44.00	774.0
44.90	383.0
47.10	338.0
47.90	143.0
49.00	1067.0
50.00	4840.0
51.00	1486.0
54.90	282.0
56.00	539.0
56.90	911.0
59.90	303.0
61.00	1401.0
62.00	1451.0
63.00	1207.0
66.90	135.0
68.00	2537.0
69.00	2971.0
70.10	246.0
71.90	204.0
73.00	1327.0
74.00	4977.0
75.00	13684.0
76.00	1353.0
76.90	203.0
77.80	156.0
78.90	1153.0
79.90	324.0
80.90	1168.0
81.90	298.0
87.00	1224.0
87.90	951.0
90.80	197.0
92.00	797.0
93.00	1135.0
94.00	3358.0
95.00	27504.0
96.00	1701.0
97.00	111.0
103.90	162.0
105.80	172.0
115.80	190.0
116.80	231.0
117.90	126.0
118.80	179.0
128.00	157.0
129.90	115.0
140.90	356.0
142.90	378.0
173.90	26816.0
174.90	2107.0
175.90	25760.0
176.90	1938.0
207.00	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71