

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (QT Reviewed)


Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 01:40:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

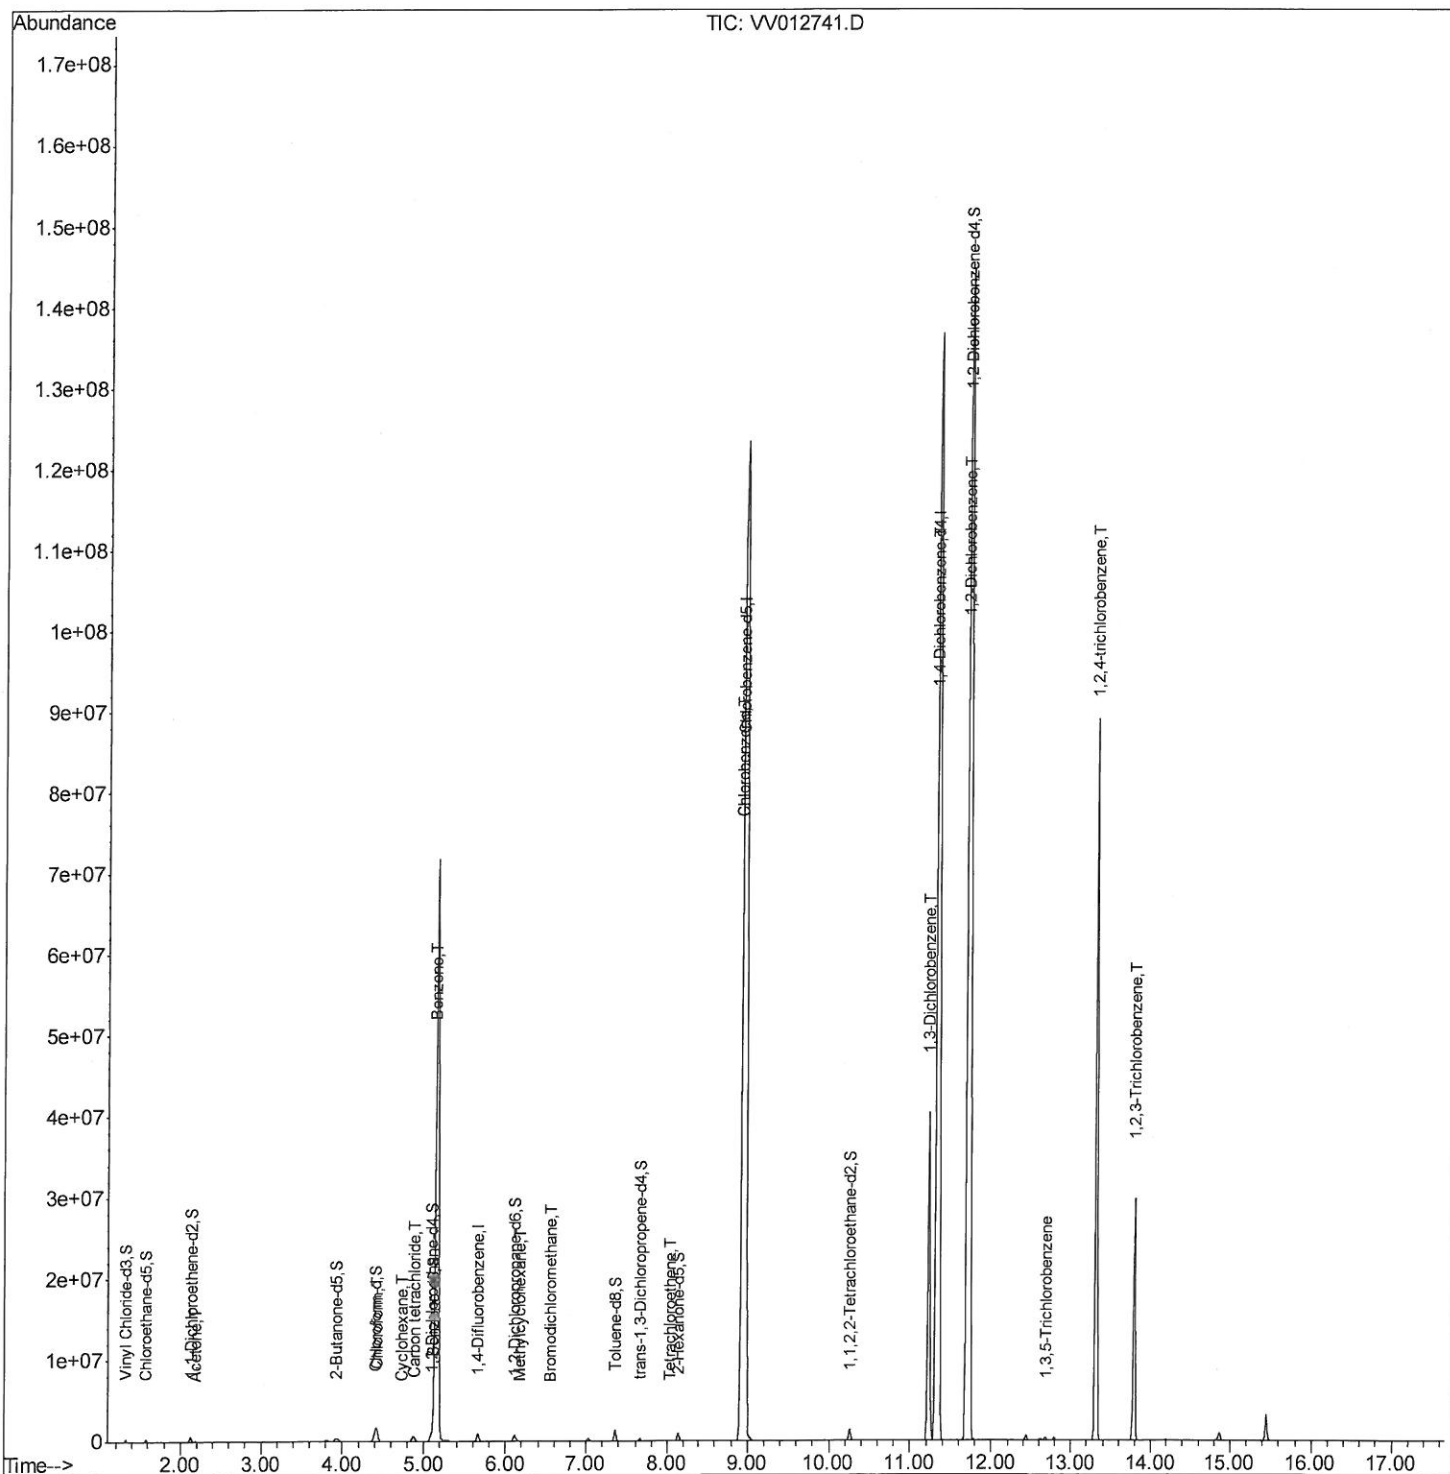

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

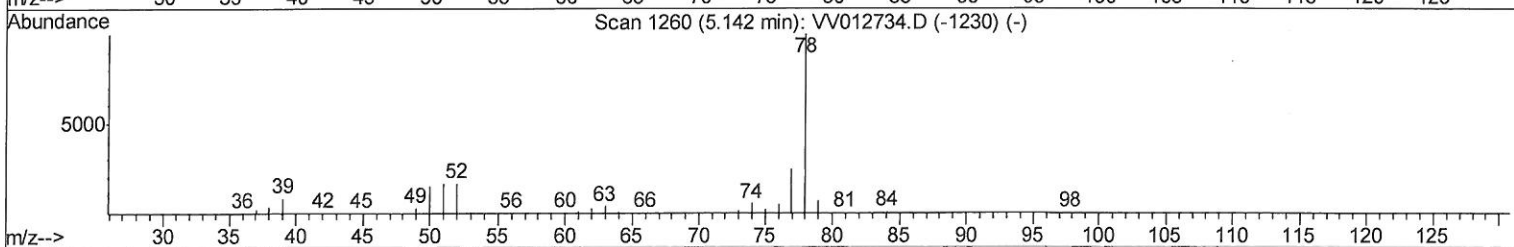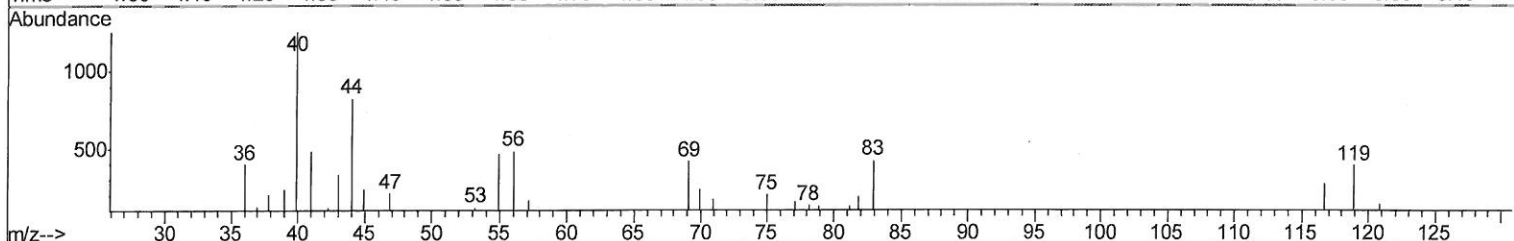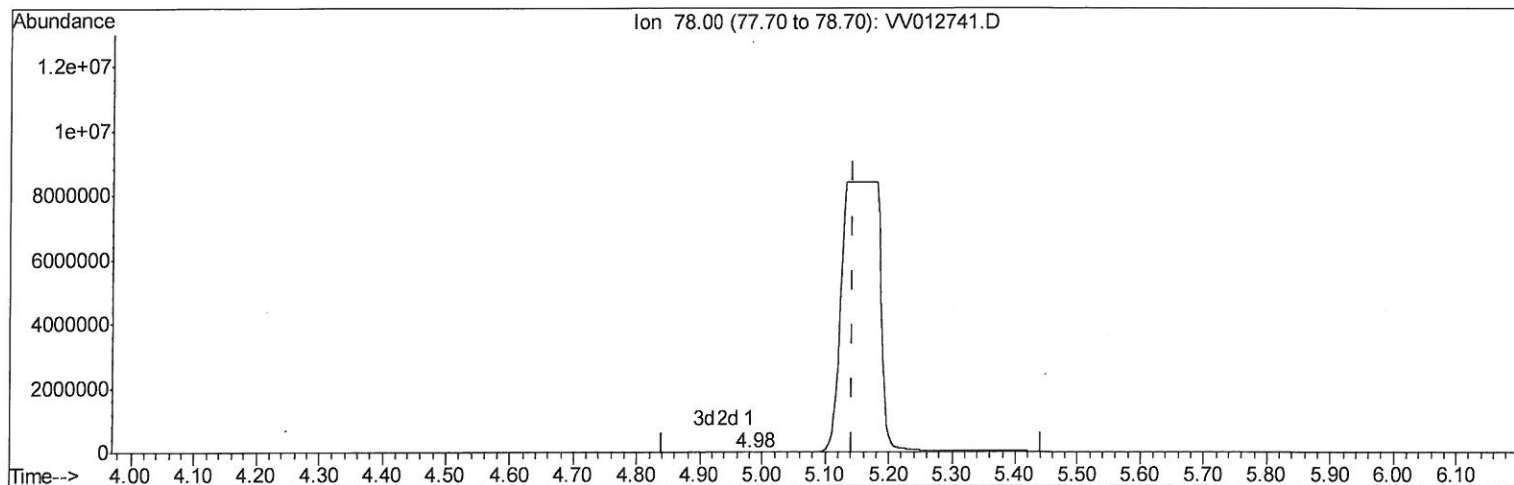

TIC: VV012741.D

(33) Benzene (T)

4.981min (-0.161) 0.00ug/L

response 92

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

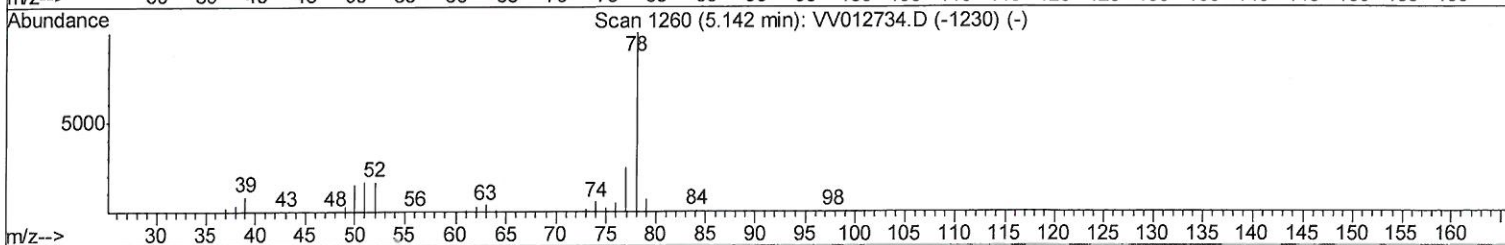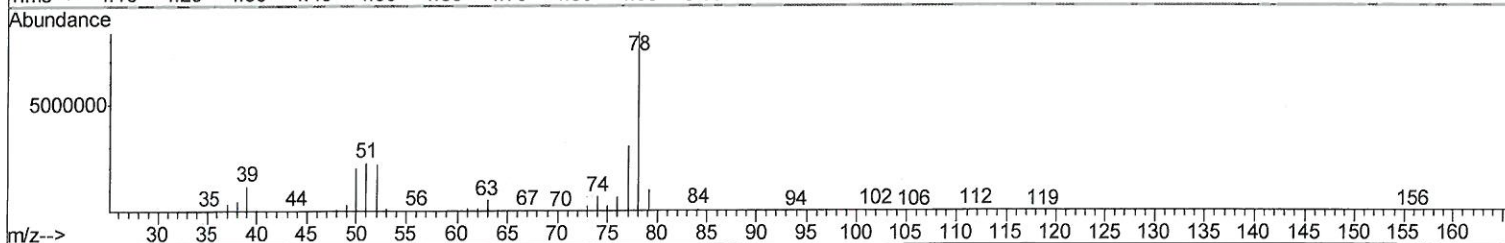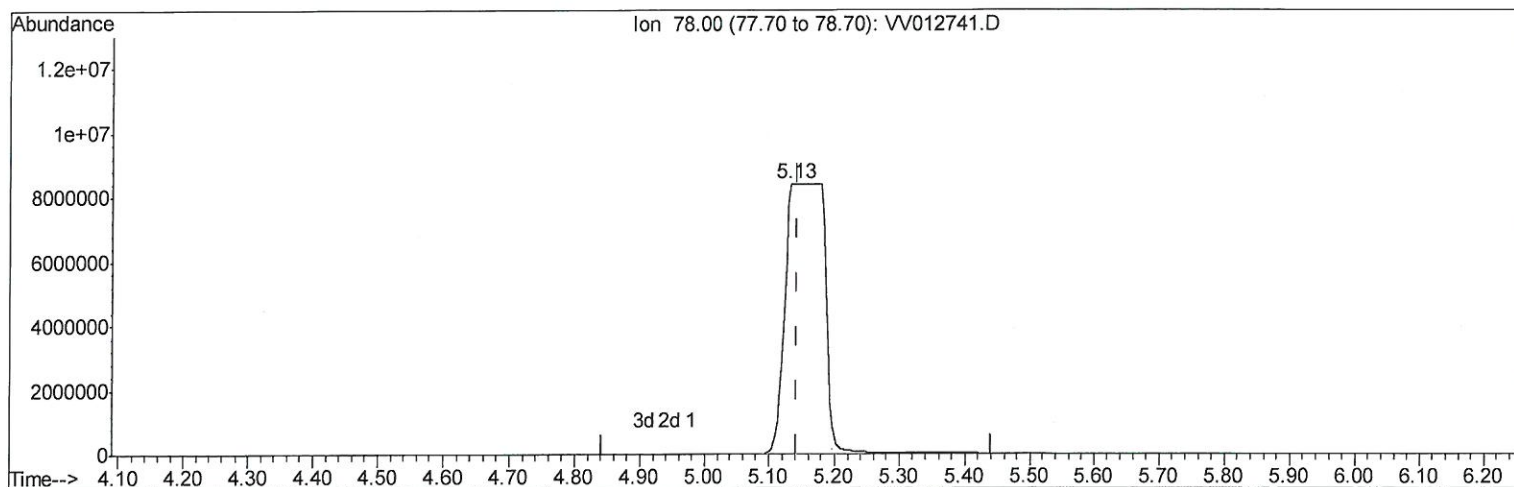

TIC: VV012741.D

(33) Benzene (T)

5.132min (-0.010) 1567.78ug/L m

response 34454113

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
9/13/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

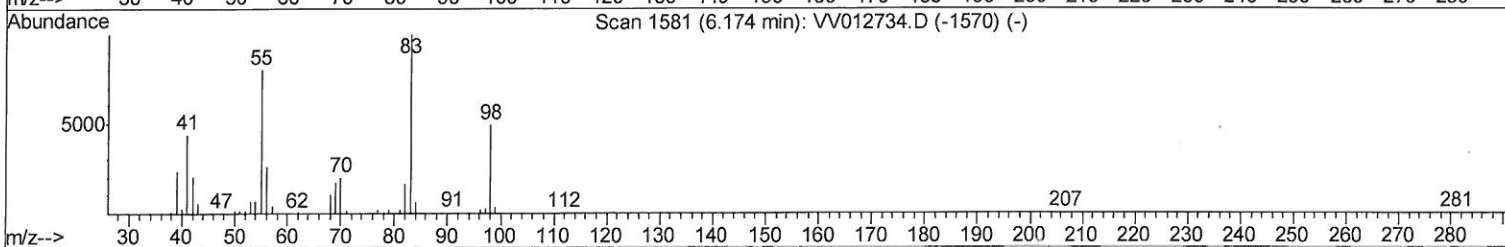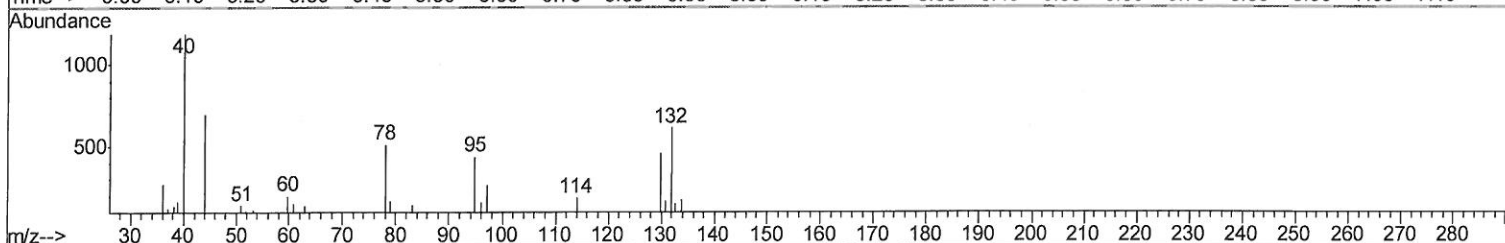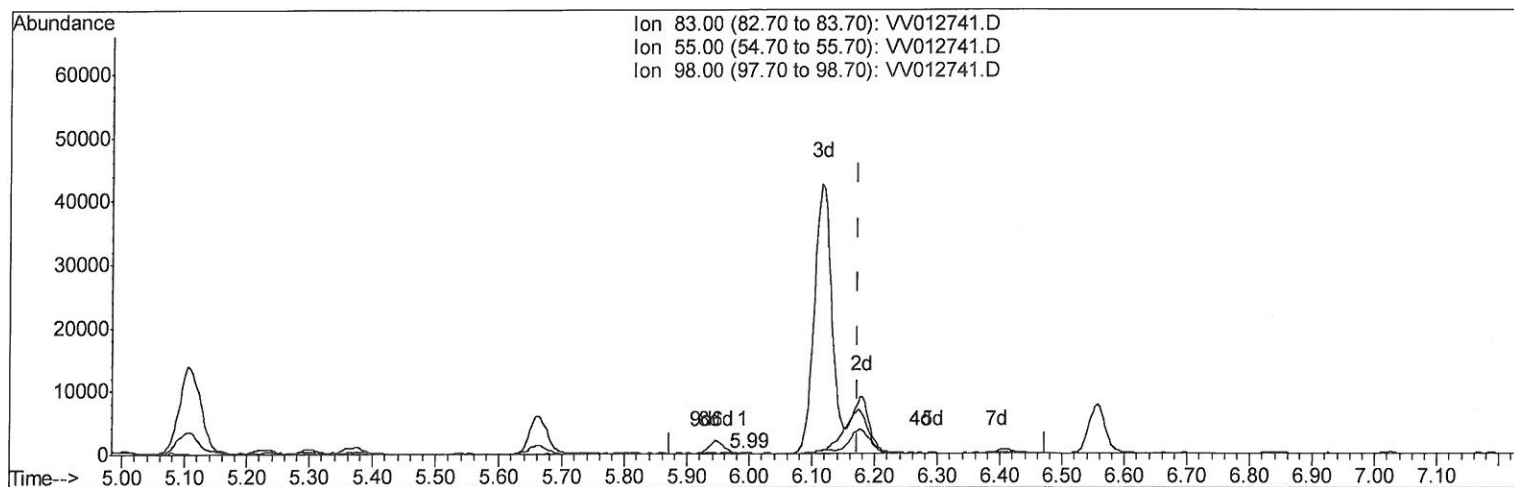

TIC: VV012741.D

(35) Methylcyclohexane (T)

5.991min (-0.183) 0.01ug/L

response 100

Ion	Exp%	Act%
83.00	100	100
55.00	77.70	71.00
98.00	49.20	45.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

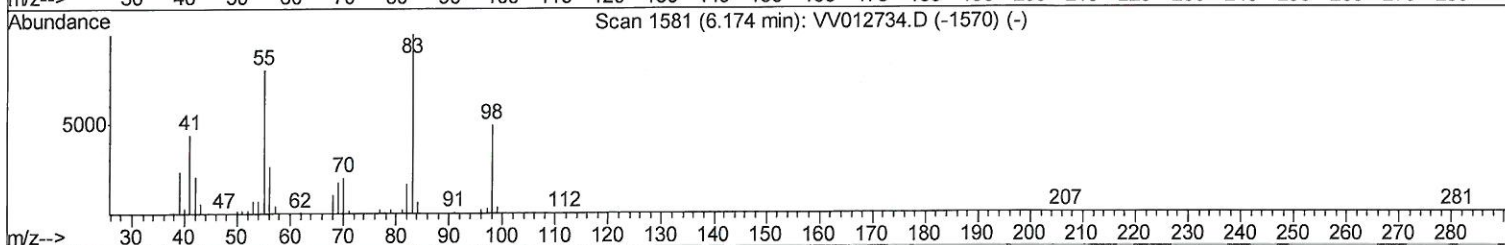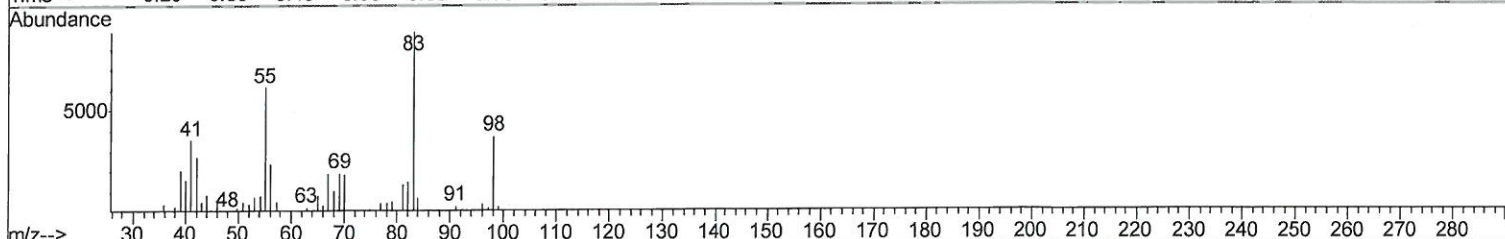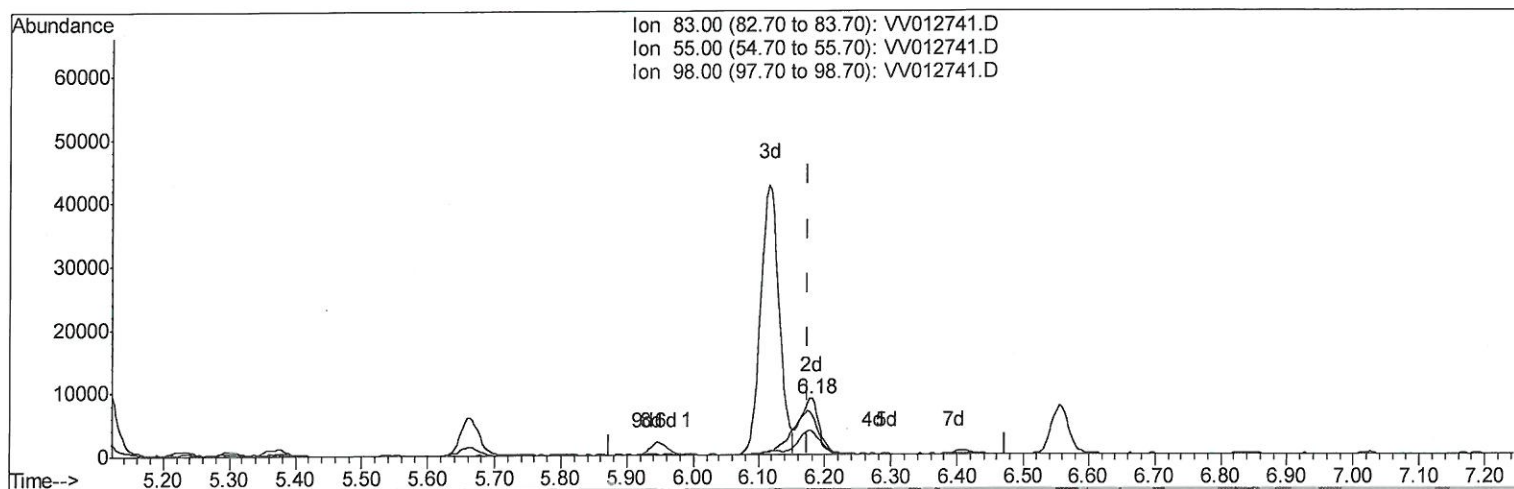

TIC: VV012741.D

(35) Methylcyclohexane (T)

6.180min (+0.006) 2.24ug/L m

response 18032

Ion	Exp%	Act%
-----	------	------

83.00	100	100
-------	-----	-----

55.00	77.70	0.39#
-------	-------	-------

98.00	49.20	0.25#
-------	-------	-------

0.00	0.00	0.00
------	------	------

7 mQ
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

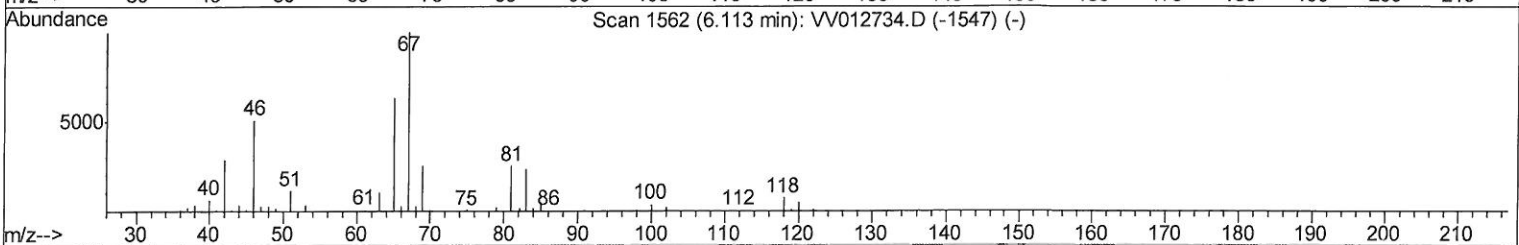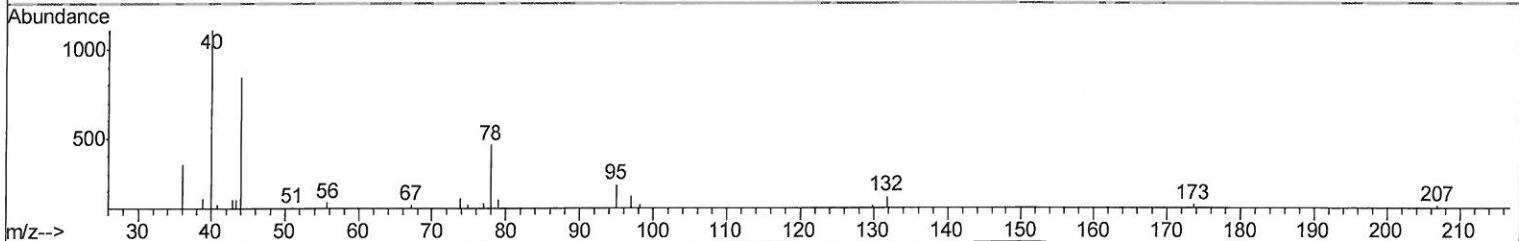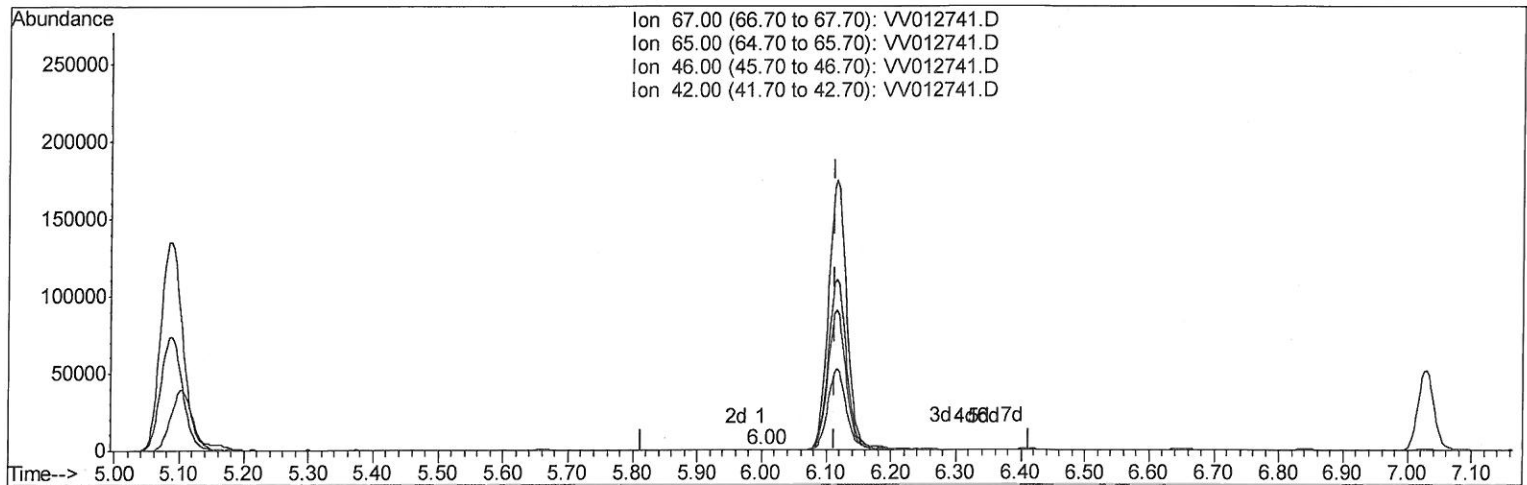

TIC: VV012741.D

(36) 1,2-Dichloropropane-d6 (S)

6.000min (-0.113) 0.01ug/L

response 46

Ion	Exp%	Act%
67.00	100	100
65.00	64.10	95.65#
46.00	50.60	139.13#
42.00	29.50	0.00#

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

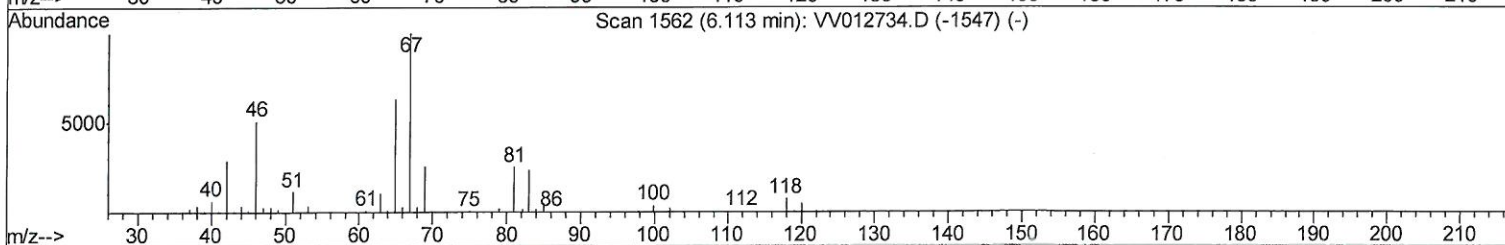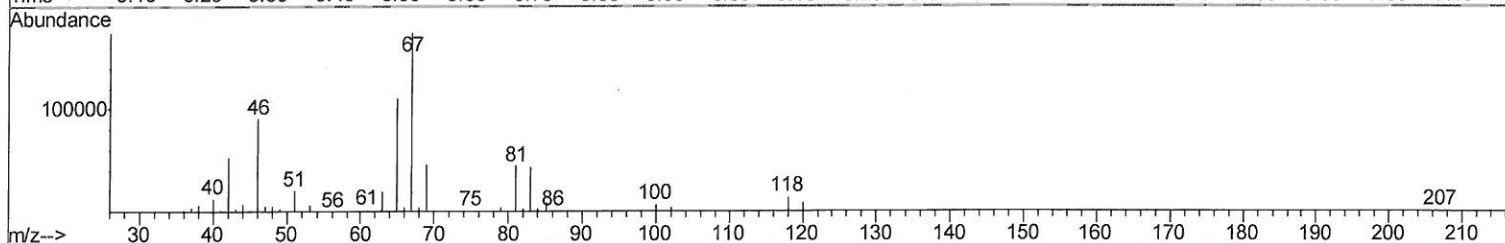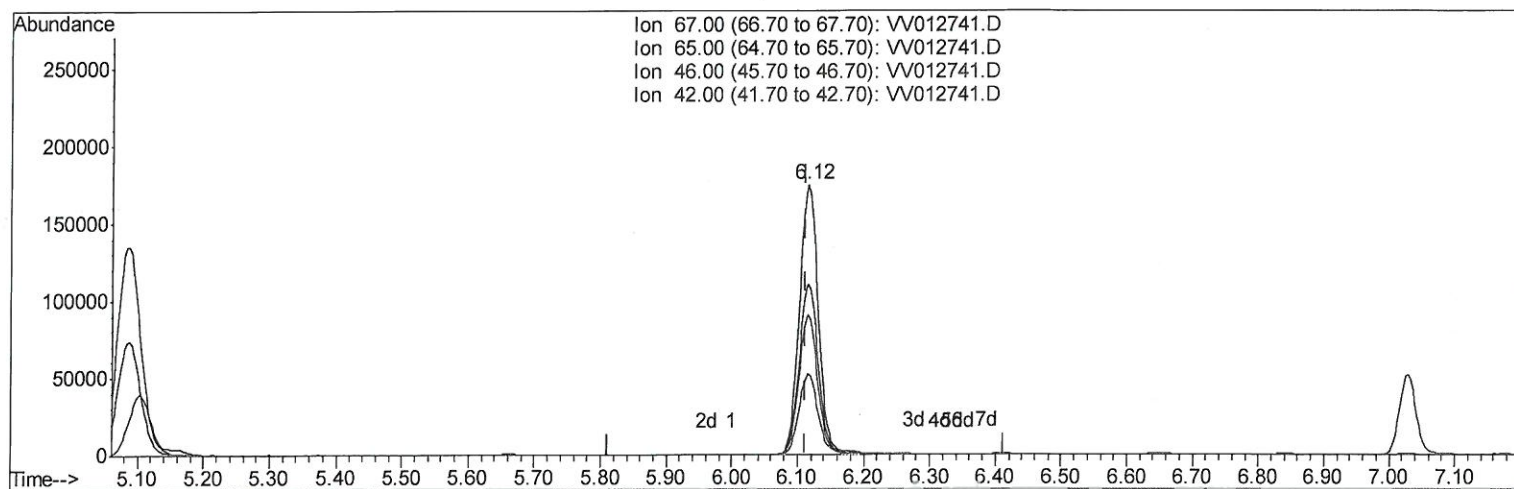

TIC: VV012741.D

(36) 1,2-Dichloropropane-d6 (S)

6.116min (+0.003) 45.46ug/L m

response 345850

Ion Exp% Act%

67.00	100	100
65.00	64.10	0.01#
46.00	50.60	0.02#
42.00	29.50	0.00#

7 MD
9/20/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

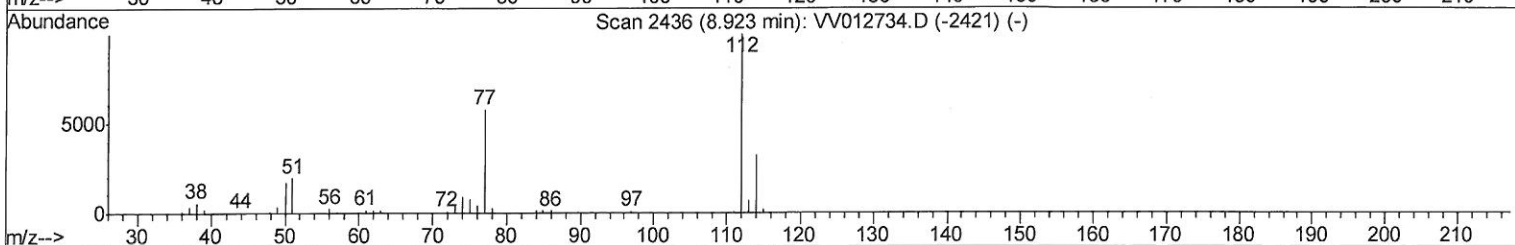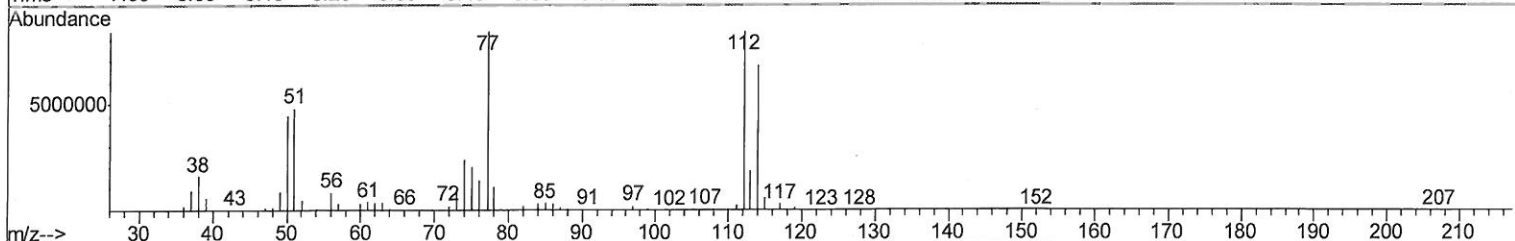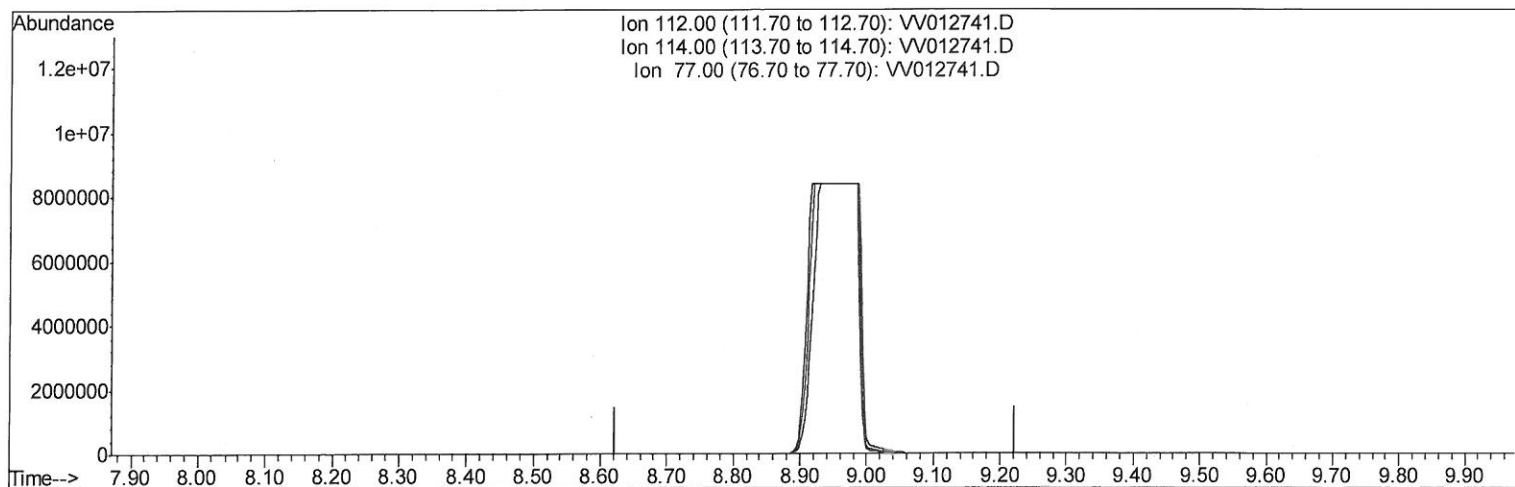

TIC: VV012741.D

(51) Chlorobenzene (T)
8.923min (-8.923) 0.00ug/L
response 0

Ion	Exp%	Act%
112.00	100	0.00
114.00	32.00	0.00#
77.00	58.40	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

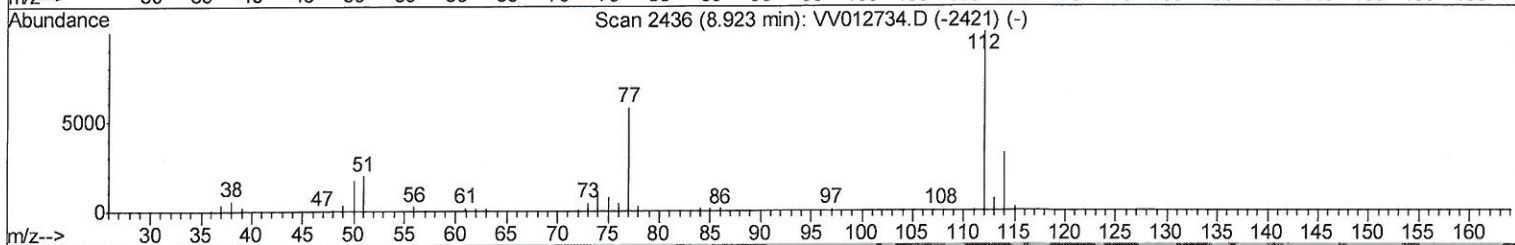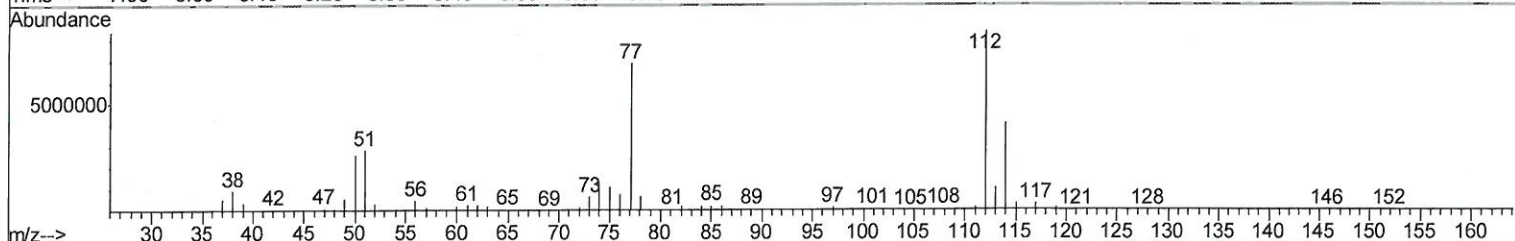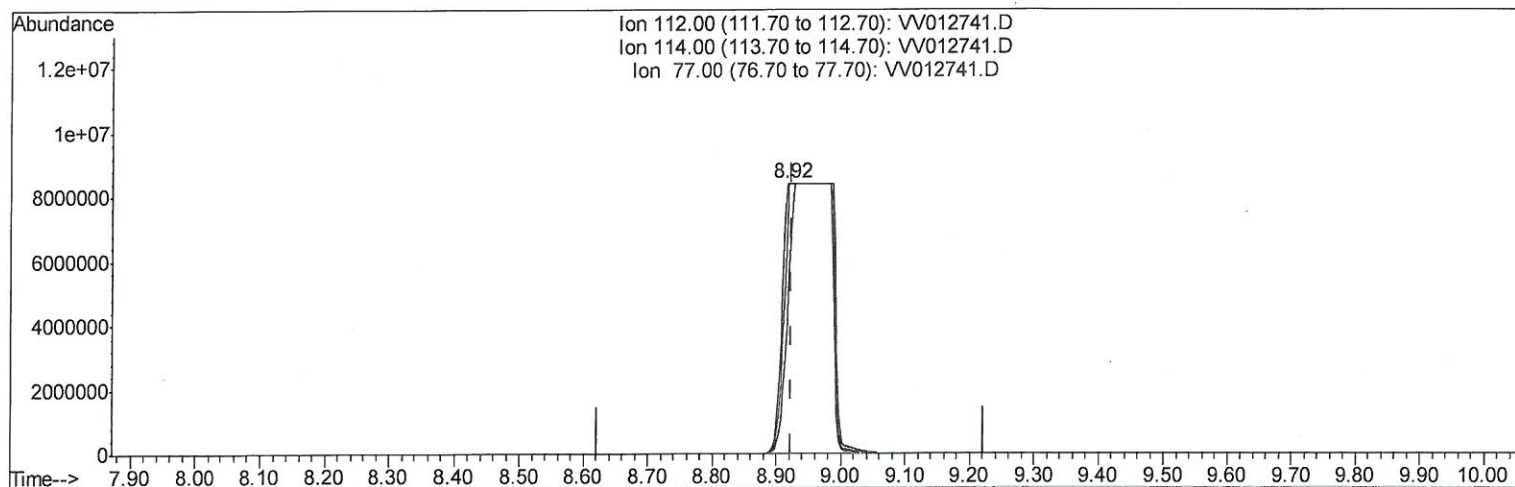

(51) Chlorobenzene (T)

8.916min (-0.006) 2783.09ug/L m

response 43517174

Ion Exp% Act%

112.00 100 100

114.00 32.00 48.40#

77.00 58.40 81.89#

0.00 0.00 0.00

7MA
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

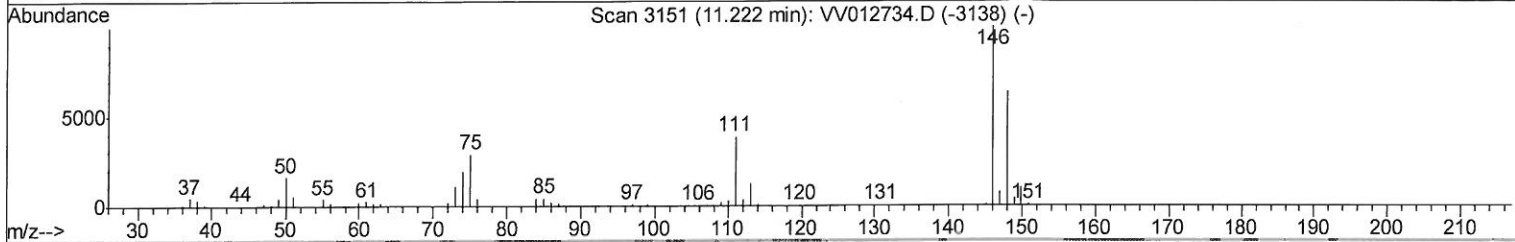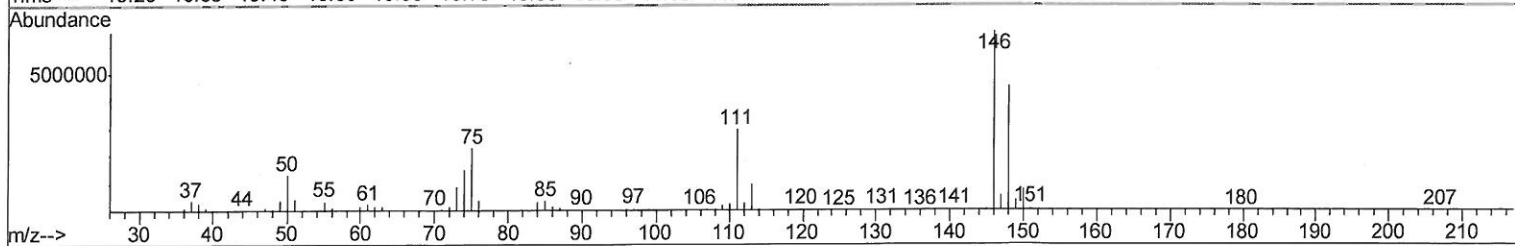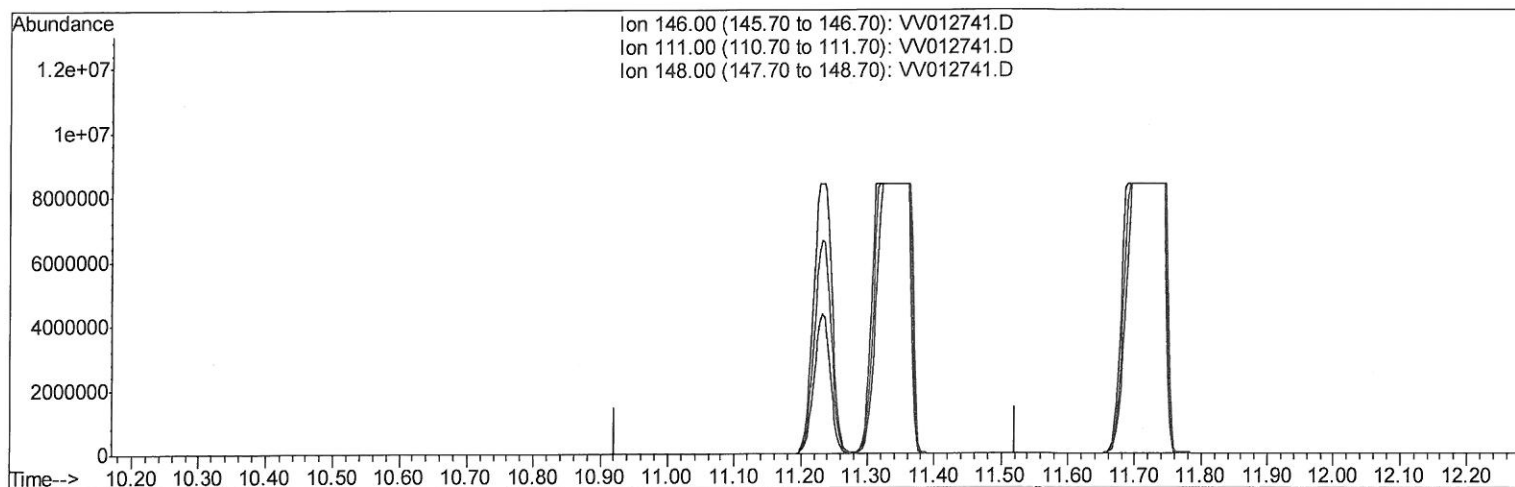

(62) 1,3-Dichlorobenzene (T)

11.222min (-11.222) 0.00ug/L

response 0

Ion	Exp%	Act%
146.00	100	0.00
111.00	38.90	0.00#
148.00	64.60	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

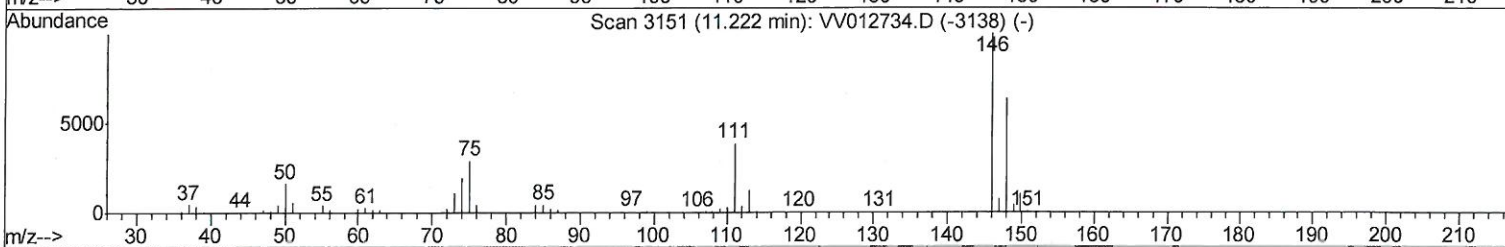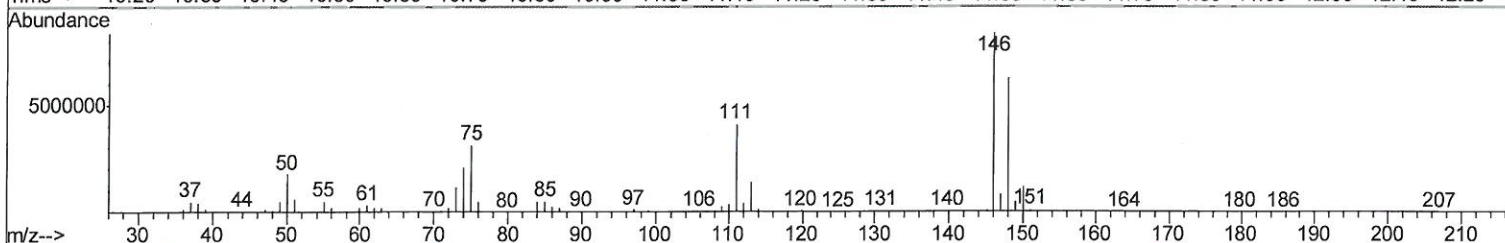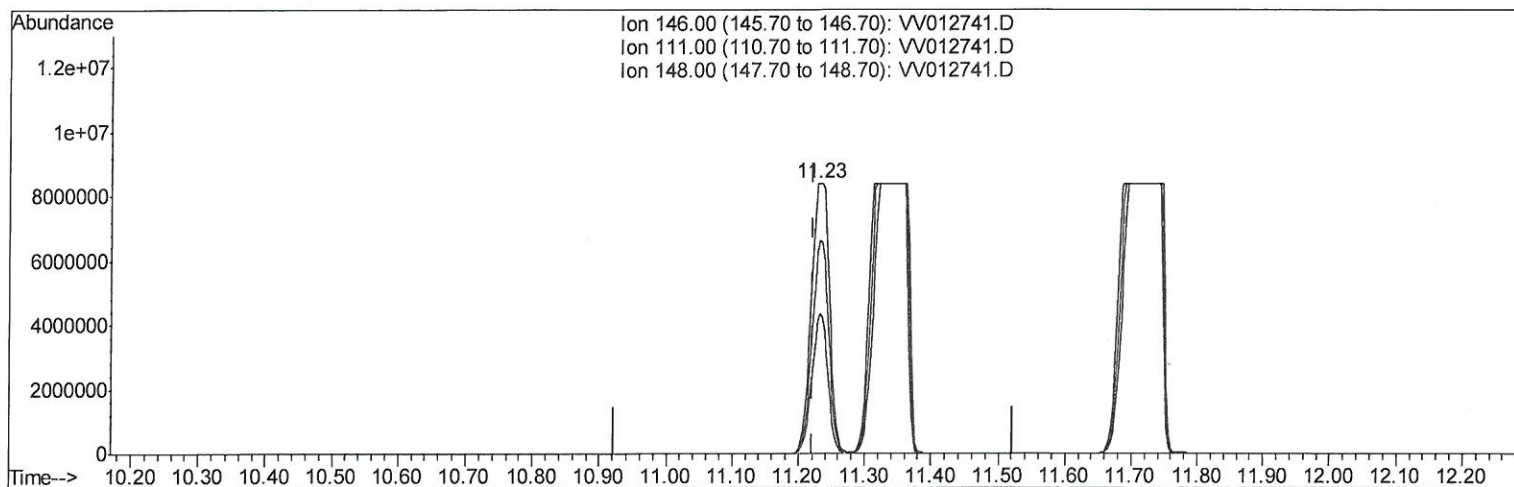

TIC: VV012741.D

(62) 1,3-Dichlorobenzene (T)

11.228min (+0.006) 1065.77ug/L m

response 16189175

Ion	Exp%	Act%
146.00	100	100
111.00	38.90	48.95
148.00	64.60	74.70
0.00	0.00	0.00

SYMD
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

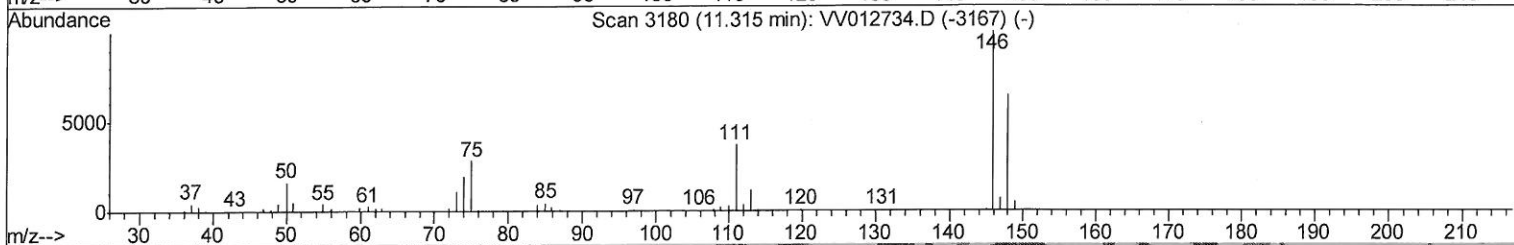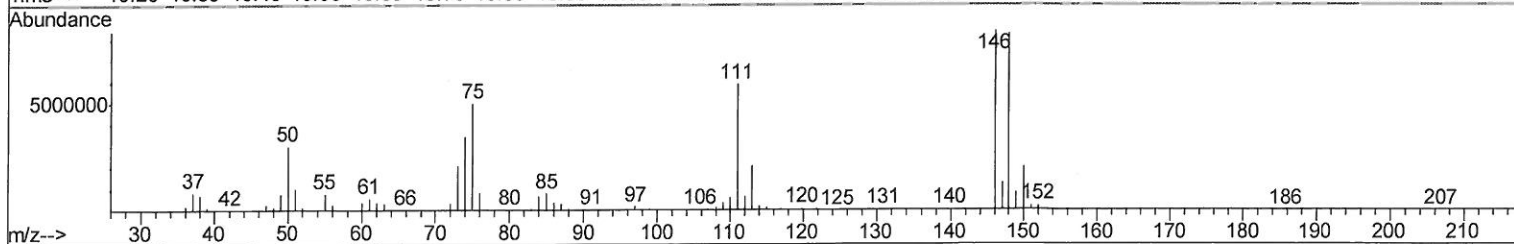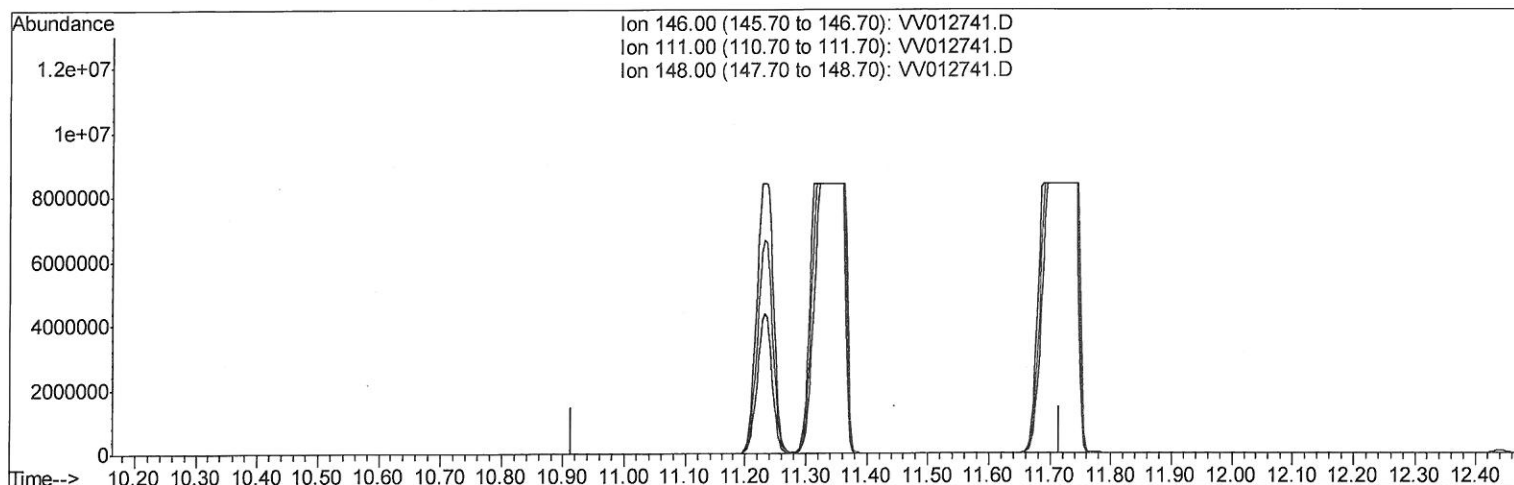

TIC: VV012741.D

(63) 1,4-Dichlorobenzene (T)

11.315min (-11.315) 0.00ug/L

response 0

Ion	Exp%	Act%
146.00	100	0.00
111.00	37.50	0.00#
148.00	64.30	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

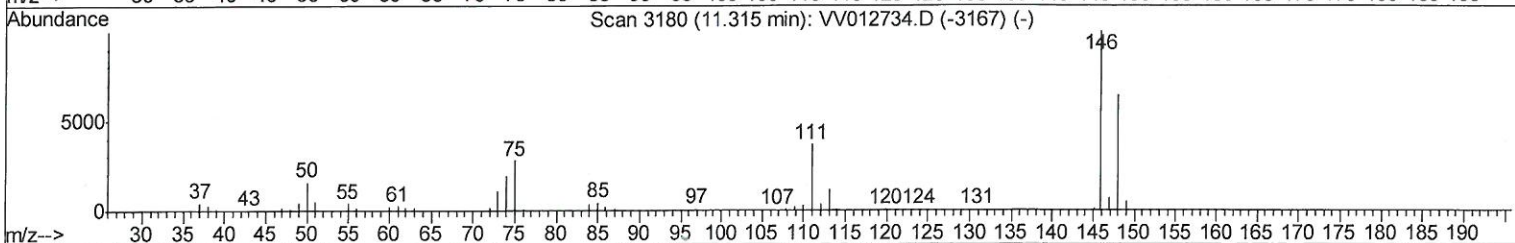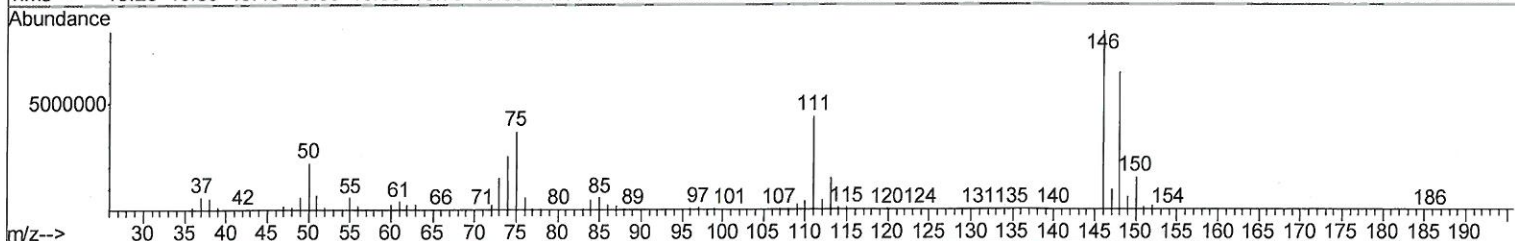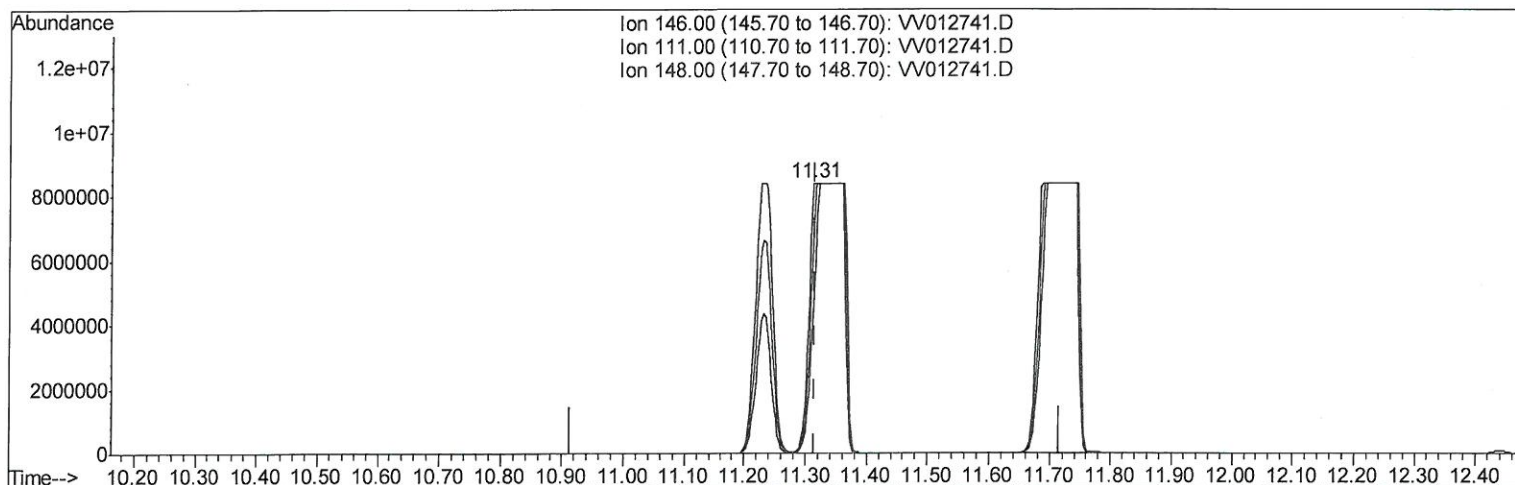

TIC: VV012741.D

(63) 1,4-Dichlorobenzene (T)

11.312min (-0.003) 2119.85ug/L m

response 33030905

Ion	Exp%	Act%
146.00	100	100
111.00	37.50	52.30#
148.00	64.30	76.90
0.00	0.00	0.00

2mD
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

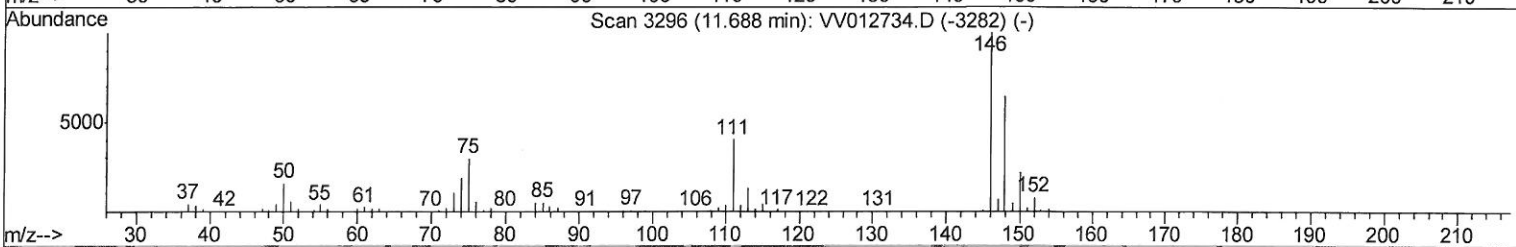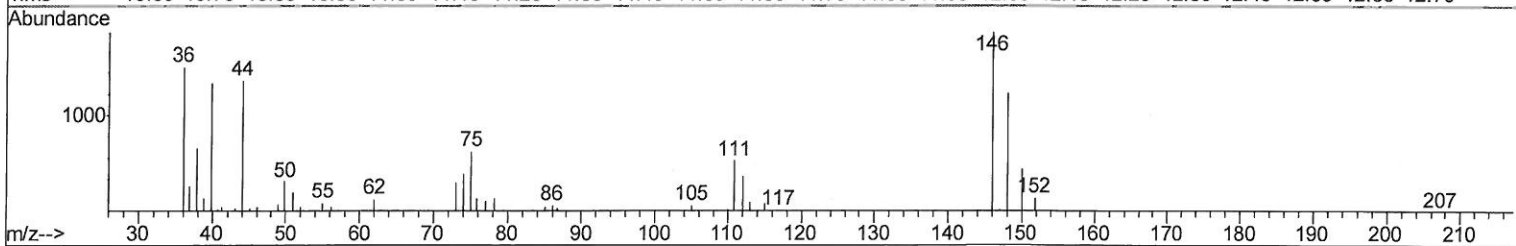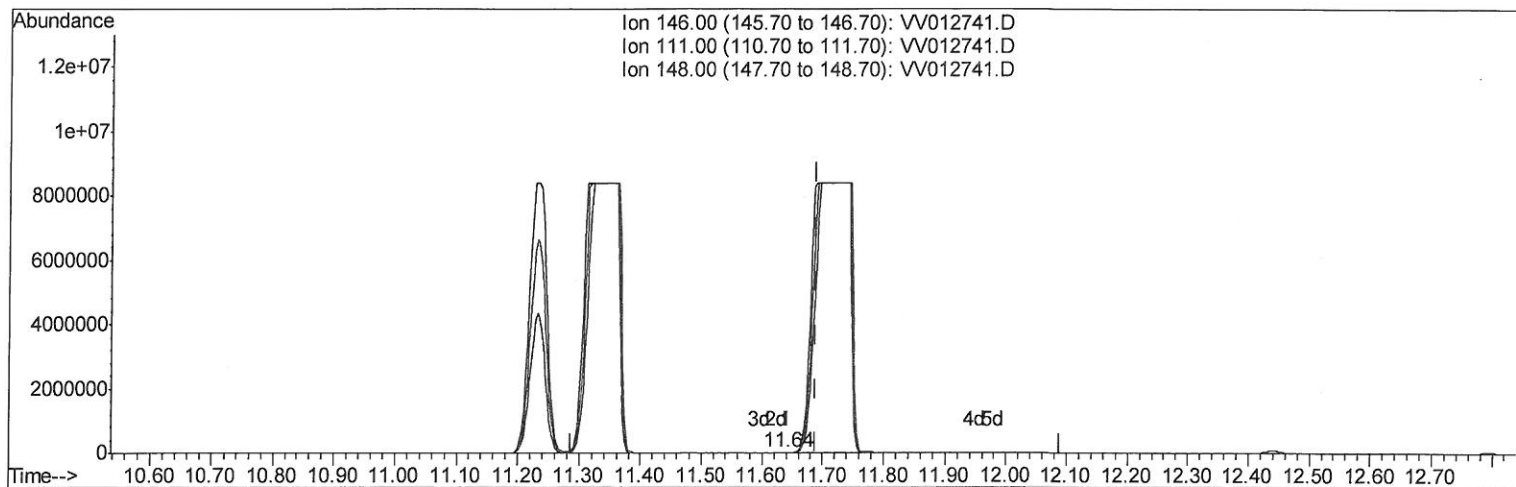

TIC: VV012741.D

(65) 1,2-Dichlorobenzene (T)

11.640min (-0.048) 0.00ug/L

response 47

Ion	Exp%	Act%
146.00	100	100
111.00	40.20	32.08#
148.00	64.40	67.98
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

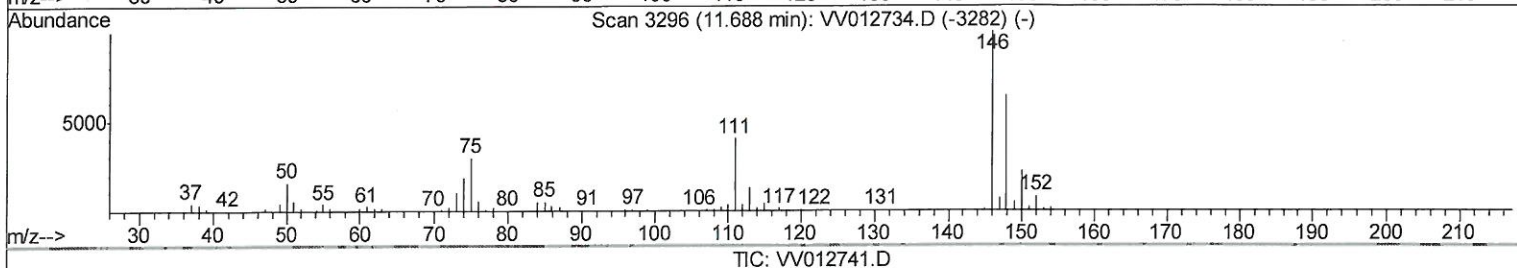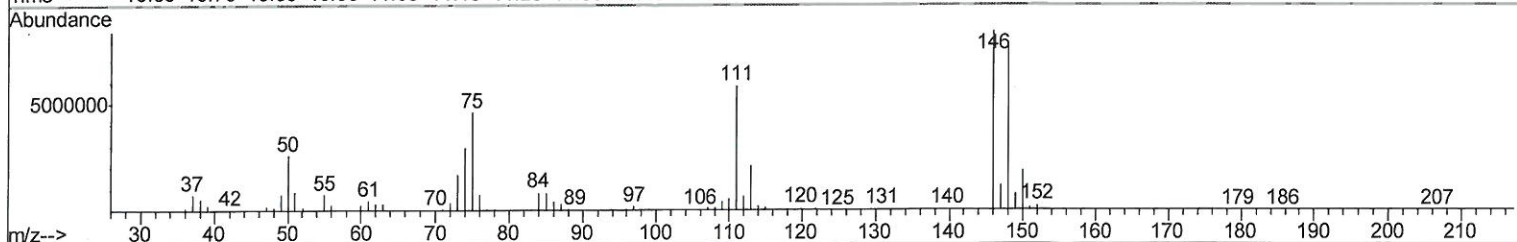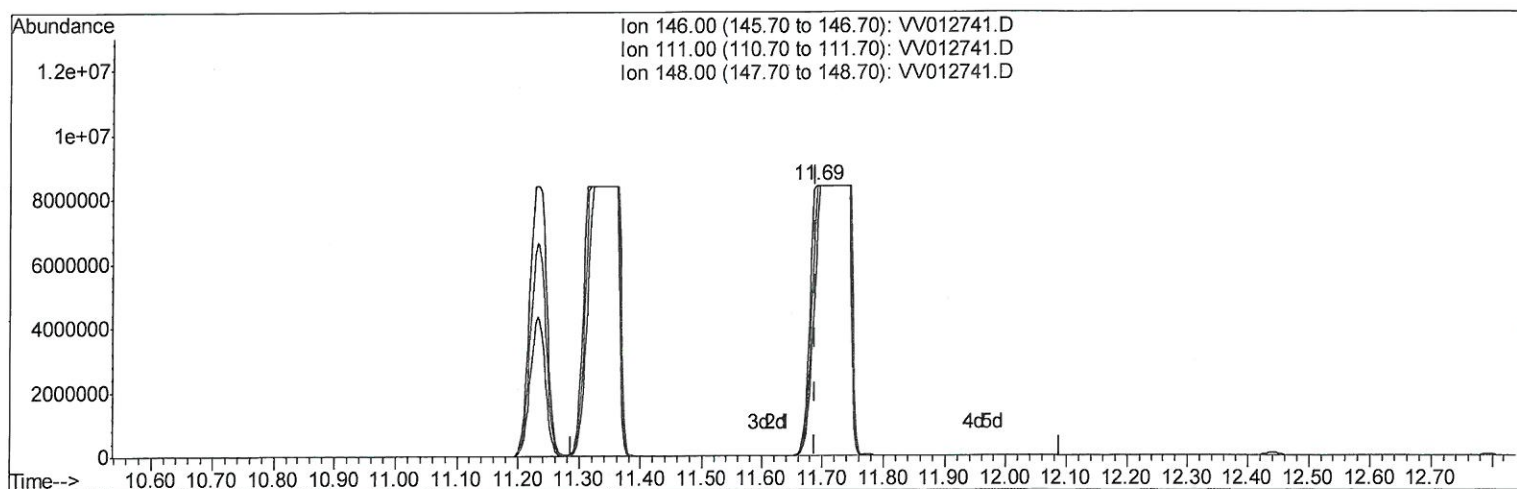

(65) 1,2-Dichlorobenzene (T)

11.688min (+0.000) 2315.91ug/L m

response 36989053

Ion	Exp%	Act%
146.00	100	100
111.00	40.20	69.18#
148.00	64.40	93.13#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

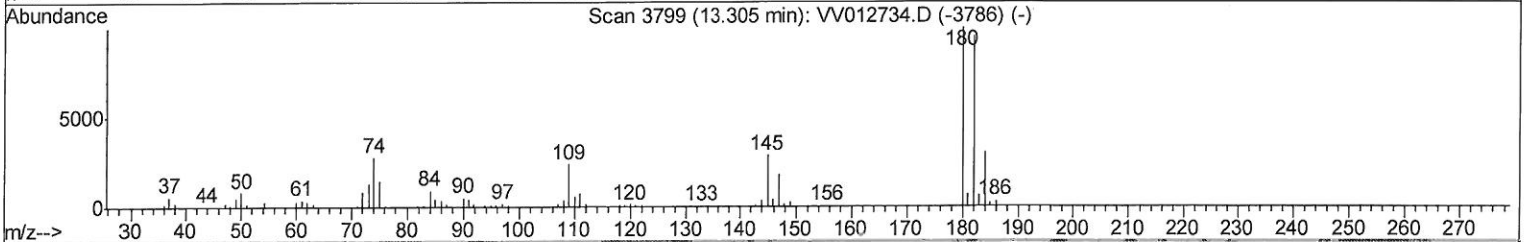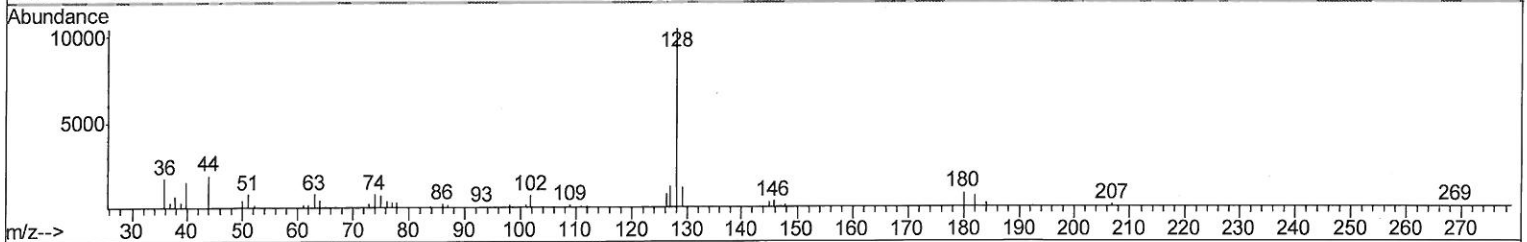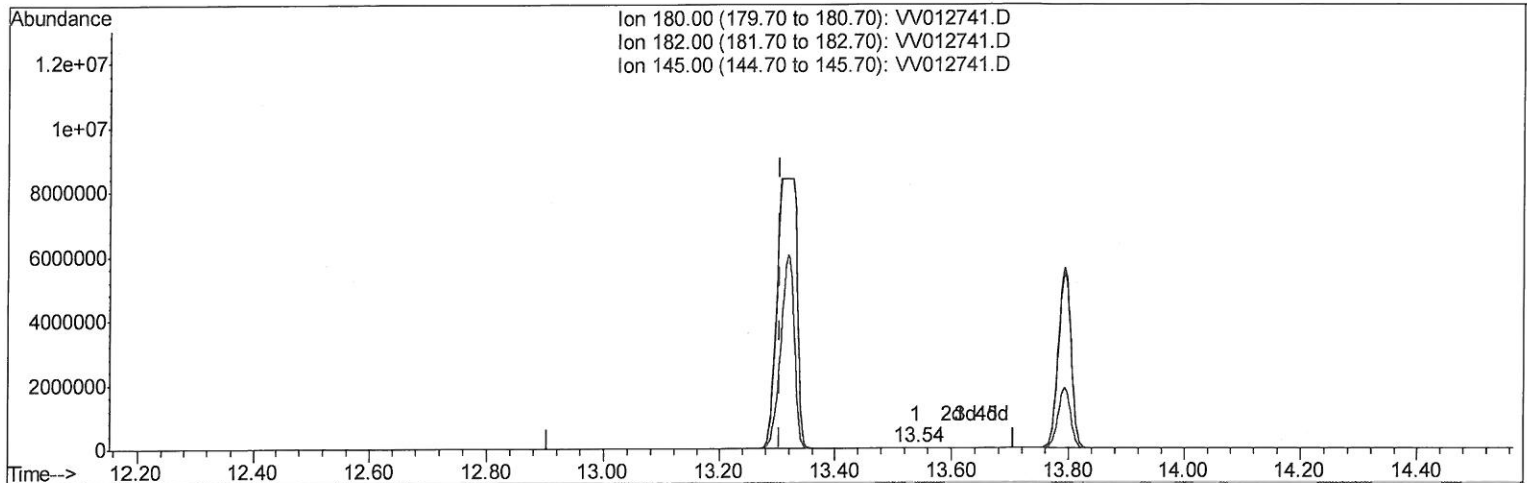

TIC: VV012741.D

(68) 1,2,4-trichlorobenzene (T)

13.540min (+0.235) 0.02ug/L

response 236

Ion	Exp%	Act%
180.00	100	100
182.00	96.00	86.86
145.00	28.70	28.81
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (Qedit)




Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 00:23:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

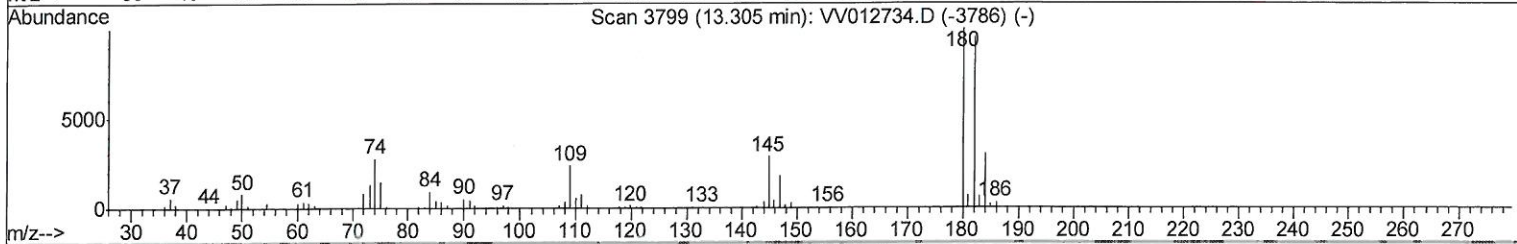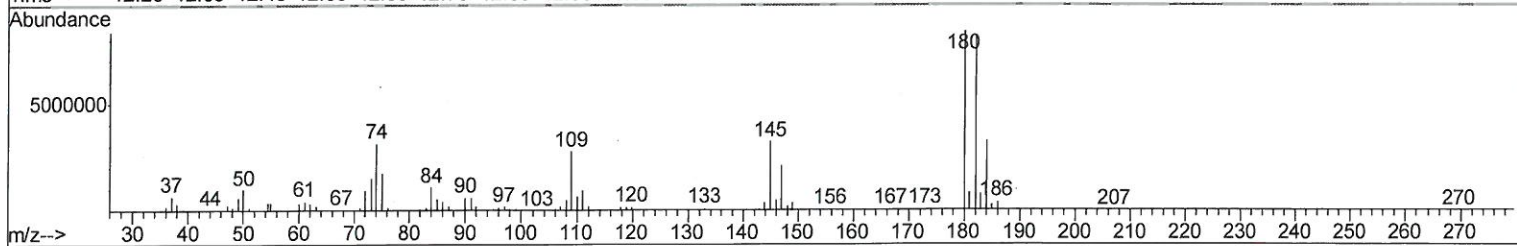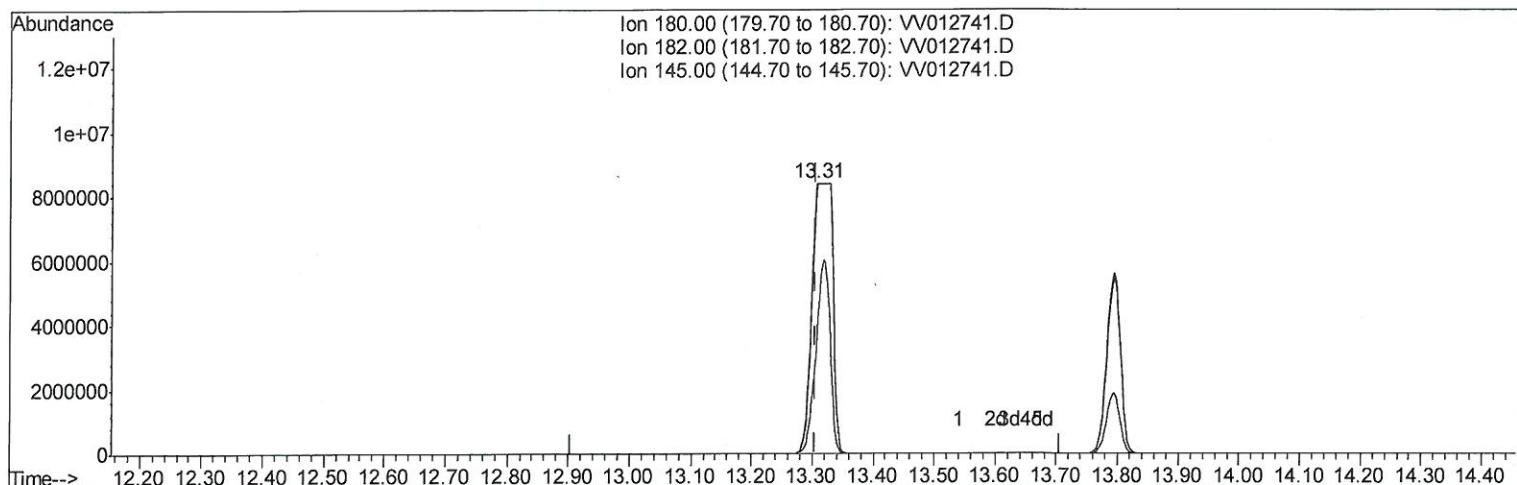

TIC: VV012741.D

(68) 1,2,4-trichlorobenzene (T)

13.305min (+0.000) 2092.59ug/L m

response 19841430

Ion Exp% Act%

180.00 100 100

182.00 96.00 0.00#

145.00 28.70 0.00#

0.00 0.00 0.00

7 MD
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\

Quantitation Report (QT Reviewed)

Data File : VV012741.D

Acq On : 13 Sep 2019 21:33

Operator : SY/MD

Sample : K4707-04

Misc : 5.0mL/MSVOA_V/WATER

ALS Vial : 21 Sample Multiplier: 1

Instrument :

MSVOA_V

ClientSampleId :

C0CJ5

Manual Integrations

APPROVED

MMDadoda

9/16/2019 1:22:25 PM

Quant Time: Sep 14 01:40:13 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M

Quant Title : VOC Analysis

QLast Update : Sat Sep 14 00:19:14 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	773195	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.92	117	807937	50.00	ug/L	0.03
60) 1,4-Dichlorobenzene-d4	11.31	152	491789	50.00	ug/L	0.02

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	202708	46.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.52%
7) Chloroethane-d5	1.58	69	189699	48.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.74%
11) 1,1-Dichloroethene-d2	2.13	63	303650	35.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.24%
21) 2-Butanone-d5	3.92	46	467622	102.90	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.90%
24) Chloroform-d	4.40	84	571353	52.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.24%
26) 1,2-Dichloroethane-d4	5.09	65	331874	50.39	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.78%
32) Benzene-d6	5.10	84	987337	45.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.58%
36) 1,2-Dichloropropane-d6	6.12	67	345850m	45.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.92%
41) Toluene-d8	7.36	98	876743	44.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.90%
43) trans-1,3-Dichloropropene-	7.66	79	143399	45.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.48%
47) 2-Hexanone-d5	8.13	63	324936	111.32	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	111.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	531010	54.56	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	109.12%
64) 1,2-Dichlorobenzene-d4	11.70	152	540479	48.15	ug/L	0.03
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.30%

7 MD
9/30/19

Target Compounds

Targets	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.19	43	64463	17.185	ug/L	99
25) Chloroform	4.42	83	1471569	145.460	ug/L	100
29) Cyclohexane	4.73	56	39513	5.152	ug/L	95
31) Carbon tetrachloride	4.88	117	472024	64.891	ug/L	99
33) Benzene	5.13	78	34454113m	1567.784	ug/L	
35) Methylcyclohexane	6.18	83	18032m	2.238	ug/L	
38) Bromodichloromethane	6.56	83	14029	1.724	ug/L	# 93
46) Tetrachloroethene	8.02	164	8813	1.989	ug/L	97
51) Chlorobenzene	8.92	112	43517174m	2783.092	ug/L	
62) 1,3-Dichlorobenzene	11.23	146	16189175m	1065.767	ug/L	
63) 1,4-Dichlorobenzene	11.31	146	33030905m	2119.853	ug/L	
65) 1,2-Dichlorobenzene	11.69	146	36989053m	2315.914	ug/L	
67) 1,3,5-Trichlorobenzene	12.69	180	22335	1.990	ug/L	99
68) 1,2,4-trichlorobenzene	13.31	180	19841430m	2092.590	ug/L	
70) 1,2,3-Trichlorobenzene	13.79	180	8784519	853.464	ug/L	97

MD
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Quantitation Report (QT Reviewed)
Data File : VV012741.D
Acq On : 13 Sep 2019 21:33
Operator : SY/MD
Sample : K4707-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ5

Manual Integrations
APPROVED

MMDadoda
9/16/2019 1:22:25 PM

Quant Time: Sep 14 01:40:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 14 00:19:14 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed