

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012735.D
 Acq On : 13 Sep 2019 19:07
 Operator : SY/MD
 Sample : VV0913WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	324270	319305	10.74%	1.371%
2	1.576	144	151	165	rVB	286872	334838	11.26%	1.438%
3	2.129	313	323	336	rBV	573069	805600	27.10%	3.460%
4	2.444	417	421	423	rBV5	908	866	0.03%	0.004%
5	2.457	423	425	428	rVV2	964	622	0.02%	0.003%
6	2.531	441	448	457	rVB3	4872	7780	0.26%	0.033%
7	2.650	473	485	502	rVB	10321	21602	0.73%	0.093%
8	2.795	522	530	534	rBV8	3019	4370	0.15%	0.019%
9	2.852	546	548	554	rVB5	707	675	0.02%	0.003%
10	3.084	615	620	625	rBV8	1306	1329	0.04%	0.006%
11	3.113	625	629	632	rBV3	944	777	0.03%	0.003%
12	3.155	639	642	644	rBV3	978	593	0.02%	0.003%
13	3.177	646	649	654	rVB4	1129	745	0.03%	0.003%
14	3.222	658	663	665	rBV4	933	863	0.03%	0.004%
15	3.338	695	699	708	rBV5	776	1007	0.03%	0.004%
16	3.431	725	728	730	rBV2	948	607	0.02%	0.003%
17	3.785	831	838	843	rBV8	1136	1427	0.05%	0.006%
18	3.836	849	854	857	rBV3	774	578	0.02%	0.002%
19	3.923	865	881	915	rBV	313048	842286	28.33%	3.617%
20	4.216	970	972	977	rBV5	849	603	0.02%	0.003%
21	4.341	1007	1011	1012	rBV2	1109	771	0.03%	0.003%
22	4.399	1012	1029	1052	rVV	513868	1251903	42.11%	5.376%
23	4.595	1086	1090	1092	rBV4	985	749	0.03%	0.003%
24	4.653	1105	1108	1110	rBV3	1290	796	0.03%	0.003%
25	4.711	1123	1126	1128	rBV3	1394	883	0.03%	0.004%
26	4.913	1187	1189	1197	rVB6	738	847	0.03%	0.004%
27	5.003	1214	1217	1219	rBV3	906	697	0.02%	0.003%
28	5.094	1224	1245	1281	rBV2	1161897	2972901	100.00%	12.768%
29	5.454	1354	1357	1360	rVB4	1181	741	0.02%	0.003%
30	5.573	1392	1394	1400	rVB6	1241	837	0.03%	0.004%
31	5.663	1405	1422	1451	rBV	990978	1944403	65.40%	8.350%
32	5.946	1495	1510	1526	rBV	137962	283861	9.55%	1.219%
33	6.116	1548	1563	1591	rBV	740581	1485354	49.96%	6.379%
34	6.618	1715	1719	1721	rBV3	1223	886	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012735.D
 Acq On : 13 Sep 2019 19:07
 Operator : SY/MD
 Sample : VV0913WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	6.647	1721	1728	1736	rBV6	5980	10534	0.35%	0.045%
36	6.788	1766	1772	1776	rBV7	769	900	0.03%	0.004%
37	6.865	1789	1796	1803	rVV5	1322	2076	0.07%	0.009%
38	7.026	1834	1846	1868	rVV	365008	650289	21.87%	2.793%
39	7.177	1888	1893	1897	rBV7	2880	3082	0.10%	0.013%
40	7.357	1935	1949	1969	rBV	1304009	2261356	76.07%	9.712%
41	7.663	2033	2044	2067	rVV	251513	432384	14.54%	1.857%
42	7.782	2079	2081	2085	rVB2	1066	557	0.02%	0.002%
43	7.884	2110	2113	2120	rVB7	2072	2341	0.08%	0.010%
44	8.084	2171	2175	2178	rBV4	887	669	0.02%	0.003%
45	8.129	2178	2189	2233	rBV2	778327	1685259	56.69%	7.238%
46	8.518	2308	2310	2313	rBV3	783	549	0.02%	0.002%
47	8.585	2329	2331	2332	rBV2	1196	572	0.02%	0.002%
48	8.650	2346	2351	2353	rBV3	1373	1200	0.04%	0.005%
49	8.685	2359	2362	2364	rBV3	1217	722	0.02%	0.003%
50	8.743	2376	2380	2383	rBV4	791	744	0.03%	0.003%
51	8.788	2392	2394	2399	rBV3	475	557	0.02%	0.002%
52	8.894	2411	2427	2455	rBV	1464315	2364678	79.54%	10.155%
53	9.187	2509	2518	2526	rBV5	4329	7629	0.26%	0.033%
54	9.235	2530	2533	2537	rVB4	860	653	0.02%	0.003%
55	9.486	2607	2611	2613	rBV3	772	562	0.02%	0.002%
56	9.515	2617	2620	2625	rBV4	1019	644	0.02%	0.003%
57	9.592	2634	2644	2645	rBV7	3456	4790	0.16%	0.021%
58	9.666	2663	2667	2672	rBV6	590	630	0.02%	0.003%
59	9.691	2672	2675	2679	rVB4	943	806	0.03%	0.003%
60	9.765	2694	2698	2700	rBV4	1041	638	0.02%	0.003%
61	9.778	2700	2702	2706	rVB3	1070	616	0.02%	0.003%
62	9.945	2750	2754	2757	rBV4	979	925	0.03%	0.004%
63	9.971	2757	2762	2772	rVB7	3193	5076	0.17%	0.022%
64	10.039	2777	2783	2785	rBV3	881	986	0.03%	0.004%
65	10.071	2789	2793	2794	rBV3	968	641	0.02%	0.003%
66	10.190	2827	2830	2834	rBV3	779	552	0.02%	0.002%
67	10.257	2839	2851	2866	rBV	872995	1360495	45.76%	5.843%
68	10.363	2880	2884	2889	rBV5	951	856	0.03%	0.004%
69	10.421	2898	2902	2903	rBV2	1297	937	0.03%	0.004%
70	10.450	2909	2911	2920	rVB6	1586	1047	0.04%	0.004%
71	10.550	2938	2942	2945	rBV4	1171	1031	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012735.D
 Acq On : 13 Sep 2019 19:07
 Operator : SY/MD
 Sample : VV0913WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	10.585	2945	2953	2961	rVB8	3786	5467	0.18%	0.023%
73	10.624	2961	2965	2966	rBV2	788	641	0.02%	0.003%
74	10.682	2980	2983	2987	rVB3	894	727	0.02%	0.003%
75	10.900	3045	3051	3054	rVB3	1232	986	0.03%	0.004%
76	10.958	3059	3069	3075	rBV5	3664	5147	0.17%	0.022%
77	11.122	3116	3120	3121	rBV3	980	656	0.02%	0.003%
78	11.228	3143	3153	3160	rBV9	4690	7820	0.26%	0.034%
79	11.293	3160	3173	3194	rBV	1221317	1884457	63.39%	8.093%
80	11.482	3230	3232	3238	rVB7	1460	1130	0.04%	0.005%
81	11.576	3257	3261	3264	rVB4	871	797	0.03%	0.003%
82	11.669	3275	3290	3318	rBV	1417585	2225579	74.86%	9.558%
83	11.929	3369	3371	3375	rVB2	862	561	0.02%	0.002%
84	12.158	3438	3442	3445	rBV3	551	586	0.02%	0.003%
85	12.286	3477	3482	3487	rBV7	1051	1421	0.05%	0.006%
86	12.405	3513	3519	3525	rBV4	1322	1933	0.07%	0.008%
87	12.453	3529	3534	3535	rVV4	813	784	0.03%	0.003%
88	12.476	3539	3541	3546	rVB5	1401	1142	0.04%	0.005%
89	12.537	3557	3560	3566	rVB5	769	638	0.02%	0.003%
90	12.604	3578	3581	3584	rBV3	690	607	0.02%	0.003%
91	12.691	3601	3608	3609	rBV5	5340	5062	0.17%	0.022%
92	12.736	3619	3622	3626	rBV4	1002	851	0.03%	0.004%
93	12.997	3699	3703	3704	rBV3	831	668	0.02%	0.003%
94	13.312	3793	3801	3812	rBV7	6425	10834	0.36%	0.047%
95	13.357	3813	3815	3818	rVB2	1179	675	0.02%	0.003%
96	13.556	3869	3877	3889	rBV4	6396	12288	0.41%	0.053%
97	13.794	3944	3951	3958	rBV7	5718	8946	0.30%	0.038%
98	14.003	4013	4016	4021	rBV4	901	832	0.03%	0.004%
99	14.084	4034	4041	4047	rBV7	1898	2688	0.09%	0.012%
100	14.222	4081	4084	4087	rBV4	1020	869	0.03%	0.004%


Sum of corrected areas: 23284877

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
Data File : VV012735.D
Acq On : 13 Sep 2019 19:07
Operator : SY/MD
Sample : VV0913WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

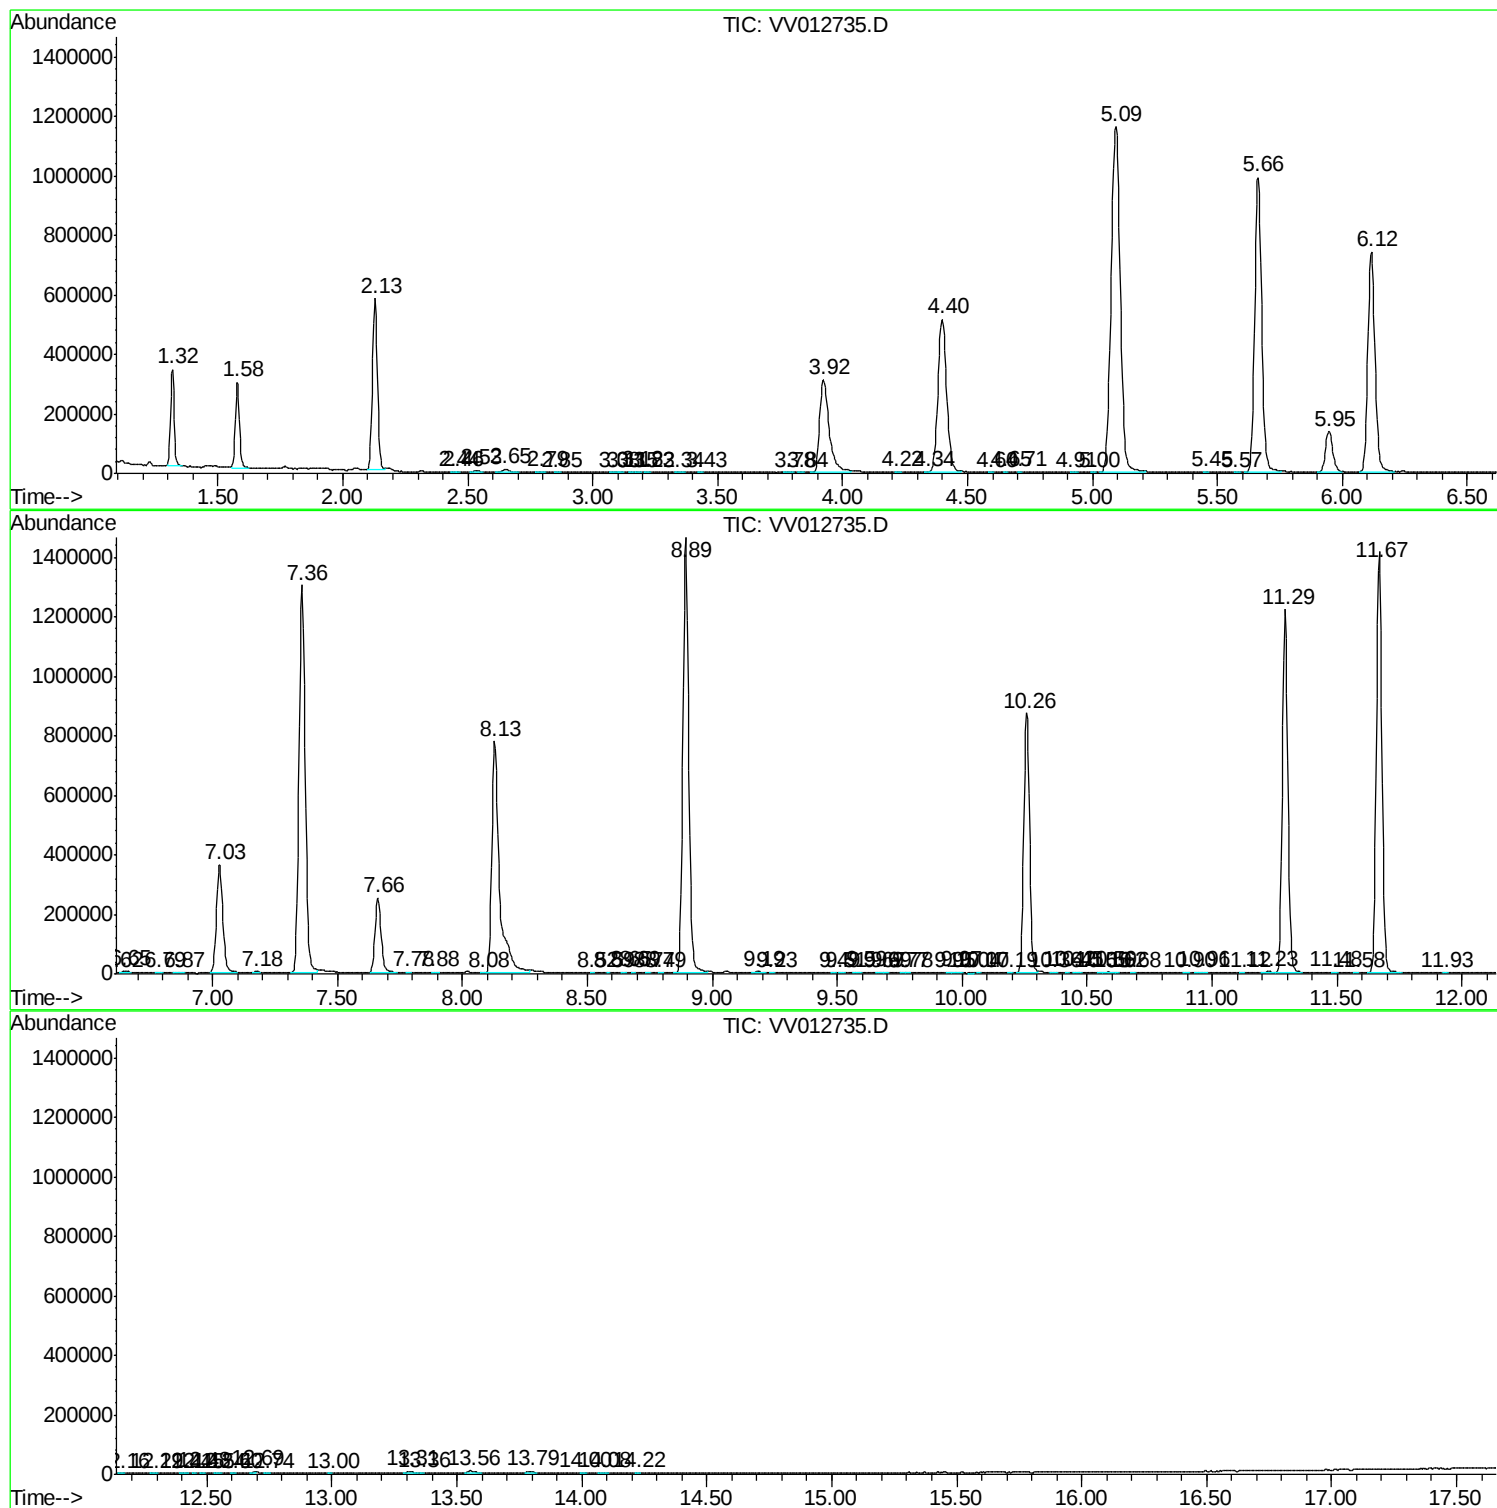

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091319\
Data File : VV012735.D
Acq On : 13 Sep 2019 19:07
Operator : SY/MD
Sample : VV0913WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091319\
Data File : VV012735.D
Acq On : 13 Sep 2019 19:07
Operator : SY/MD
Sample : VV0913WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc