

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012736.D
 Acq On : 13 Sep 2019 19:31
 Operator : SY/MD
 Sample : K4707-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	338365	336274	11.66%	1.546%
2	1.576	144	151	165	rVB	301825	345217	11.97%	1.587%
3	2.126	312	322	334	rBV	590503	834335	28.94%	3.835%
4	2.299	368	376	390	rBV	33526	58315	2.02%	0.268%
5	2.405	407	409	412	rVB3	1346	707	0.02%	0.003%
6	2.492	434	436	440	rVB3	1035	548	0.02%	0.003%
7	2.515	440	443	444	rBV2	1192	621	0.02%	0.003%
8	2.589	463	466	472	rVB6	1269	1028	0.04%	0.005%
9	2.650	472	485	501	rBV5	4342	10229	0.35%	0.047%
10	2.782	523	526	527	rBV3	1142	652	0.02%	0.003%
11	2.878	554	556	560	rVB4	1041	633	0.02%	0.003%
12	2.987	580	590	603	rBV4	7488	14586	0.51%	0.067%
13	3.167	644	646	658	rVV6	1080	1277	0.04%	0.006%
14	3.216	658	661	663	rVV3	870	609	0.02%	0.003%
15	3.286	679	683	689	rBV4	879	983	0.03%	0.005%
16	3.344	697	701	703	rVB3	1266	884	0.03%	0.004%
17	3.364	703	707	711	rBV3	896	850	0.03%	0.004%
18	3.505	746	751	754	rVB4	697	574	0.02%	0.003%
19	3.528	754	758	760	rBV4	1494	911	0.03%	0.004%
20	3.540	760	762	767	rVB3	1119	770	0.03%	0.004%
21	3.566	767	770	772	rBV2	940	645	0.02%	0.003%
22	3.601	778	781	787	rVB2	1053	1008	0.03%	0.005%
23	3.630	787	790	795	rBV2	719	882	0.03%	0.004%
24	3.868	859	864	868	rBV5	746	695	0.02%	0.003%
25	3.920	868	880	910	rBV	284228	742426	25.75%	3.413%
26	4.396	1010	1028	1052	rBV	504368	1226264	42.53%	5.637%
27	4.515	1063	1065	1072	rVB8	1845	1752	0.06%	0.008%
28	4.630	1097	1101	1103	rBV3	755	567	0.02%	0.003%
29	4.704	1121	1124	1128	rBV6	1262	1250	0.04%	0.006%
30	4.775	1143	1146	1149	rVB3	973	674	0.02%	0.003%
31	4.913	1187	1189	1195	rVB5	963	840	0.03%	0.004%
32	4.981	1207	1210	1216	rVB7	1480	1572	0.05%	0.007%
33	5.007	1216	1218	1220	rBV2	1359	641	0.02%	0.003%
34	5.093	1225	1245	1270	rBV2	1133641	2883425	100.00%	13.255%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012736.D
 Acq On : 13 Sep 2019 19:31
 Operator : SY/MD
 Sample : K4707-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	5.428	1344	1349	1354	rBV7	1701	2245	0.08%	0.010%
36	5.662	1407	1422	1452	rBV	888662	1758363	60.98%	8.083%
37	5.945	1496	1510	1527	rBV	147202	298001	10.33%	1.370%
38	6.116	1545	1563	1586	rBV	726360	1448045	50.22%	6.657%
39	6.405	1650	1653	1657	rBV5	916	702	0.02%	0.003%
40	6.431	1657	1661	1666	rVB6	1457	1383	0.05%	0.006%
41	6.489	1676	1679	1683	rVB3	976	733	0.03%	0.003%
42	6.515	1683	1687	1690	rBV2	1082	784	0.03%	0.004%
43	6.608	1709	1716	1717	rBV6	1569	1543	0.05%	0.007%
44	6.801	1772	1776	1778	rBV2	1011	566	0.02%	0.003%
45	6.839	1782	1788	1792	rVB3	872	646	0.02%	0.003%
46	7.026	1834	1846	1868	rBV	350708	623665	21.63%	2.867%
47	7.177	1886	1893	1907	rVB6	9129	18630	0.65%	0.086%
48	7.270	1919	1922	1928	rVB6	937	1007	0.03%	0.005%
49	7.357	1936	1949	1974	rBV	1267917	2198070	76.23%	10.104%
50	7.614	2026	2029	2031	rBV2	1065	678	0.02%	0.003%
51	7.659	2031	2043	2070	rVV	244751	422146	14.64%	1.941%
52	7.833	2095	2097	2099	rBV3	938	550	0.02%	0.003%
53	7.981	2134	2143	2150	rVV3	4511	7631	0.26%	0.035%
54	8.129	2178	2189	2220	rBV2	696737	1513885	52.50%	6.959%
55	8.447	2284	2288	2294	rBV6	1006	1064	0.04%	0.005%
56	8.524	2309	2312	2314	rBV3	827	644	0.02%	0.003%
57	8.614	2338	2340	2345	rBV4	663	674	0.02%	0.003%
58	8.649	2349	2351	2355	rVB3	917	553	0.02%	0.003%
59	8.733	2372	2377	2378	rBV3	903	772	0.03%	0.004%
60	8.894	2413	2427	2459	rBV	1283480	2096591	72.71%	9.638%
61	9.061	2473	2479	2484	rVB8	3049	3591	0.12%	0.017%
62	9.154	2504	2508	2509	rBV3	1605	1262	0.04%	0.006%
63	9.392	2578	2582	2586	rVV5	1009	721	0.03%	0.003%
64	9.540	2623	2628	2630	rBV3	1075	852	0.03%	0.004%
65	9.592	2633	2644	2647	rBV7	3049	4622	0.16%	0.021%
66	9.691	2672	2675	2678	rBV4	843	745	0.03%	0.003%
67	9.971	2752	2762	2769	rBV8	1631	2807	0.10%	0.013%
68	10.042	2781	2784	2785	rBV2	959	537	0.02%	0.002%
69	10.064	2785	2791	2794	rBV7	1867	2044	0.07%	0.009%
70	10.257	2837	2851	2871	rBV	795772	1252673	43.44%	5.758%
71	10.421	2895	2902	2908	rBV3	4653	6493	0.23%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012736.D
 Acq On : 13 Sep 2019 19:31
 Operator : SY/MD
 Sample : K4707-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	10.495	2920	2925	2930	rBV5	861	1002	0.03%	0.005%
73	10.575	2945	2950	2951	rBV4	2008	1368	0.05%	0.006%
74	10.778	3011	3013	3018	rVV3	930	715	0.02%	0.003%
75	10.842	3028	3033	3036	rBV5	923	825	0.03%	0.004%
76	10.897	3048	3050	3055	rVV3	796	621	0.02%	0.003%
77	10.919	3055	3057	3062	rVB2	713	554	0.02%	0.003%
78	10.958	3063	3069	3073	rBV6	2562	2857	0.10%	0.013%
79	11.055	3097	3099	3105	rBV5	971	799	0.03%	0.004%
80	11.225	3140	3152	3160	rBV5	4729	8744	0.30%	0.040%
81	11.292	3160	3173	3192	rBV	1013126	1553086	53.86%	7.139%
82	11.527	3242	3246	3253	rVB6	1210	1178	0.04%	0.005%
83	11.588	3254	3265	3274	rBV8	3271	6878	0.24%	0.032%
84	11.669	3274	3290	3311	rBV	1262642	1982785	68.76%	9.115%
85	11.884	3355	3357	3361	rVB3	1183	717	0.02%	0.003%
86	11.910	3362	3365	3367	rBV3	763	541	0.02%	0.002%
87	12.241	3465	3468	3472	rBV3	728	755	0.03%	0.003%
88	12.302	3479	3487	3492	rBV5	1548	1831	0.06%	0.008%
89	12.598	3574	3579	3581	rVV4	968	852	0.03%	0.004%
90	12.694	3602	3609	3617	rVB8	4315	6440	0.22%	0.030%
91	12.730	3618	3620	3624	rVB3	1041	635	0.02%	0.003%
92	12.826	3647	3650	3659	rVB5	1355	1392	0.05%	0.006%
93	12.926	3678	3681	3683	rBV2	1126	709	0.02%	0.003%
94	13.305	3789	3799	3800	rBV8	4860	5162	0.18%	0.024%
95	13.427	3833	3837	3839	rBV4	1529	1210	0.04%	0.006%
96	13.550	3869	3875	3888	rBV2	6870	12276	0.43%	0.056%
97	13.791	3943	3950	3962	rBV8	4735	9120	0.32%	0.042%
98	13.990	4010	4012	4015	rBV3	704	523	0.02%	0.002%
99	14.038	4022	4027	4029	rBV2	1171	947	0.03%	0.004%
100	15.308	4420	4422	4425	rBV2	1193	671	0.02%	0.003%


Sum of corrected areas: 21753755

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
Data File : VV012736.D
Acq On : 13 Sep 2019 19:31
Operator : SY/MD
Sample : K4707-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

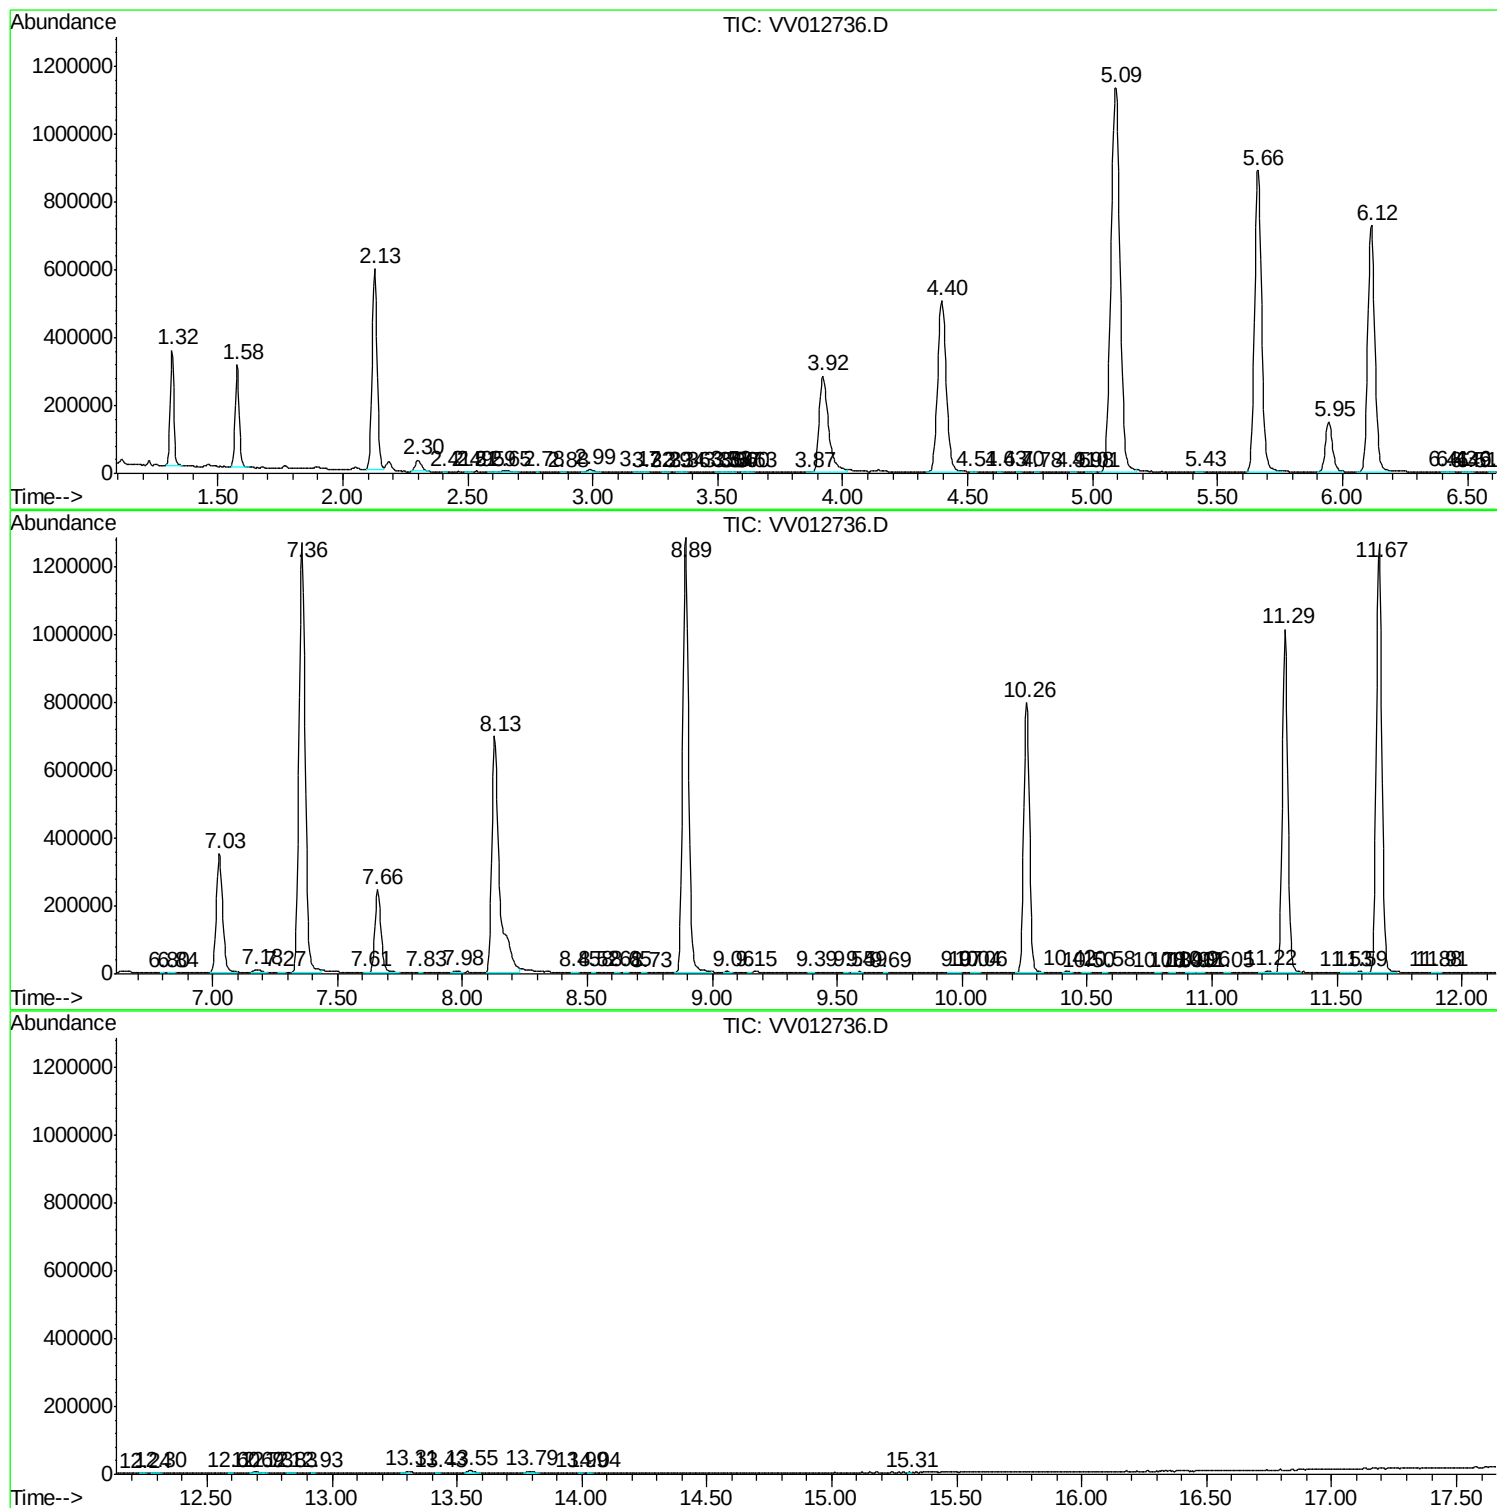

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091319\
Data File : VV012736.D
Acq On : 13 Sep 2019 19:31
Operator : SY/MD
Sample : K4707-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091319\
Data File : VV012736.D
Acq On : 13 Sep 2019 19:31
Operator : SY/MD
Sample : K4707-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
