

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012740.D
 Acq On : 13 Sep 2019 21:09
 Operator : SY/MD
 Sample : K4707-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rVB	339514	337180	11.35%	1.501%
2	1.579	144	152	170	rVB	304282	353692	11.90%	1.574%
3	2.129	313	323	335	rBV	600482	840146	28.28%	3.740%
4	2.303	367	377	393	rBV	31881	59502	2.00%	0.265%
5	2.457	423	425	427	rBV2	1025	629	0.02%	0.003%
6	2.650	473	485	499	rBV	71051	147365	4.96%	0.656%
7	2.759	517	519	523	rVB3	1443	1025	0.03%	0.005%
8	2.791	523	529	530	rBV5	2059	1847	0.06%	0.008%
9	2.994	578	592	605	rBV3	8577	19676	0.66%	0.088%
10	3.061	610	613	617	rVV4	683	634	0.02%	0.003%
11	3.203	653	657	661	rVB5	1398	1436	0.05%	0.006%
12	3.225	661	664	667	rBV3	1161	705	0.02%	0.003%
13	3.306	686	689	692	rVV3	873	648	0.02%	0.003%
14	3.322	692	694	698	rVB2	1152	747	0.03%	0.003%
15	3.653	792	797	799	rVB2	823	652	0.02%	0.003%
16	3.695	803	810	813	rVV5	1053	964	0.03%	0.004%
17	3.926	865	882	928	rBV2	344826	1096265	36.90%	4.880%
18	4.399	1013	1029	1065	rVB2	540152	1476424	49.69%	6.572%
19	4.836	1162	1165	1168	rBV5	847	559	0.02%	0.002%
20	4.942	1195	1198	1205	rVB6	1310	1324	0.04%	0.006%
21	5.093	1224	1245	1291	rBV2	1164161	2971132	100.00%	13.225%
22	5.441	1345	1353	1361	rVB10	1685	3035	0.10%	0.014%
23	5.537	1380	1383	1388	rVB5	1127	957	0.03%	0.004%
24	5.576	1388	1395	1398	rBV6	2625	3452	0.12%	0.015%
25	5.663	1408	1422	1447	rBV	876106	1715751	57.75%	7.637%
26	5.946	1497	1510	1532	rBV	148957	303693	10.22%	1.352%
27	6.116	1545	1563	1588	rBV	737918	1484693	49.97%	6.609%
28	6.399	1643	1651	1656	rVB7	1311	1724	0.06%	0.008%
29	6.608	1709	1716	1720	rBV7	1615	2433	0.08%	0.011%
30	6.650	1720	1729	1740	rBV5	5137	11257	0.38%	0.050%
31	6.743	1756	1758	1764	rVB6	1220	901	0.03%	0.004%
32	6.788	1768	1772	1774	rVB3	1184	838	0.03%	0.004%
33	6.830	1783	1785	1793	rVB2	1306	1150	0.04%	0.005%
34	6.881	1793	1801	1803	rBV5	1021	1174	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012740.D
 Acq On : 13 Sep 2019 21:09
 Operator : SY/MD
 Sample : K4707-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	7.029	1833	1847	1865	rBV	354558	629106	21.17%	2.800%
36	7.180	1883	1894	1905	rBV	8224	17904	0.60%	0.080%
37	7.357	1936	1949	1966	rBV	1292579	2213531	74.50%	9.853%
38	7.662	2032	2044	2065	rBV	249321	427775	14.40%	1.904%
39	7.794	2081	2085	2089	rBV7	1293	1037	0.03%	0.005%
40	7.913	2121	2122	2130	rVB4	1710	1620	0.05%	0.007%
41	7.981	2130	2143	2151	rBV2	4654	10323	0.35%	0.046%
42	8.129	2176	2189	2202	rBV2	741500	1407947	47.39%	6.267%
43	8.518	2307	2310	2316	rVB6	1383	1494	0.05%	0.007%
44	8.582	2327	2330	2332	rBV3	961	685	0.02%	0.003%
45	8.666	2354	2356	2361	rVB6	1343	1066	0.04%	0.005%
46	8.839	2407	2410	2412	rBV4	782	570	0.02%	0.003%
47	8.894	2413	2427	2452	rBV	1263704	2051968	69.06%	9.134%
48	9.051	2473	2476	2478	rBV4	1700	1160	0.04%	0.005%
49	9.109	2487	2494	2498	rBV8	1376	1688	0.06%	0.008%
50	9.170	2507	2513	2522	rBV8	2686	4473	0.15%	0.020%
51	9.267	2540	2543	2547	rVB4	1259	919	0.03%	0.004%
52	9.338	2561	2565	2569	rVB5	628	566	0.02%	0.003%
53	9.367	2571	2574	2581	rBV6	795	1005	0.03%	0.004%
54	9.402	2583	2585	2592	rVB4	701	703	0.02%	0.003%
55	9.588	2639	2643	2646	rBV4	1436	1325	0.04%	0.006%
56	9.650	2657	2662	2663	rBV4	867	774	0.03%	0.003%
57	9.740	2687	2690	2692	rBV2	1285	852	0.03%	0.004%
58	9.775	2697	2701	2704	rVV3	779	601	0.02%	0.003%
59	9.929	2747	2749	2754	rVB2	981	688	0.02%	0.003%
60	9.961	2754	2759	2761	rBV4	1428	1299	0.04%	0.006%
61	10.096	2796	2801	2805	rBV5	626	721	0.02%	0.003%
62	10.132	2808	2812	2816	rVB5	994	766	0.03%	0.003%
63	10.164	2816	2822	2827	rBV5	832	1057	0.04%	0.005%
64	10.212	2833	2837	2838	rBV2	1035	581	0.02%	0.003%
65	10.257	2838	2851	2874	rVB	835869	1300887	43.78%	5.791%
66	10.344	2874	2878	2879	rBV2	939	633	0.02%	0.003%
67	10.418	2895	2901	2911	rVB2	4691	7109	0.24%	0.032%
68	10.588	2949	2954	2959	rBV7	906	973	0.03%	0.004%
69	10.678	2978	2982	2985	rBV3	572	578	0.02%	0.003%
70	10.807	3019	3022	3026	rBV4	761	565	0.02%	0.003%
71	10.849	3030	3035	3037	rBV3	663	634	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012740.D
 Acq On : 13 Sep 2019 21:09
 Operator : SY/MD
 Sample : K4707-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CJ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	11.003	3079	3083	3084	rBV3	798	587	0.02%	0.003%
73	11.170	3131	3135	3138	rVB4	834	609	0.02%	0.003%
74	11.199	3138	3144	3146	rBV4	1558	1443	0.05%	0.006%
75	11.215	3146	3149	3154	rVV5	776	846	0.03%	0.004%
76	11.293	3160	3173	3191	rBV	966353	1493095	50.25%	6.646%
77	11.492	3229	3235	3238	rBV7	984	1258	0.04%	0.006%
78	11.669	3277	3290	3309	rBV	1270182	2006402	67.53%	8.931%
79	11.820	3334	3337	3339	rVB4	1210	725	0.02%	0.003%
80	11.936	3369	3373	3375	rBV3	1498	966	0.03%	0.004%
81	11.952	3376	3378	3382	rVB3	1357	821	0.03%	0.004%
82	12.032	3401	3403	3409	rVB5	1117	604	0.02%	0.003%
83	12.138	3431	3436	3438	rBV2	862	831	0.03%	0.004%
84	12.276	3475	3479	3483	rVB4	923	616	0.02%	0.003%
85	12.299	3483	3486	3489	rBV4	770	560	0.02%	0.002%
86	12.694	3604	3609	3611	rBV3	1678	1538	0.05%	0.007%
87	12.746	3623	3625	3627	rVV3	1124	733	0.02%	0.003%
88	12.842	3651	3655	3658	rBV2	692	635	0.02%	0.003%
89	13.061	3721	3723	3727	rVB2	914	610	0.02%	0.003%
90	13.090	3727	3732	3735	rBV4	1087	1155	0.04%	0.005%
91	13.309	3792	3800	3801	rBV7	2596	2815	0.09%	0.013%
92	13.595	3887	3889	3893	rBV3	1001	718	0.02%	0.003%
93	13.675	3909	3914	3918	rBV7	1099	1241	0.04%	0.006%
94	13.749	3934	3937	3941	rBV3	1129	1055	0.04%	0.005%
95	13.794	3945	3951	3957	rBV7	2325	2989	0.10%	0.013%
96	13.952	3998	4000	4004	rBV3	848	617	0.02%	0.003%
97	14.299	4105	4108	4110	rBV4	1188	723	0.02%	0.003%
98	14.527	4176	4179	4182	rBV2	1010	774	0.03%	0.003%
99	14.656	4217	4219	4226	rBV5	977	703	0.02%	0.003%
100	15.138	4366	4369	4371	rBV3	1408	914	0.03%	0.004%


Sum of corrected areas: 22465776

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012740.D
Acq On : 13 Sep 2019 21:09
Operator : SY/MD
Sample : K4707-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0CJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

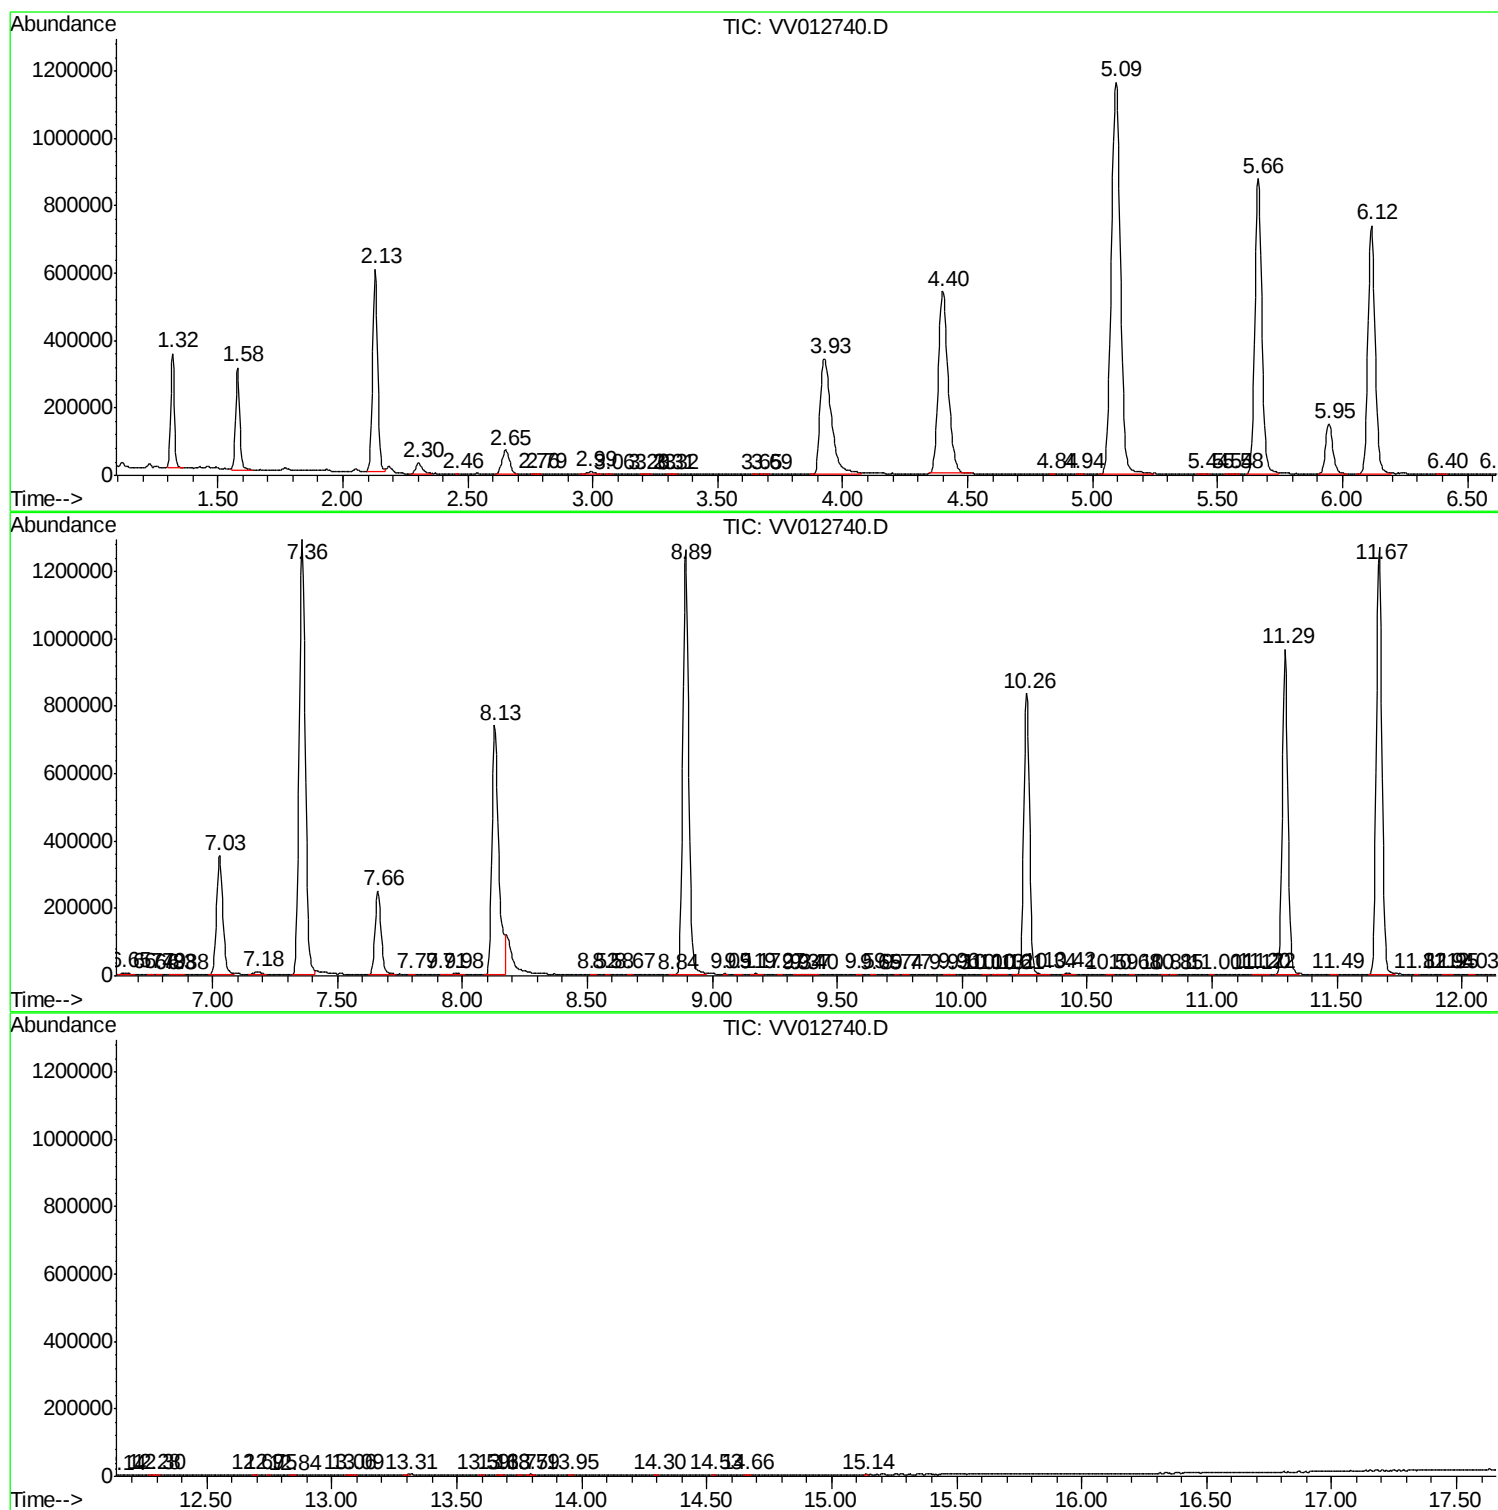

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012740.D
Acq On : 13 Sep 2019 21:09
Operator : SY/MD
Sample : K4707-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091319\
Data File : VV012740.D
Acq On : 13 Sep 2019 21:09
Operator : SY/MD
Sample : K4707-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0CJ4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
