

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012744.D
 Acq On : 13 Sep 2019 23:10
 Operator : SY/MD
 Sample : K4868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	334055	336903	11.27%	1.417%
2	1.579	144	152	163	rVB	290542	340842	11.40%	1.434%
3	2.129	313	323	336	rBV	570650	804676	26.91%	3.385%
4	2.302	368	377	391	rBV3	29742	56741	1.90%	0.239%
5	2.534	442	449	454	rBV7	3524	5144	0.17%	0.022%
6	2.650	472	485	503	rVB	26561	57275	1.92%	0.241%
7	2.778	522	525	526	rBV3	1665	897	0.03%	0.004%
8	2.794	526	530	535	rVB5	3158	3765	0.13%	0.016%
9	2.878	553	556	560	rBV4	953	739	0.02%	0.003%
10	3.061	610	613	616	rBV5	874	813	0.03%	0.003%
11	3.164	641	645	647	rBV3	893	721	0.02%	0.003%
12	3.499	745	749	751	rBV3	1286	795	0.03%	0.003%
13	3.550	762	765	772	rVB5	813	768	0.03%	0.003%
14	3.598	776	780	782	rBV2	1200	841	0.03%	0.004%
15	3.843	853	856	861	rVB3	808	887	0.03%	0.004%
16	3.923	868	881	918	rBV	315329	897093	30.00%	3.774%
17	4.286	990	994	997	rBV6	1193	1183	0.04%	0.005%
18	4.399	1007	1029	1061	rBV	518038	1261647	42.19%	5.308%
19	4.720	1119	1129	1130	rBV8	2297	2957	0.10%	0.012%
20	4.820	1156	1160	1162	rBV3	1188	1041	0.03%	0.004%
21	4.917	1186	1190	1192	rBV3	1118	819	0.03%	0.003%
22	5.007	1213	1218	1221	rBV3	851	742	0.02%	0.003%
23	5.093	1225	1245	1282	rBV2	1157895	2990580	100.00%	12.581%
24	5.380	1329	1334	1337	rBV6	1146	1118	0.04%	0.005%
25	5.505	1369	1373	1374	rBV2	1041	611	0.02%	0.003%
26	5.601	1399	1403	1407	rBV7	1189	1332	0.04%	0.006%
27	5.662	1407	1422	1449	rBV	942599	1876063	62.73%	7.893%
28	5.904	1492	1497	1498	rBV5	1246	1039	0.03%	0.004%
29	5.945	1498	1510	1530	rVV2	119712	244827	8.19%	1.030%
30	6.116	1548	1563	1593	rBV	727639	1468445	49.10%	6.178%
31	6.334	1627	1631	1634	rVB5	1252	906	0.03%	0.004%
32	6.354	1634	1637	1641	rVB5	1396	1036	0.03%	0.004%
33	6.376	1641	1644	1647	rBV3	1010	717	0.02%	0.003%
34	6.518	1685	1688	1693	rBV3	840	911	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012744.D
 Acq On : 13 Sep 2019 23:10
 Operator : SY/MD
 Sample : K4868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	6.650	1721	1729	1734	rBV4	5706	9373	0.31%	0.039%
36	6.749	1758	1760	1767	rVB5	1311	1076	0.04%	0.005%
37	6.868	1793	1797	1800	rVB4	956	736	0.02%	0.003%
38	7.029	1833	1847	1872	rBV	360971	648896	21.70%	2.730%
39	7.174	1886	1892	1897	rBV6	3140	4999	0.17%	0.021%
40	7.273	1916	1923	1936	rBV9	3211	5934	0.20%	0.025%
41	7.357	1936	1949	1967	rBV	1297897	2235810	74.76%	9.406%
42	7.662	2031	2044	2066	rBV	256745	436533	14.60%	1.836%
43	7.871	2106	2109	2110	rBV3	1383	785	0.03%	0.003%
44	7.884	2111	2113	2116	rVB3	1136	674	0.02%	0.003%
45	7.977	2137	2142	2148	rVV6	2205	2446	0.08%	0.010%
46	8.019	2148	2155	2164	rVB10	6903	11783	0.39%	0.050%
47	8.055	2164	2166	2173	rBV6	908	978	0.03%	0.004%
48	8.129	2177	2189	2231	rBV2	775707	1658619	55.46%	6.978%
49	8.720	2370	2373	2380	rBV3	722	743	0.02%	0.003%
50	8.836	2405	2409	2411	rBV3	1381	699	0.02%	0.003%
51	8.894	2411	2427	2454	rBV	1370085	2398378	80.20%	10.090%
52	9.058	2472	2478	2486	rVB2	7738	11486	0.38%	0.048%
53	9.125	2497	2499	2506	rVB6	1427	1551	0.05%	0.007%
54	9.183	2506	2517	2524	rBV5	7282	13285	0.44%	0.056%
55	9.389	2574	2581	2583	rBV6	648	645	0.02%	0.003%
56	9.502	2612	2616	2619	rVB2	936	692	0.02%	0.003%
57	9.534	2623	2626	2630	rBV2	1097	781	0.03%	0.003%
58	9.595	2632	2645	2649	rBV4	8882	16290	0.54%	0.069%
59	9.733	2684	2688	2691	rBV4	1679	1261	0.04%	0.005%
60	9.762	2694	2697	2700	rBV4	987	911	0.03%	0.004%
61	9.878	2730	2733	2736	rBV3	1124	966	0.03%	0.004%
62	9.977	2756	2764	2774	rVB5	7632	12377	0.41%	0.052%
63	10.193	2826	2831	2834	rBV6	641	756	0.03%	0.003%
64	10.257	2839	2851	2879	rVB	885820	1382602	46.23%	5.817%
65	10.415	2897	2900	2901	rBV3	1991	1055	0.04%	0.004%
66	10.585	2941	2953	2959	rBV2	7220	11741	0.39%	0.049%
67	10.775	3010	3012	3016	rBV2	959	628	0.02%	0.003%
68	10.891	3046	3048	3051	rVB2	1355	725	0.02%	0.003%
69	10.913	3051	3055	3056	rBV2	922	777	0.03%	0.003%
70	10.961	3061	3070	3079	rBV4	7646	12407	0.41%	0.052%
71	11.055	3096	3099	3104	rVV4	960	759	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012744.D
 Acq On : 13 Sep 2019 23:10
 Operator : SY/MD
 Sample : K4868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	11.225	3141	3152	3161	rBV2	27001	45389	1.52%	0.191%
73	11.292	3161	3173	3196	rVV2	1089307	1893469	63.31%	7.966%
74	11.508	3238	3240	3243	rVB3	1382	759	0.03%	0.003%
75	11.534	3246	3248	3253	rBV5	774	656	0.02%	0.003%
76	11.669	3275	3290	3311	rBV	1319306	2268603	75.86%	9.544%
77	11.845	3342	3345	3350	rBV6	1226	1180	0.04%	0.005%
78	11.868	3350	3352	3356	rVB4	1186	763	0.03%	0.003%
79	11.948	3376	3377	3380	rVV3	1303	723	0.02%	0.003%
80	11.964	3380	3382	3386	rVB3	1303	868	0.03%	0.004%
81	12.341	3497	3499	3502	rVB3	1121	672	0.02%	0.003%
82	12.366	3502	3507	3508	rBV2	876	788	0.03%	0.003%
83	12.469	3534	3539	3541	rBV4	1890	1601	0.05%	0.007%
84	12.559	3563	3567	3569	rBV3	1183	912	0.03%	0.004%
85	12.691	3600	3608	3619	rVV3	14451	23548	0.79%	0.099%
86	12.765	3628	3631	3634	rVB5	1131	949	0.03%	0.004%
87	12.797	3637	3641	3643	rBV3	748	619	0.02%	0.003%
88	12.980	3694	3698	3700	rBV3	1004	807	0.03%	0.003%
89	13.038	3713	3716	3721	rVB6	797	629	0.02%	0.003%
90	13.067	3721	3725	3731	rBV5	1159	1317	0.04%	0.006%
91	13.167	3752	3756	3758	rVB3	900	695	0.02%	0.003%
92	13.196	3762	3765	3770	rVB3	817	688	0.02%	0.003%
93	13.218	3770	3772	3779	rVB6	1142	793	0.03%	0.003%
94	13.263	3783	3786	3790	rBV3	1108	698	0.02%	0.003%
95	13.305	3790	3799	3815	rBV2	85912	138435	4.63%	0.582%
96	13.482	3850	3854	3858	rBV4	890	827	0.03%	0.003%
97	13.553	3863	3876	3890	rBV	29872	54089	1.81%	0.228%
98	13.720	3925	3928	3931	rBV5	966	696	0.02%	0.003%
99	13.791	3940	3950	3967	rVB2	41565	67519	2.26%	0.284%
100	15.447	4462	4465	4475	rVB10	4749	6399	0.21%	0.027%


Sum of corrected areas: 23770122

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012744.D
Acq On : 13 Sep 2019 23:10
Operator : SY/MD
Sample : K4868-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

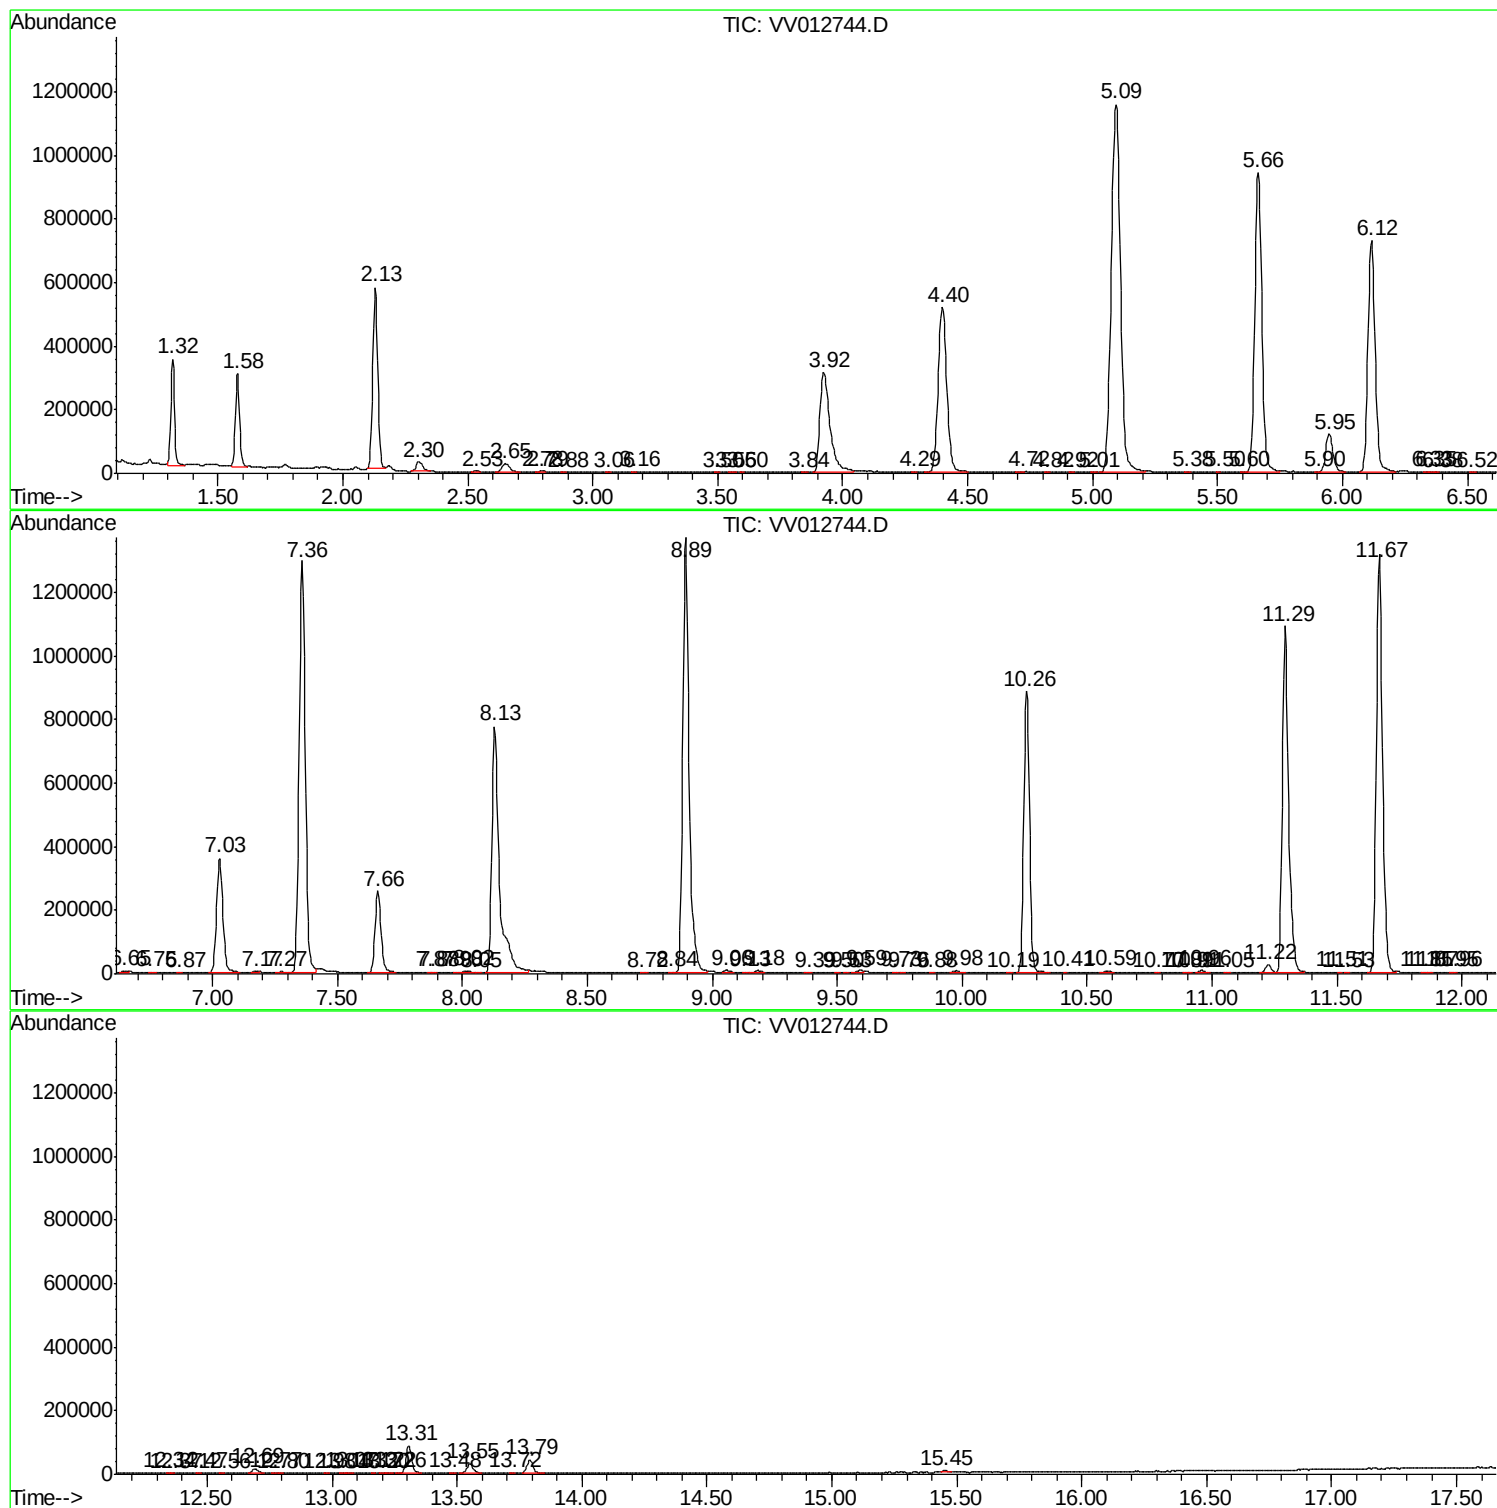

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012744.D
Acq On : 13 Sep 2019 23:10
Operator : SY/MD
Sample : K4868-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091319\
Data File : VV012744.D
Acq On : 13 Sep 2019 23:10
Operator : SY/MD
Sample : K4868-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0MK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
