

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012746.D
 Acq On : 13 Sep 2019 23:59
 Operator : SY/MD
 Sample : K4868-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	86	rVB	339549	340233	11.31%	1.498%
2	1.579	144	152	164	rVB	295193	348470	11.59%	1.534%
3	2.129	312	323	335	rBV	586761	837361	27.84%	3.687%
4	2.302	369	377	389	rVB	18055	31116	1.03%	0.137%
5	2.537	443	450	457	rVB8	2164	3254	0.11%	0.014%
6	2.650	475	485	500	rVB	14400	29121	0.97%	0.128%
7	2.855	545	549	552	rBV5	888	708	0.02%	0.003%
8	2.923	568	570	574	rVB3	886	558	0.02%	0.002%
9	2.952	574	579	581	rBV2	1100	1074	0.04%	0.005%
10	3.077	614	618	620	rBV3	1007	629	0.02%	0.003%
11	3.110	623	628	632	rVV3	974	933	0.03%	0.004%
12	3.161	640	644	646	rBV3	776	646	0.02%	0.003%
13	3.212	657	660	662	rBV3	959	670	0.02%	0.003%
14	3.232	663	666	668	rVV3	601	494	0.02%	0.002%
15	3.318	690	693	696	rBV2	1087	739	0.02%	0.003%
16	3.357	696	705	706	rBV5	929	1078	0.04%	0.005%
17	3.598	777	780	783	rBV2	829	485	0.02%	0.002%
18	3.669	798	802	805	rBV3	950	954	0.03%	0.004%
19	3.691	806	809	813	rVB2	992	691	0.02%	0.003%
20	3.727	817	820	824	rBV3	929	678	0.02%	0.003%
21	3.749	824	827	830	rBV2	844	648	0.02%	0.003%
22	3.923	869	881	912	rBV	305500	827286	27.50%	3.642%
23	4.187	958	963	967	rBV6	1311	1496	0.05%	0.007%
24	4.399	1011	1029	1057	rBV	519126	1268135	42.16%	5.583%
25	4.711	1123	1126	1131	rBV7	1299	1220	0.04%	0.005%
26	4.772	1142	1145	1148	rBV4	817	698	0.02%	0.003%
27	4.884	1178	1180	1186	rVB4	940	727	0.02%	0.003%
28	5.093	1222	1245	1284	rBV2	1162401	3007823	100.00%	13.242%
29	5.383	1333	1335	1339	rBV4	1055	1070	0.04%	0.005%
30	5.537	1381	1383	1386	rBV4	1090	791	0.03%	0.003%
31	5.662	1407	1422	1444	rBV	911387	1787540	59.43%	7.870%
32	5.945	1495	1510	1526	rBV	129292	260812	8.67%	1.148%
33	6.116	1547	1563	1591	rBV	728857	1486386	49.42%	6.544%
34	6.248	1597	1604	1606	rBV7	1972	2584	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012746.D
 Acq On : 13 Sep 2019 23:59
 Operator : SY/MD
 Sample : K4868-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	6.441	1662	1664	1666	rBV2	885	483	0.02%	0.002%
36	6.576	1703	1706	1709	rBV4	744	530	0.02%	0.002%
37	6.650	1721	1729	1740	rBV5	6220	12901	0.43%	0.057%
38	7.026	1833	1846	1863	rBV	355843	632302	21.02%	2.784%
39	7.174	1886	1892	1900	rBV8	3342	5486	0.18%	0.024%
40	7.357	1936	1949	1968	rBV	1301720	2235121	74.31%	9.840%
41	7.662	2029	2044	2065	rBV	253095	432203	14.37%	1.903%
42	7.804	2086	2088	2091	rVV3	933	634	0.02%	0.003%
43	7.968	2134	2139	2140	rBV4	2399	1731	0.06%	0.008%
44	8.051	2162	2165	2168	rBV3	1301	786	0.03%	0.003%
45	8.129	2177	2189	2234	rBV2	747937	1634390	54.34%	7.195%
46	8.460	2290	2292	2295	rBV2	777	556	0.02%	0.002%
47	8.479	2296	2298	2303	rVB5	1335	859	0.03%	0.004%
48	8.502	2303	2305	2308	rBV5	916	587	0.02%	0.003%
49	8.553	2320	2321	2327	rBV5	925	609	0.02%	0.003%
50	8.781	2388	2392	2393	rBV2	948	588	0.02%	0.003%
51	8.894	2414	2427	2453	rBV	1321415	2224438	73.96%	9.793%
52	9.100	2489	2491	2495	rVB4	954	631	0.02%	0.003%
53	9.177	2511	2515	2516	rBV2	1542	1068	0.04%	0.005%
54	9.453	2596	2601	2604	rBV4	1279	1258	0.04%	0.006%
55	9.524	2616	2623	2625	rBV6	951	1157	0.04%	0.005%
56	9.582	2635	2641	2643	rBV7	1696	1639	0.05%	0.007%
57	9.698	2672	2677	2680	rBV6	944	1069	0.04%	0.005%
58	9.756	2692	2695	2699	rBV3	893	550	0.02%	0.002%
59	9.829	2715	2718	2722	rVB3	849	676	0.02%	0.003%
60	9.923	2745	2747	2753	rVB5	883	817	0.03%	0.004%
61	9.952	2753	2756	2759	rBV3	1175	778	0.03%	0.003%
62	9.981	2759	2765	2768	rBV5	1232	1049	0.03%	0.005%
63	10.026	2775	2779	2781	rBV3	578	482	0.02%	0.002%
64	10.257	2838	2851	2871	rBV	875421	1365363	45.39%	6.011%
65	10.421	2895	2902	2913	rVV3	4387	7132	0.24%	0.031%
66	10.521	2931	2933	2937	rVB4	863	553	0.02%	0.002%
67	10.585	2949	2953	2955	rBV3	1081	799	0.03%	0.004%
68	10.627	2960	2966	2968	rBV4	695	673	0.02%	0.003%
69	10.678	2978	2982	2984	rBV3	696	565	0.02%	0.002%
70	10.874	3037	3043	3045	rBV2	671	669	0.02%	0.003%
71	10.958	3066	3069	3071	rVV3	1092	629	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012746.D
 Acq On : 13 Sep 2019 23:59
 Operator : SY/MD
 Sample : K4868-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	10.993	3077	3080	3084	rBV3	1450	1022	0.03%	0.004%
73	11.225	3133	3152	3160	rBV4	10073	18916	0.63%	0.083%
74	11.292	3160	3173	3195	rVV	1007464	1664302	55.33%	7.327%
75	11.479	3229	3231	3235	rVB3	1282	492	0.02%	0.002%
76	11.505	3235	3239	3242	rBV5	904	833	0.03%	0.004%
77	11.669	3277	3290	3313	rBV	1303978	2125802	70.68%	9.359%
78	11.942	3373	3375	3378	rBV3	952	521	0.02%	0.002%
79	12.263	3472	3475	3478	rBV3	665	527	0.02%	0.002%
80	12.363	3503	3506	3508	rVB	997	613	0.02%	0.003%
81	12.392	3510	3515	3516	rBV3	814	689	0.02%	0.003%
82	12.421	3521	3524	3525	rBV2	1129	497	0.02%	0.002%
83	12.472	3538	3540	3543	rVV2	915	485	0.02%	0.002%
84	12.630	3586	3589	3592	rVB3	897	495	0.02%	0.002%
85	12.691	3602	3608	3612	rBV8	2270	2796	0.09%	0.012%
86	12.797	3639	3641	3647	rVB6	943	640	0.02%	0.003%
87	12.897	3669	3672	3673	rBV2	705	478	0.02%	0.002%
88	13.048	3717	3719	3722	rBV2	808	510	0.02%	0.002%
89	13.125	3741	3743	3746	rBV3	799	518	0.02%	0.002%
90	13.308	3791	3800	3813	rVB2	32393	50974	1.69%	0.224%
91	13.357	3813	3815	3817	rBV2	935	598	0.02%	0.003%
92	13.424	3833	3836	3840	rBV3	1328	1051	0.03%	0.005%
93	13.543	3869	3873	3874	rBV3	1734	1304	0.04%	0.006%
94	13.685	3913	3917	3918	rBV2	841	709	0.02%	0.003%
95	13.762	3939	3941	3944	rVB4	1181	599	0.02%	0.003%
96	13.794	3944	3951	3963	rBV5	9269	16284	0.54%	0.072%
97	13.958	3998	4002	4004	rBV4	934	772	0.03%	0.003%
98	14.032	4022	4025	4026	rBV2	1164	525	0.02%	0.002%
99	14.109	4046	4049	4051	rBV2	863	656	0.02%	0.003%
100	15.360	4434	4438	4441	rBV5	1861	1741	0.06%	0.008%


Sum of corrected areas: 22714218

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012746.D
Acq On : 13 Sep 2019 23:59
Operator : SY/MD
Sample : K4868-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
COMK7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

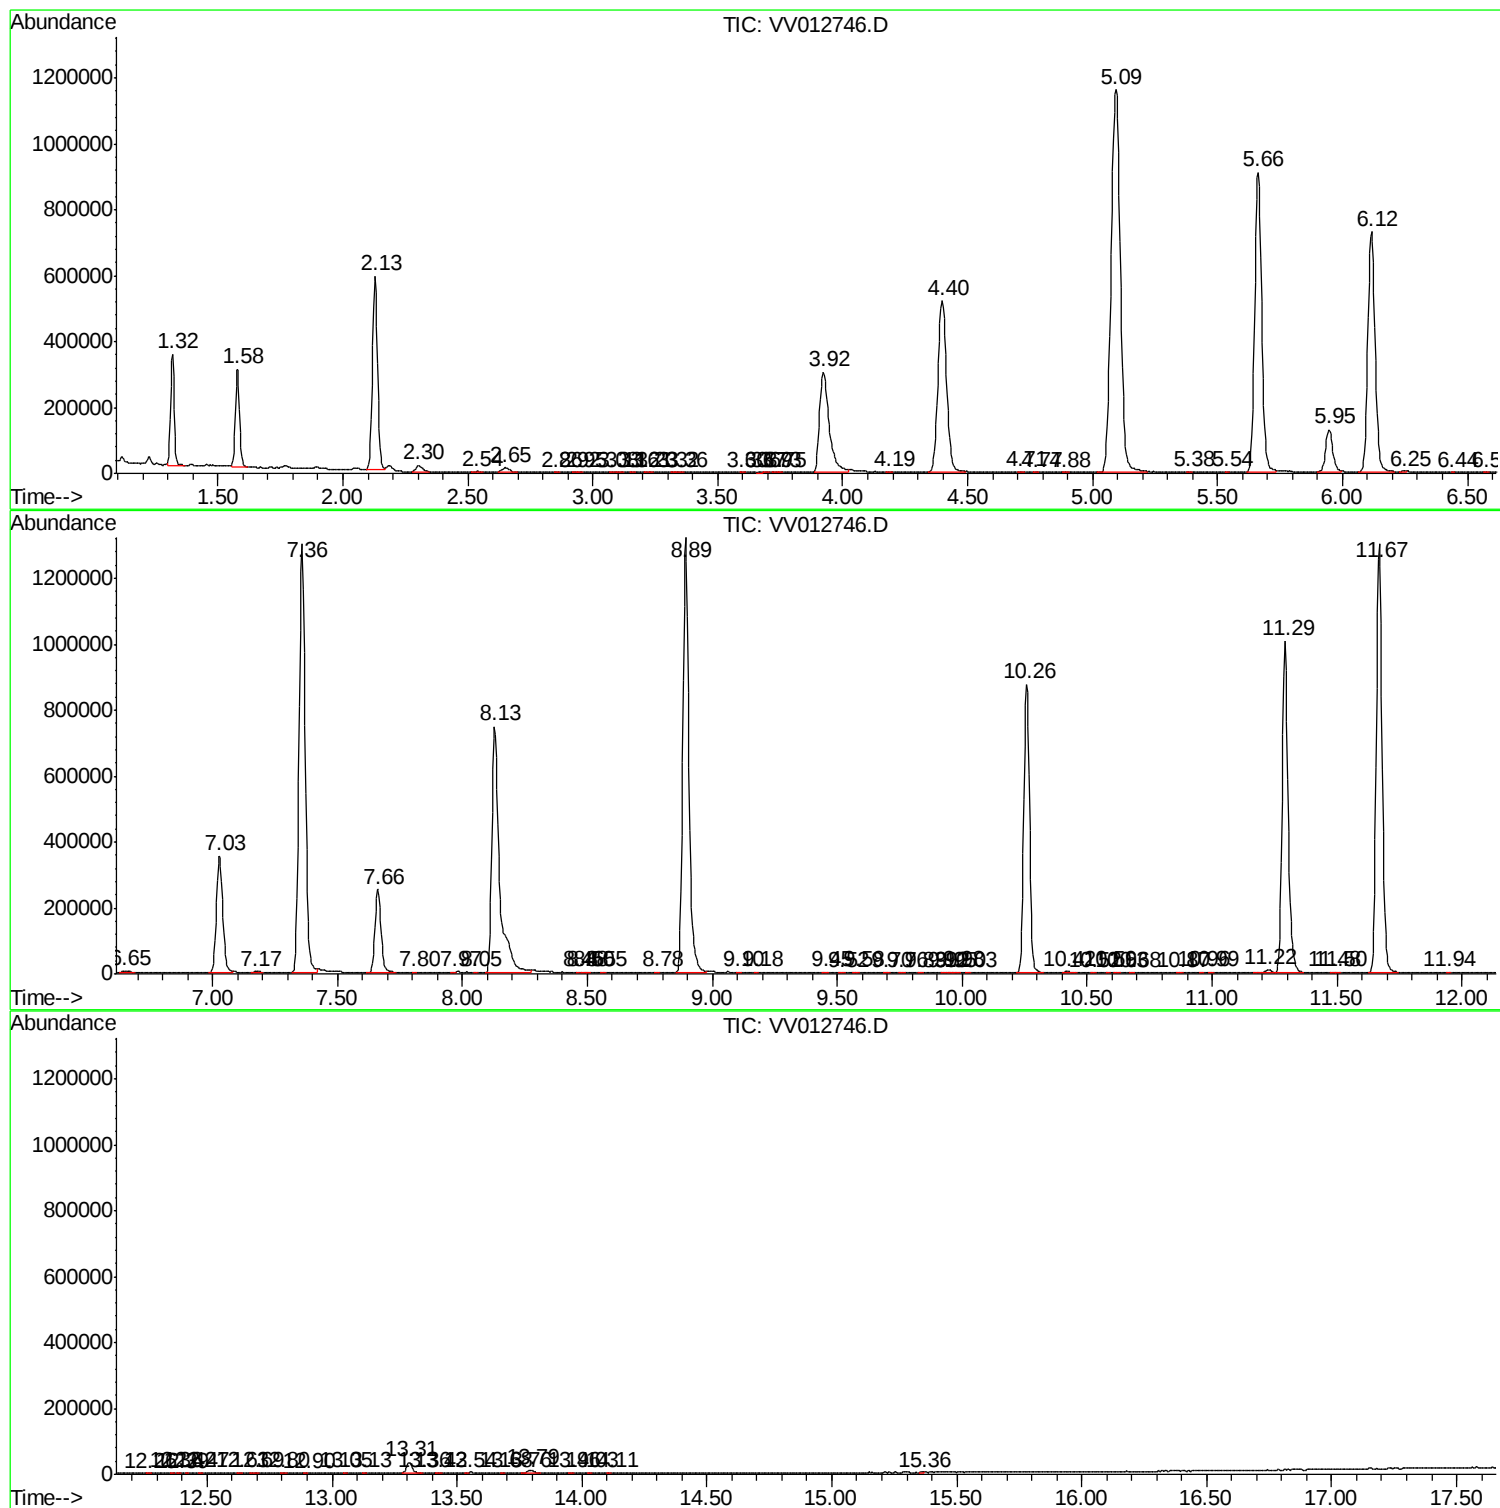

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012746.D
Acq On : 13 Sep 2019 23:59
Operator : SY/MD
Sample : K4868-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MK7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091319\
Data File : VV012746.D
Acq On : 13 Sep 2019 23:59
Operator : SY/MD
Sample : K4868-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0MK7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc