

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012747.D
 Acq On : 14 Sep 2019 00:23
 Operator : SY/MD
 Sample : K4868-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	85	rVB	340997	335608	11.37%	1.480%
2	1.579	145	152	166	rVB	298768	343934	11.65%	1.517%
3	2.129	313	323	335	rBV	585573	822006	27.85%	3.625%
4	2.303	369	377	391	rVB	33568	57771	1.96%	0.255%
5	2.528	441	447	448	rBV4	2541	2028	0.07%	0.009%
6	2.650	471	485	500	rBV	21785	46249	1.57%	0.204%
7	2.791	525	529	530	rBV4	1400	1070	0.04%	0.005%
8	2.923	565	570	572	rBV2	936	655	0.02%	0.003%
9	3.000	589	594	596	rVB4	894	818	0.03%	0.004%
10	3.061	608	613	617	rBV3	1149	1078	0.04%	0.005%
11	3.225	659	664	665	rBV2	1086	990	0.03%	0.004%
12	3.534	756	760	765	rVB3	933	805	0.03%	0.004%
13	3.576	770	773	775	rBV3	929	577	0.02%	0.003%
14	3.730	818	821	823	rBV3	1136	731	0.02%	0.003%
15	3.923	869	881	935	rBV	305096	882223	29.89%	3.891%
16	4.328	1002	1007	1011	rBV7	1042	1116	0.04%	0.005%
17	4.399	1011	1029	1050	rBV	515746	1241478	42.06%	5.475%
18	4.688	1115	1119	1121	rBV5	1302	959	0.03%	0.004%
19	4.717	1126	1128	1131	rVB3	1097	582	0.02%	0.003%
20	4.804	1153	1155	1162	rVB7	1250	984	0.03%	0.004%
21	5.093	1226	1245	1285	rBV2	1151084	2951548	100.00%	13.017%
22	5.502	1367	1372	1373	rBV4	1160	924	0.03%	0.004%
23	5.556	1386	1389	1394	rBV4	1538	1175	0.04%	0.005%
24	5.579	1394	1396	1400	rVB3	885	594	0.02%	0.003%
25	5.662	1407	1422	1450	rBV	922991	1814929	61.49%	8.004%
26	5.836	1473	1476	1479	rBV4	1225	1117	0.04%	0.005%
27	5.952	1498	1512	1540	rVB4	163117	379149	12.85%	1.672%
28	6.116	1546	1563	1589	rBV	727165	1459279	49.44%	6.436%
29	6.289	1615	1617	1620	rVB2	1322	644	0.02%	0.003%
30	6.370	1638	1642	1646	rVB7	1241	1103	0.04%	0.005%
31	6.540	1691	1695	1697	rBV2	1054	658	0.02%	0.003%
32	6.646	1718	1728	1741	rBV5	6031	13427	0.45%	0.059%
33	6.778	1761	1769	1770	rBV5	725	825	0.03%	0.004%
34	6.817	1776	1781	1784	rVB6	1175	1117	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012747.D
 Acq On : 14 Sep 2019 00:23
 Operator : SY/MD
 Sample : K4868-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	6.836	1784	1787	1790	rBV3	1034	746	0.03%	0.003%
36	7.029	1833	1847	1867	rBV	345272	624188	21.15%	2.753%
37	7.180	1887	1894	1901	rBV9	3201	5339	0.18%	0.024%
38	7.244	1910	1914	1917	rBV4	1410	1159	0.04%	0.005%
39	7.357	1935	1949	1969	rBV	1275183	2209100	74.85%	9.742%
40	7.662	2028	2044	2062	rBV	248187	421441	14.28%	1.859%
41	7.907	2116	2120	2125	rVB5	1408	1288	0.04%	0.006%
42	7.974	2135	2141	2148	rVV7	1964	2783	0.09%	0.012%
43	8.016	2149	2154	2156	rBV5	1787	1578	0.05%	0.007%
44	8.129	2178	2189	2225	rBV2	757079	1611300	54.59%	7.106%
45	8.691	2361	2364	2367	rBV4	864	656	0.02%	0.003%
46	8.727	2371	2375	2378	rBV2	1022	720	0.02%	0.003%
47	8.810	2398	2401	2405	rVB4	1434	1066	0.04%	0.005%
48	8.836	2405	2409	2410	rBV3	1347	990	0.03%	0.004%
49	8.894	2413	2427	2463	rBV	1324727	2243118	76.00%	9.893%
50	9.119	2494	2497	2501	rVB4	991	702	0.02%	0.003%
51	9.180	2511	2516	2517	rBV3	1567	1127	0.04%	0.005%
52	9.421	2588	2591	2596	rVB5	1461	1076	0.04%	0.005%
53	9.450	2596	2600	2602	rBV4	1145	752	0.03%	0.003%
54	9.466	2602	2605	2611	rVB4	1015	867	0.03%	0.004%
55	9.518	2618	2621	2626	rBV3	809	725	0.02%	0.003%
56	9.588	2639	2643	2644	rBV3	1236	855	0.03%	0.004%
57	9.723	2680	2685	2689	rBV5	667	581	0.02%	0.003%
58	9.759	2693	2696	2703	rBV6	855	950	0.03%	0.004%
59	9.887	2733	2736	2740	rBV2	1002	959	0.03%	0.004%
60	9.974	2761	2763	2769	rVB3	1541	1136	0.04%	0.005%
61	10.061	2788	2790	2795	rVB5	815	627	0.02%	0.003%
62	10.090	2795	2799	2801	rBV	798	577	0.02%	0.003%
63	10.154	2813	2819	2822	rBV4	1023	961	0.03%	0.004%
64	10.215	2834	2838	2839	rVV2	871	604	0.02%	0.003%
65	10.257	2839	2851	2875	rVB	856268	1362922	46.18%	6.011%
66	10.418	2896	2901	2903	rBV5	2645	2784	0.09%	0.012%
67	10.588	2949	2954	2959	rBV5	1181	1296	0.04%	0.006%
68	10.871	3035	3042	3045	rBV3	821	1057	0.04%	0.005%
69	10.897	3047	3050	3055	rVB4	1215	937	0.03%	0.004%
70	10.920	3055	3057	3062	rVB3	983	827	0.03%	0.004%
71	10.958	3066	3069	3071	rBV3	1224	791	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012747.D
 Acq On : 14 Sep 2019 00:23
 Operator : SY/MD
 Sample : K4868-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMK8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	11.225	3141	3152	3161	rBV7	6640	11800	0.40%	0.052%
73	11.293	3161	3173	3194	rBV	1011640	1657111	56.14%	7.308%
74	11.585	3260	3264	3266	rBV	1028	829	0.03%	0.004%
75	11.669	3278	3290	3315	rBV	1286822	2057922	69.72%	9.076%
76	11.981	3385	3387	3392	rVB4	979	922	0.03%	0.004%
77	12.026	3396	3401	3402	rBV3	923	582	0.02%	0.003%
78	12.061	3409	3412	3417	rVB6	1219	851	0.03%	0.004%
79	12.177	3445	3448	3450	rBV3	916	719	0.02%	0.003%
80	12.296	3483	3485	3490	rVB5	962	669	0.02%	0.003%
81	12.337	3496	3498	3502	rVB3	1156	770	0.03%	0.003%
82	12.572	3568	3571	3574	rBV2	878	634	0.02%	0.003%
83	12.688	3601	3607	3608	rBV3	1785	1415	0.05%	0.006%
84	12.746	3621	3625	3627	rBV4	1107	1027	0.03%	0.005%
85	12.772	3631	3633	3640	rVB4	843	763	0.03%	0.003%
86	13.006	3703	3706	3708	rBV4	1165	691	0.02%	0.003%
87	13.061	3721	3723	3728	rVB2	1570	1128	0.04%	0.005%
88	13.116	3737	3740	3745	rVB4	1109	1026	0.03%	0.005%
89	13.228	3770	3775	3780	rBV6	1193	1142	0.04%	0.005%
90	13.309	3791	3800	3813	rVV2	22081	37427	1.27%	0.165%
91	13.466	3846	3849	3853	rBV2	842	747	0.03%	0.003%
92	13.653	3904	3907	3914	rBV5	891	1032	0.03%	0.005%
93	13.730	3925	3931	3933	rBV2	1283	1173	0.04%	0.005%
94	13.746	3933	3936	3940	rVV3	934	904	0.03%	0.004%
95	13.797	3943	3952	3959	rBV4	6856	11088	0.38%	0.049%
96	14.019	4018	4021	4023	rBV4	865	599	0.02%	0.003%
97	14.154	4060	4063	4068	rBV4	1274	935	0.03%	0.004%
98	14.662	4218	4221	4226	rBV4	1258	1258	0.04%	0.006%
99	15.029	4332	4335	4338	rVB4	1666	1172	0.04%	0.005%
100	15.109	4355	4360	4364	rBV6	1636	1861	0.06%	0.008%


Sum of corrected areas: 22674933

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012747.D
Acq On : 14 Sep 2019 00:23
Operator : SY/MD
Sample : K4868-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMK8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

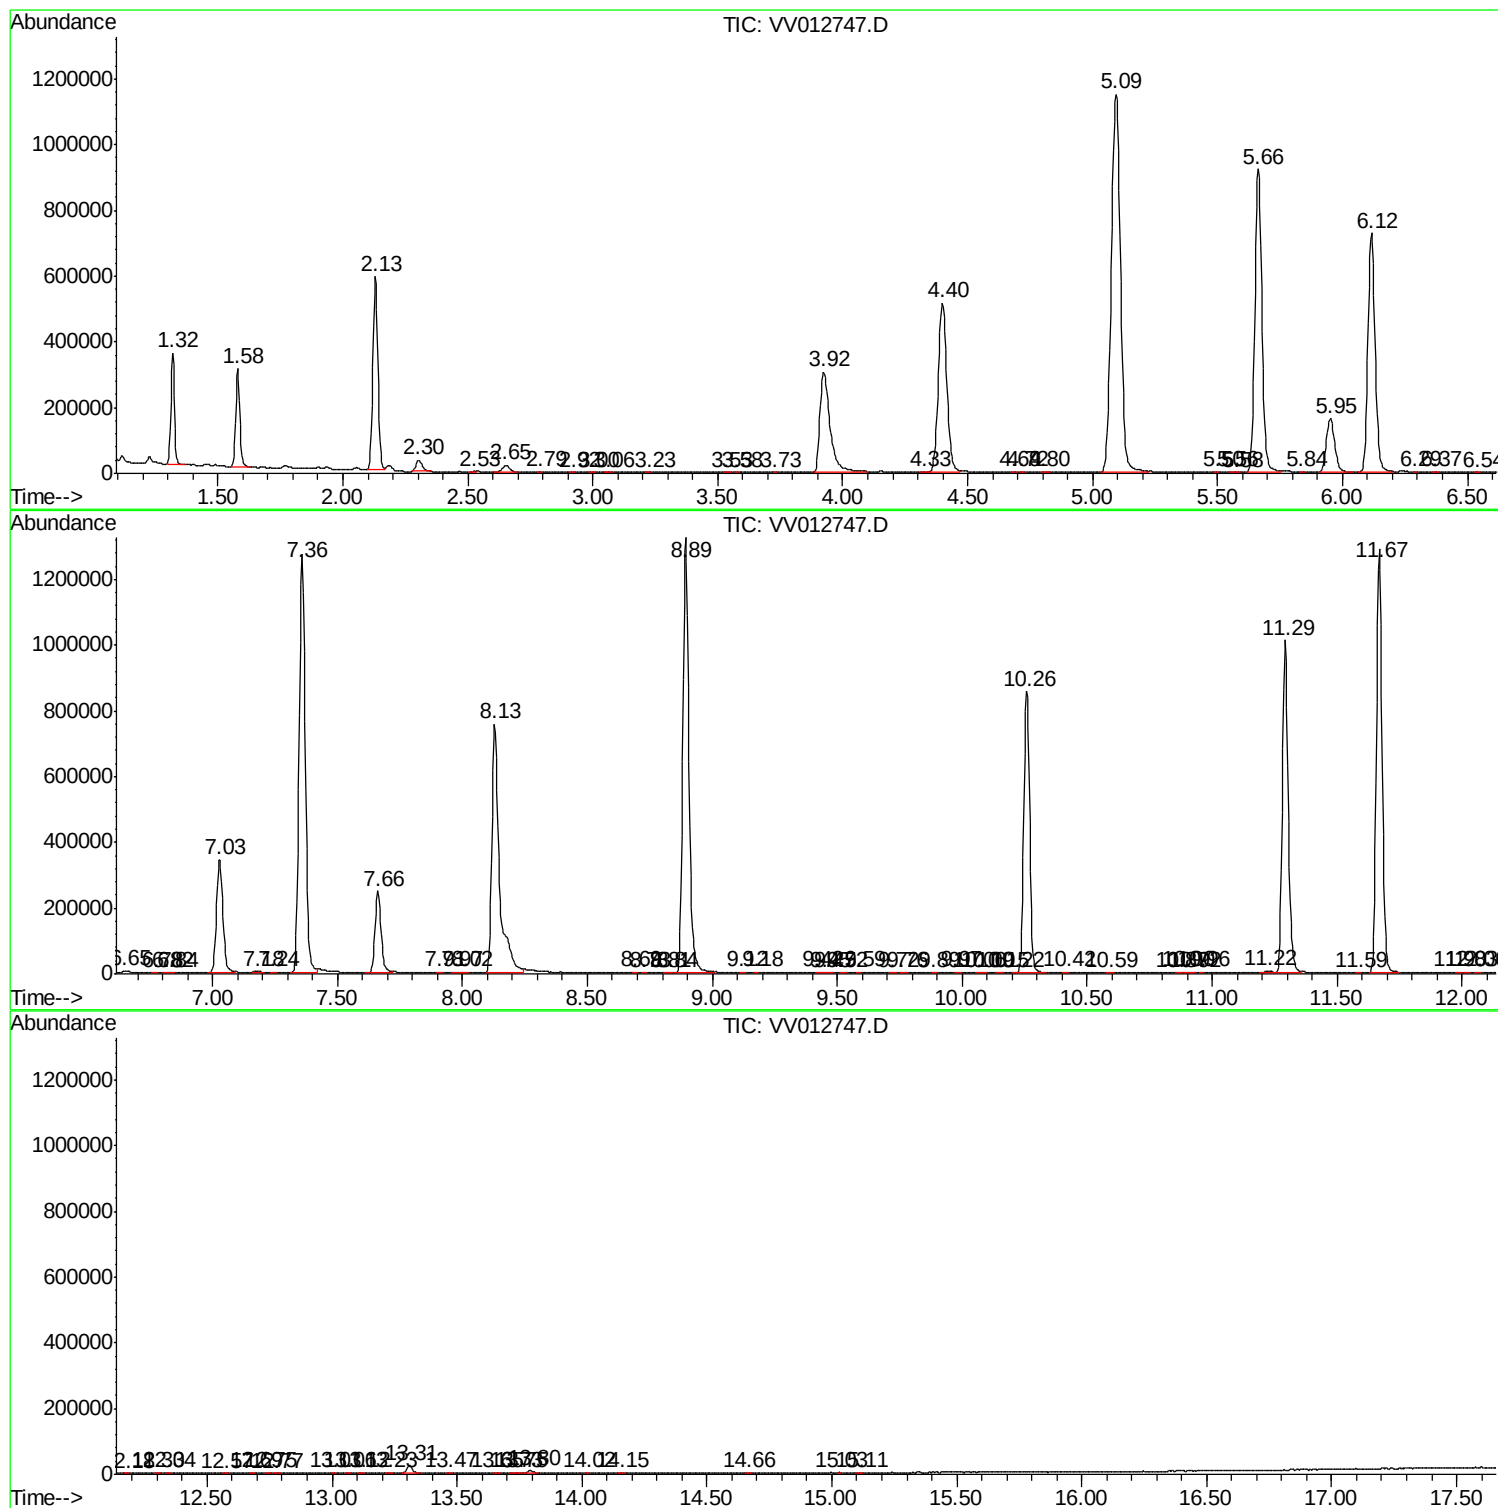

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012747.D
Acq On : 14 Sep 2019 00:23
Operator : SY/MD
Sample : K4868-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMK8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091319\
Data File : VV012747.D
Acq On : 14 Sep 2019 00:23
Operator : SY/MD
Sample : K4868-04
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
COMK8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc