

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012754.D
 Acq On : 14 Sep 2019 03:14
 Operator : SY/MD
 Sample : K4867-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMGO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	314593	306105	10.91%	1.447%
2	1.576	145	151	162	rVB	279711	321480	11.45%	1.519%
3	2.129	314	323	334	rVB	549772	770230	27.44%	3.640%
4	2.650	473	485	497	rBV2	9561	18736	0.67%	0.089%
5	2.862	548	551	553	rBV3	706	432	0.02%	0.002%
6	2.962	581	582	586	rVB3	596	268	0.01%	0.001%
7	3.074	607	617	619	rBV7	1502	2012	0.07%	0.010%
8	3.113	627	629	630	rBV	682	287	0.01%	0.001%
9	3.155	640	642	646	rBV3	566	350	0.01%	0.002%
10	3.225	660	664	667	rBV3	1044	1115	0.04%	0.005%
11	3.286	681	683	685	rBV3	520	317	0.01%	0.001%
12	3.335	696	698	701	rVB2	583	217	0.01%	0.001%
13	3.380	708	712	716	rBV4	741	901	0.03%	0.004%
14	3.421	721	725	727	rBV3	927	563	0.02%	0.003%
15	3.489	744	746	750	rBV3	367	200	0.01%	0.001%
16	3.518	753	755	759	rVB3	482	335	0.01%	0.002%
17	3.540	759	762	764	rVB2	789	361	0.01%	0.002%
18	3.556	764	767	769	rBV2	496	261	0.01%	0.001%
19	3.572	769	772	774	rBV2	532	399	0.01%	0.002%
20	3.611	779	784	786	rBV4	954	749	0.03%	0.004%
21	3.701	807	812	813	rBV3	559	406	0.01%	0.002%
22	3.727	818	820	822	rBV	334	204	0.01%	0.001%
23	3.749	825	827	828	rVB	359	105	0.00%	0.000%
24	3.765	828	832	833	rBV	662	482	0.02%	0.002%
25	3.814	845	847	849	rBV2	245	106	0.00%	0.001%
26	3.826	849	851	852	rBV2	421	114	0.00%	0.001%
27	3.865	862	863	865	rBV2	329	98	0.00%	0.000%
28	3.923	868	881	916	rBV	284221	775891	27.65%	3.667%
29	4.399	1014	1029	1059	rVB	487078	1183169	42.16%	5.592%
30	4.695	1119	1121	1122	rBV	866	374	0.01%	0.002%
31	4.807	1152	1156	1157	rBV2	410	210	0.01%	0.001%
32	4.817	1157	1159	1160	rBV	598	199	0.01%	0.001%
33	4.849	1166	1169	1171	rVB4	839	501	0.02%	0.002%
34	4.900	1183	1185	1190	rVB4	892	573	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012754.D
 Acq On : 14 Sep 2019 03:14
 Operator : SY/MD
 Sample : K4867-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMGO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	4.939	1195	1197	1202	rBV2	731	661	0.02%	0.003%
36	5.026	1219	1224	1226	rBV4	814	758	0.03%	0.004%
37	5.093	1226	1245	1283	rVV2	1089757	2806478	100.00%	13.264%
38	5.540	1382	1384	1388	rBV4	1342	701	0.02%	0.003%
39	5.560	1388	1390	1395	rVB4	939	650	0.02%	0.003%
40	5.598	1400	1402	1404	rBV2	457	169	0.01%	0.001%
41	5.662	1407	1422	1454	rBV	909710	1814121	64.64%	8.574%
42	5.945	1499	1510	1535	rVB	119286	242470	8.64%	1.146%
43	6.116	1548	1563	1595	rBV	702668	1401816	49.95%	6.625%
44	6.373	1640	1643	1648	rBV6	1183	1176	0.04%	0.006%
45	6.415	1653	1656	1658	rBV3	864	586	0.02%	0.003%
46	6.473	1672	1674	1676	rBV2	824	370	0.01%	0.002%
47	6.563	1698	1702	1703	rBV3	678	524	0.02%	0.002%
48	6.797	1772	1775	1777	rBV3	682	370	0.01%	0.002%
49	6.814	1777	1780	1783	rVV4	813	688	0.02%	0.003%
50	6.842	1787	1789	1795	rVB5	959	529	0.02%	0.003%
51	6.868	1795	1797	1801	rVB3	827	595	0.02%	0.003%
52	6.897	1803	1806	1810	rVB4	970	625	0.02%	0.003%
53	6.920	1810	1813	1814	rBV3	709	371	0.01%	0.002%
54	7.029	1833	1847	1868	rBV	323720	580120	20.67%	2.742%
55	7.357	1936	1949	1971	rBV	1199496	2066631	73.64%	9.768%
56	7.662	2032	2044	2063	rBV	228779	386853	13.78%	1.828%
57	8.058	2165	2167	2169	rBV2	490	237	0.01%	0.001%
58	8.084	2173	2175	2177	rBV3	1127	646	0.02%	0.003%
59	8.129	2178	2189	2229	rBV2	710140	1529492	54.50%	7.229%
60	8.894	2413	2427	2457	rBV	1327410	2179745	77.67%	10.302%
61	9.183	2509	2517	2518	rBV6	1833	2252	0.08%	0.011%
62	9.318	2557	2559	2560	rBV	669	205	0.01%	0.001%
63	9.370	2574	2575	2576	rBV	834	313	0.01%	0.001%
64	9.418	2586	2590	2592	rBV4	846	615	0.02%	0.003%
65	9.489	2608	2612	2615	rBV5	872	683	0.02%	0.003%
66	9.505	2615	2617	2619	rBV2	448	150	0.01%	0.001%
67	9.579	2634	2640	2643	rBV4	1755	1986	0.07%	0.009%
68	9.784	2702	2704	2705	rBV4	596	241	0.01%	0.001%
69	9.846	2721	2723	2729	rVB4	684	457	0.02%	0.002%
70	9.878	2729	2733	2734	rBV2	572	446	0.02%	0.002%
71	9.993	2766	2769	2771	rBV4	1058	500	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012754.D
 Acq On : 14 Sep 2019 03:14
 Operator : SY/MD
 Sample : K4867-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	10.061	2788	2790	2791	rBV2	778	347	0.01%	0.002%
73	10.161	2819	2821	2824	rBV3	699	445	0.02%	0.002%
74	10.257	2838	2851	2867	rBV	824564	1298634	46.27%	6.138%
75	10.521	2928	2933	2936	rBV5	729	603	0.02%	0.003%
76	10.543	2937	2940	2945	rVV5	781	626	0.02%	0.003%
77	10.778	3011	3013	3014	rBV2	569	213	0.01%	0.001%
78	10.810	3020	3023	3025	rVB3	1244	521	0.02%	0.002%
79	10.820	3025	3026	3029	rBV	637	351	0.01%	0.002%
80	10.852	3034	3036	3037	rBV	435	133	0.00%	0.001%
81	10.887	3041	3047	3050	rBV6	1469	1352	0.05%	0.006%
82	10.932	3059	3061	3065	rVB2	981	658	0.02%	0.003%
83	10.955	3065	3068	3069	rBV3	827	559	0.02%	0.003%
84	11.019	3085	3088	3089	rBV	495	276	0.01%	0.001%
85	11.048	3094	3097	3098	rBV2	769	384	0.01%	0.002%
86	11.106	3112	3115	3117	rBV2	674	490	0.02%	0.002%
87	11.292	3160	3173	3195	rBV	979972	1554066	55.37%	7.345%
88	11.669	3277	3290	3315	rBV	1190297	1883168	67.10%	8.900%
89	11.984	3385	3388	3389	rBV3	1226	647	0.02%	0.003%
90	12.170	3444	3446	3450	rVB4	1049	560	0.02%	0.003%
91	12.354	3500	3503	3506	rBV2	1027	855	0.03%	0.004%
92	12.559	3564	3567	3569	rBV2	725	347	0.01%	0.002%


Sum of corrected areas: 21158215

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012754.D
Acq On : 14 Sep 2019 03:14
Operator : SY/MD
Sample : K4867-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

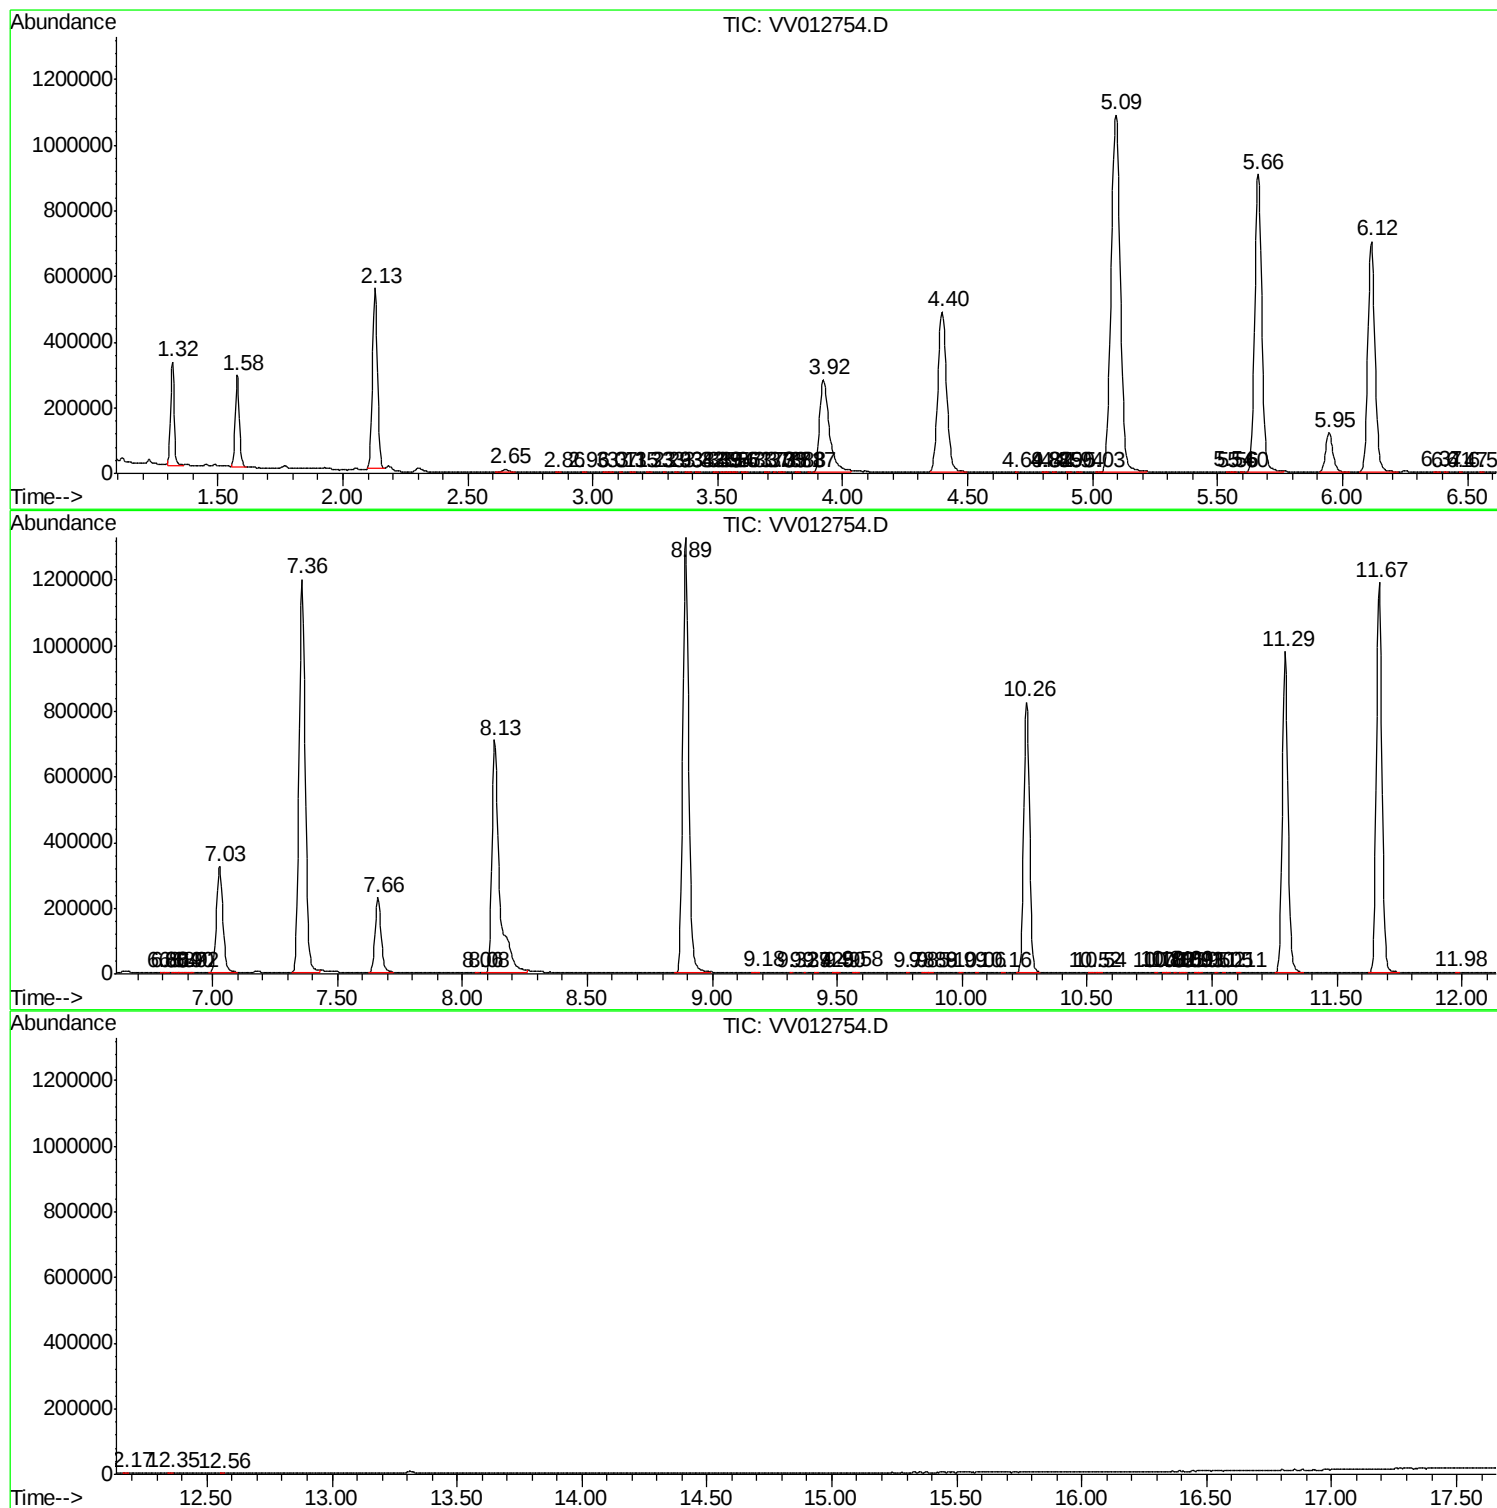

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012754.D
Acq On : 14 Sep 2019 03:14
Operator : SY/MD
Sample : K4867-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012754.D
Acq On : 14 Sep 2019 03:14
Operator : SY/MD
Sample : K4867-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc