

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012783.D
 Acq On : 14 Sep 2019 22:13
 Operator : SY/MD
 Sample : K4867-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	256783	254355	10.11%	1.314%
2	1.579	145	152	168	rVB	228826	273682	10.88%	1.414%
3	2.129	312	323	335	rBV	460947	655300	26.05%	3.385%
4	2.303	369	377	395	rVB	25963	47544	1.89%	0.246%
5	2.579	460	463	468	rVV3	881	751	0.03%	0.004%
6	2.650	475	485	500	rVB	17352	37517	1.49%	0.194%
7	2.801	522	532	539	rBV9	2534	4772	0.19%	0.025%
8	2.872	551	554	563	rVB5	1178	1230	0.05%	0.006%
9	2.965	578	583	586	rBV5	1027	984	0.04%	0.005%
10	3.026	599	602	606	rVB3	1365	851	0.03%	0.004%
11	3.068	610	615	617	rVV4	882	658	0.03%	0.003%
12	3.168	640	646	648	rBV4	952	961	0.04%	0.005%
13	3.351	698	703	706	rBV4	751	631	0.03%	0.003%
14	3.399	716	718	724	rVB4	934	582	0.02%	0.003%
15	3.537	758	761	763	rVV3	1138	653	0.03%	0.003%
16	3.717	813	817	823	rVB5	601	680	0.03%	0.004%
17	3.923	867	881	923	rBV	273075	776188	30.85%	4.009%
18	4.322	1001	1005	1007	rVB4	987	741	0.03%	0.004%
19	4.399	1007	1029	1057	rBV	451787	1115951	44.35%	5.764%
20	4.650	1103	1107	1113	rVB7	890	836	0.03%	0.004%
21	4.698	1119	1122	1125	rBV5	995	825	0.03%	0.004%
22	4.958	1197	1203	1205	rBV4	975	747	0.03%	0.004%
23	4.978	1205	1209	1211	rBV2	1034	538	0.02%	0.003%
24	5.093	1226	1245	1273	rBV2	976489	2515959	100.00%	12.995%
25	5.354	1324	1326	1329	rVB3	1643	941	0.04%	0.005%
26	5.376	1329	1333	1335	rBV4	1343	977	0.04%	0.005%
27	5.396	1335	1339	1344	rVB7	1072	912	0.04%	0.005%
28	5.425	1344	1348	1351	rBV3	780	725	0.03%	0.004%
29	5.444	1351	1354	1359	rVB4	1186	966	0.04%	0.005%
30	5.553	1383	1388	1392	rBV5	908	1033	0.04%	0.005%
31	5.663	1408	1422	1451	rBV	825784	1629108	64.75%	8.414%
32	5.820	1469	1471	1474	rVB3	1803	857	0.03%	0.004%
33	5.946	1494	1510	1528	rBV4	123963	265891	10.57%	1.373%
34	6.116	1548	1563	1594	rBV	631863	1275359	50.69%	6.587%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012783.D
 Acq On : 14 Sep 2019 22:13
 Operator : SY/MD
 Sample : K4867-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

35	6.232	1594	1599	1600	rBV5	1731	1382	0.05%	0.007%
36	6.354	1634	1637	1640	rBV4	934	674	0.03%	0.003%
37	6.421	1655	1658	1662	rVB2	1395	984	0.04%	0.005%
38	6.553	1695	1699	1705	rVB5	1018	1088	0.04%	0.006%
39	6.579	1705	1707	1711	rBV4	913	637	0.03%	0.003%
40	6.627	1717	1722	1723	rBV4	711	593	0.02%	0.003%
41	6.650	1723	1729	1738	rBV4	4896	8882	0.35%	0.046%
42	6.724	1749	1752	1756	rVB3	1540	1343	0.05%	0.007%
43	6.749	1756	1760	1764	rBV6	990	955	0.04%	0.005%
44	6.788	1769	1772	1776	rBV4	958	674	0.03%	0.003%
45	6.904	1805	1808	1814	rVB5	944	989	0.04%	0.005%
46	6.955	1822	1824	1829	rVB4	677	516	0.02%	0.003%
47	7.029	1834	1847	1876	rBV	290314	529059	21.03%	2.733%
48	7.177	1887	1893	1899	rBV5	4016	5536	0.22%	0.029%
49	7.293	1925	1929	1933	rBV4	1306	1065	0.04%	0.006%
50	7.357	1935	1949	1984	rBV	1059137	1861123	73.97%	9.613%
51	7.515	1995	1998	2001	rBV4	1152	606	0.02%	0.003%
52	7.662	2032	2044	2065	rBV	205798	350984	13.95%	1.813%
53	7.843	2096	2100	2103	rVB3	1445	912	0.04%	0.005%
54	7.978	2133	2142	2145	rBV8	1997	2521	0.10%	0.013%
55	8.013	2151	2153	2155	rBV3	1129	690	0.03%	0.004%
56	8.071	2169	2171	2176	rVB2	933	543	0.02%	0.003%
57	8.129	2176	2189	2230	rBV2	656878	1442139	57.32%	7.449%
58	8.473	2293	2296	2299	rBV5	774	725	0.03%	0.004%
59	8.627	2342	2344	2348	rBV3	1151	896	0.04%	0.005%
60	8.724	2368	2374	2377	rBV4	774	956	0.04%	0.005%
61	8.894	2411	2427	2454	rBV	1206793	1964297	78.07%	10.146%
62	9.058	2473	2478	2482	rBV8	1621	1833	0.07%	0.009%
63	9.100	2488	2491	2494	rVB3	1407	762	0.03%	0.004%
64	9.116	2494	2496	2500	rVB4	850	535	0.02%	0.003%
65	9.273	2543	2545	2550	rVB3	884	549	0.02%	0.003%
66	9.370	2573	2575	2581	rVB4	935	689	0.03%	0.004%
67	9.572	2634	2638	2639	rBV3	642	512	0.02%	0.003%
68	9.592	2640	2644	2650	rVV7	937	1290	0.05%	0.007%
69	9.675	2666	2670	2673	rBV3	707	634	0.03%	0.003%
70	9.698	2673	2677	2679	rVV4	1081	739	0.03%	0.004%
71	9.714	2679	2682	2688	rVV6	819	1043	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091319\
 Data File : VV012783.D
 Acq On : 14 Sep 2019 22:13
 Operator : SY/MD
 Sample : K4867-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis

72	9.759	2691	2696	2699	rVV6	645	760	0.03%	0.004%
73	9.775	2699	2701	2705	rVB3	725	502	0.02%	0.003%
74	9.833	2715	2719	2725	rVB4	645	647	0.03%	0.003%
75	9.978	2759	2764	2767	rBV3	657	668	0.03%	0.003%
76	10.055	2785	2788	2792	rVB4	803	789	0.03%	0.004%
77	10.077	2792	2795	2797	rBV2	952	572	0.02%	0.003%
78	10.257	2834	2851	2876	rBV	755393	1200093	47.70%	6.199%
79	10.344	2876	2878	2880	rVV2	972	594	0.02%	0.003%
80	10.370	2884	2886	2887	rVV2	1136	564	0.02%	0.003%
81	10.421	2891	2902	2911	rVB8	3226	4966	0.20%	0.026%
82	10.582	2949	2952	2955	rBV3	847	786	0.03%	0.004%
83	10.791	3013	3017	3021	rBV5	794	808	0.03%	0.004%
84	10.961	3063	3070	3072	rBV5	931	928	0.04%	0.005%
85	11.222	3148	3151	3154	rVV4	990	524	0.02%	0.003%
86	11.235	3154	3155	3159	rVB4	1121	527	0.02%	0.003%
87	11.293	3160	3173	3194	rBV	896314	1375641	54.68%	7.105%
88	11.521	3242	3244	3248	rVB3	900	541	0.02%	0.003%
89	11.669	3277	3290	3311	rBV	1084391	1701953	67.65%	8.791%
90	12.122	3427	3431	3432	rBV2	943	733	0.03%	0.004%
91	12.328	3493	3495	3499	rVB2	907	594	0.02%	0.003%
92	12.775	3631	3634	3638	rBV3	1002	566	0.02%	0.003%
93	12.894	3666	3671	3673	rBV5	986	973	0.04%	0.005%
94	13.106	3732	3737	3741	rVB6	1092	1097	0.04%	0.006%
95	13.312	3796	3801	3806	rBV5	1149	1678	0.07%	0.009%
96	13.334	3806	3808	3816	rVB5	1268	1150	0.05%	0.006%
97	13.874	3974	3976	3980	rBV3	738	677	0.03%	0.003%
98	13.968	4003	4005	4009	rVV2	824	526	0.02%	0.003%
99	14.100	4044	4046	4050	rBV3	938	603	0.02%	0.003%
100	15.337	4428	4431	4435	rBV4	1260	1391	0.06%	0.007%


Sum of corrected areas: 19360911

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091319\
Data File : VV012783.D
Acq On : 14 Sep 2019 22:13
Operator : SY/MD
Sample : K4867-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
COMH6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

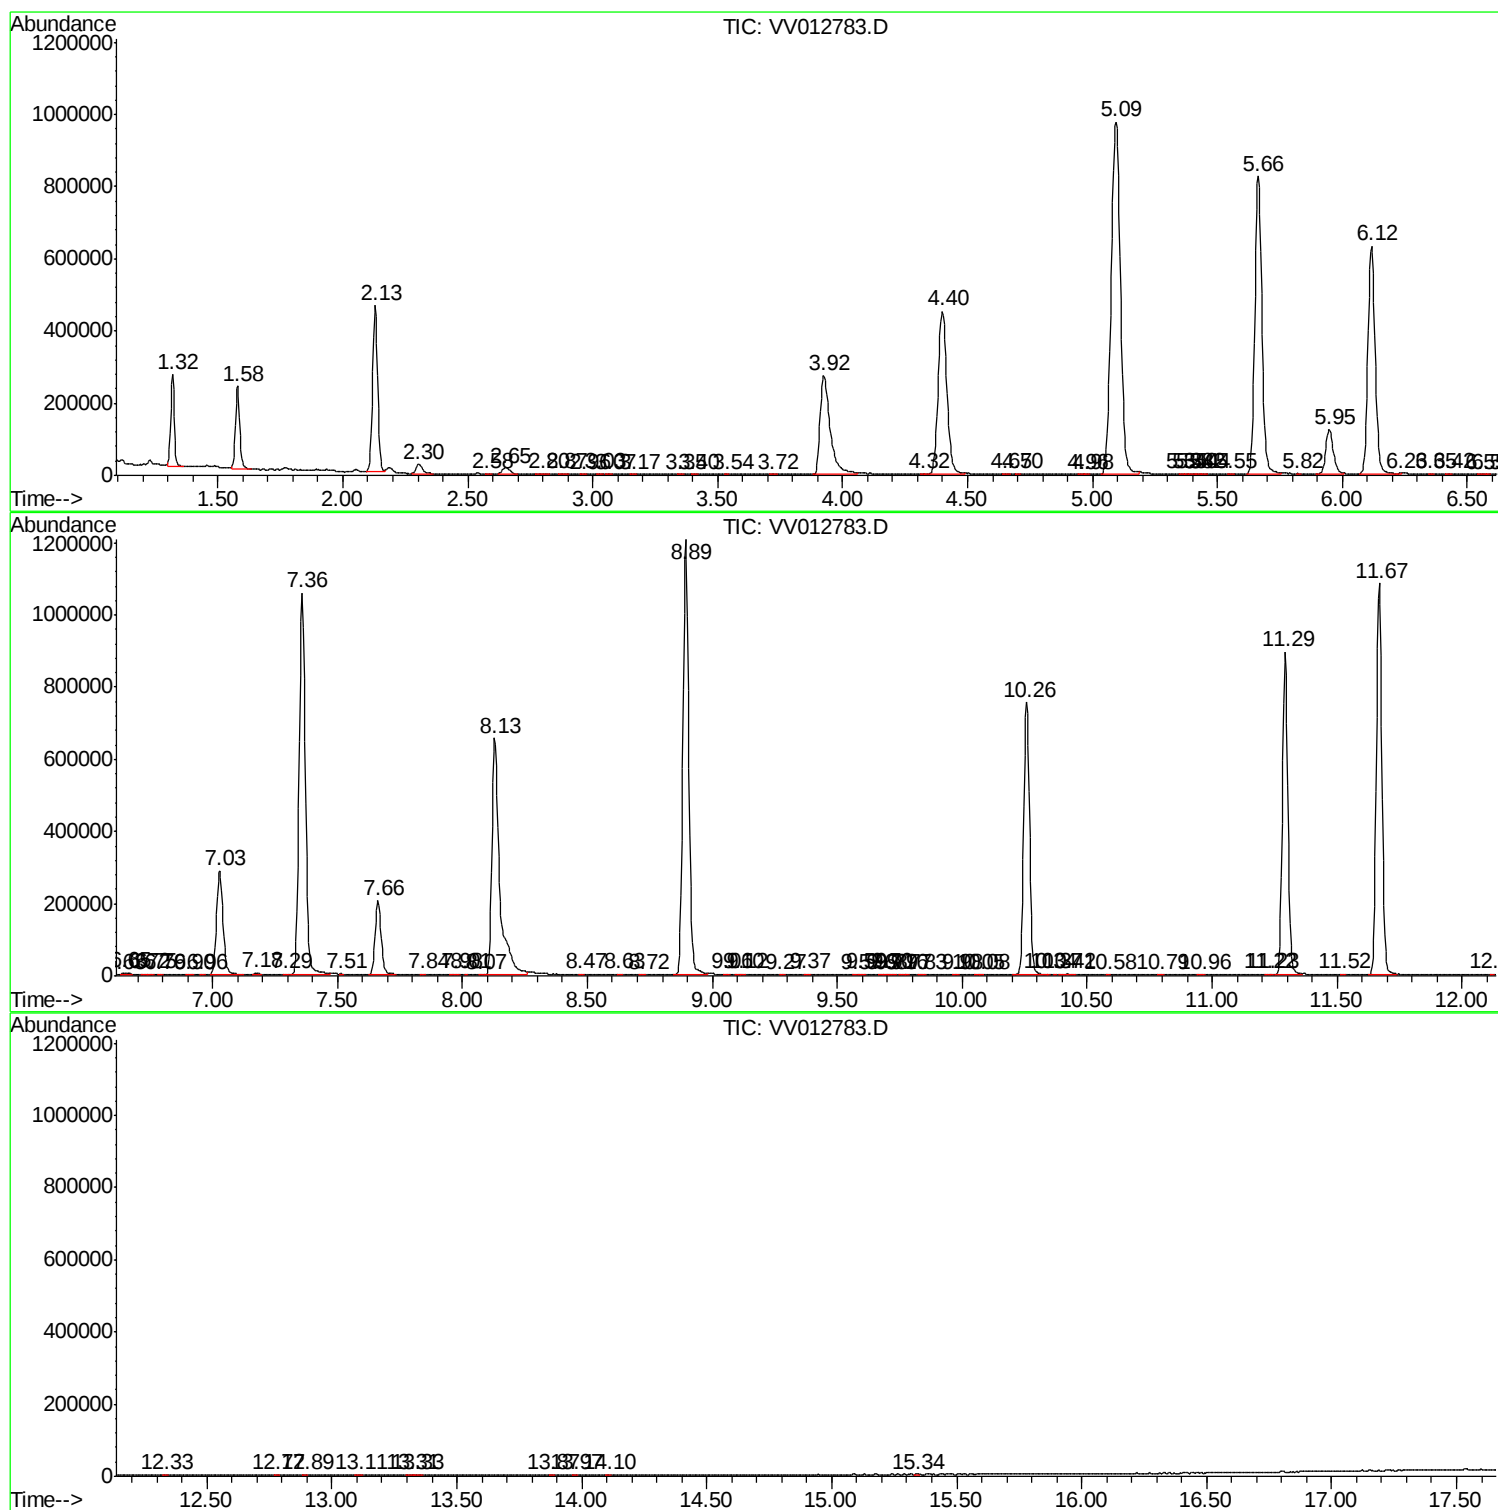

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091319\
Data File : VV012783.D
Acq On : 14 Sep 2019 22:13
Operator : SY/MD
Sample : K4867-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091319\
Data File : VV012783.D
Acq On : 14 Sep 2019 22:13
Operator : SY/MD
Sample : K4867-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
COMH6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM091319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc