


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091319\
 Data File : VV012724.D
 Acq On : 13 Sep 2019 08:32
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM091319WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 16 04:57:02 2019

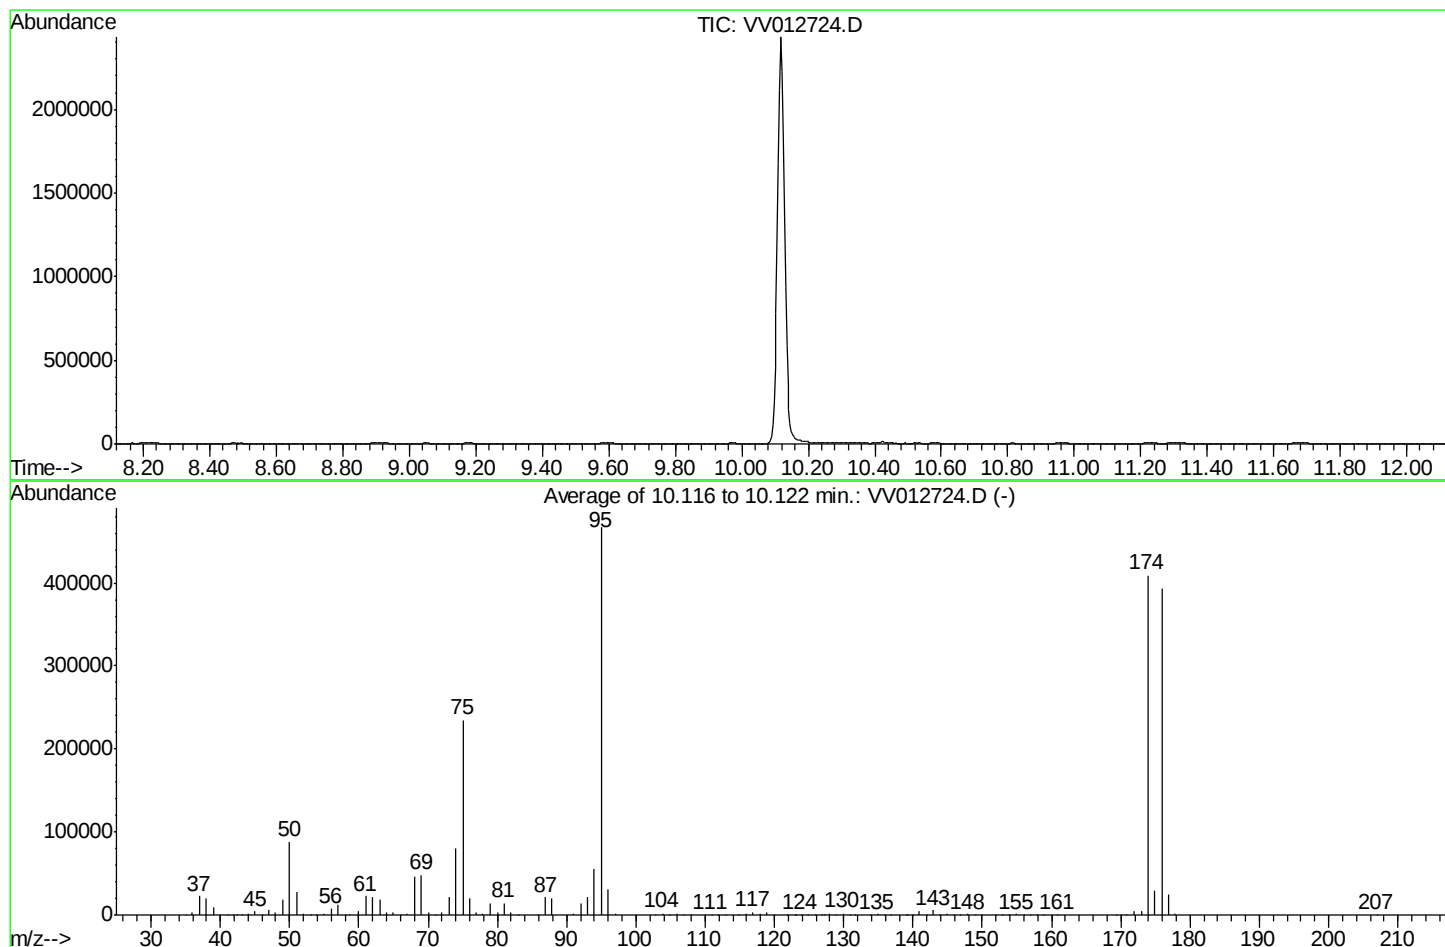

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	88589	PASS
75	95	30	80	50.3	234752	PASS
95	95	100	100	100.0	466880	PASS
96	95	5	9	6.6	31040	PASS
173	174	0.00	2	1.1	4659	PASS
174	95	50	120	87.6	408896	PASS
175	174	5	9	7.3	29778	PASS
176	174	95	101	96.1	393045	PASS
177	176	5	9	6.4	25008	PASS

m/z	Abundance
35.00	184.0
36.00	4138.0
37.00	23256.0
38.00	20576.0
39.00	8970.0
40.00	1514.0
41.10	158.0
41.90	123.0
42.30	105.0
43.10	226.0
44.00	3350.0
45.00	4484.0
46.00	549.0
47.00	6383.0
48.00	2929.0
49.00	19752.0
50.00	92416.0
51.00	28104.0
52.10	1492.0
53.10	528.0
53.90	252.0
55.00	1340.0
56.00	7083.0
57.00	12822.0
58.00	687.0
58.60	101.0
60.00	4222.0
61.00	23944.0
62.00	23312.0
63.00	18992.0
64.00	2679.0
65.00	3388.0
66.00	440.0
66.90	1366.0
68.00	47688.0
69.00	49688.0
70.00	3724.0
71.00	289.0
72.00	2480.0
73.00	21288.0
74.00	81264.0
75.00	241920.0
76.00	20984.0
77.00	2849.0
77.90	2310.0
78.90	14951.0
80.00	3732.0
80.90	14808.0
81.90	3262.0
83.00	383.0
85.80	618.0
86.90	21208.0
87.90	21224.0
90.90	1633.0
92.00	13723.0
93.00	21888.0
94.00	56640.0
95.00	477440.0
96.00	31592.0
97.00	937.0
102.80	267.0
103.90	1947.0
104.90	544.0
105.90	1943.0
106.90	578.0
107.90	138.0
109.90	348.0
110.80	393.0
111.90	259.0
113.00	334.0
114.90	485.0
116.00	1712.0
116.90	3194.0
117.90	1617.0
118.90	2902.0
119.90	114.0
121.80	151.0
122.90	165.0
123.90	334.0
124.80	137.0
125.90	225.0
126.90	222.0
127.80	1501.0
128.80	764.0
129.90	1550.0
130.90	730.0
131.70	112.0
133.80	152.0
134.90	941.0
136.90	755.0
139.00	126.0
140.00	333.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

140.90	4421.0
141.90	630.0
142.90	6189.0
143.90	260.0
144.90	1779.0
145.80	731.0
146.80	303.0
147.90	1155.0
149.00	312.0
150.00	352.0
152.10	287.0
152.90	287.0
153.90	278.0
155.00	1053.0
155.90	286.0
156.80	708.0
157.80	206.0
158.80	503.0
160.90	606.0
169.40	207.0
170.10	136.0
170.80	603.0
171.90	4455.0
173.00	4783.0
173.90	407296.0
174.90	30552.0
175.90	391232.0
176.90	25576.0
177.90	825.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	3917.0
37.00	23216.0
38.00	20120.0
39.00	8959.0
40.00	1521.0
41.10	224.0
41.90	151.0
42.30	102.0
43.10	270.0
44.00	3293.0
45.00	4451.0
46.10	491.0
47.00	6278.0
47.90	2922.0
49.00	19416.0
50.00	91792.0
51.00	28168.0
52.10	1423.0
53.00	445.0
53.90	224.0
55.00	1240.0
56.00	7380.0
57.00	12784.0
58.00	688.0
58.70	177.0
60.00	4003.0
61.00	23584.0
62.00	23032.0
63.00	18632.0
64.00	2787.0
65.00	3114.0
66.00	440.0
66.90	1246.0
68.00	48360.0
69.00	49776.0
70.00	3747.0
70.90	285.0
72.00	2619.0
73.00	21768.0
74.00	82600.0
75.00	243328.0
76.00	21376.0
77.00	2902.0
77.90	2205.0
78.90	15009.0
80.00	3721.0
80.90	14613.0
81.90	3282.0
83.00	352.0
85.80	601.0
86.90	21784.0
87.90	21344.0
90.90	1656.0
92.00	13720.0
93.00	22120.0
94.00	57872.0
95.00	483904.0
96.00	32256.0
97.00	880.0
102.80	284.0
103.90	2036.0
104.90	545.0
105.90	1930.0
106.80	654.0
107.90	166.0
109.90	387.0
110.80	441.0
111.90	370.0
113.00	378.0
114.80	453.0
115.90	1779.0
116.90	3178.0
117.90	1613.0
118.90	2828.0
119.90	121.0
121.90	120.0
122.90	147.0
123.90	314.0
124.90	181.0
125.90	272.0
127.10	215.0
127.80	1385.0
128.90	815.0
129.90	1703.0
130.90	723.0
133.70	140.0
134.90	983.0
135.80	120.0
136.80	841.0
139.20	115.0
140.00	365.0
140.90	4513.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

141.90	766.0
142.90	6144.0
143.80	250.0
144.90	1398.0
145.90	705.0
146.80	328.0
147.90	1176.0
148.90	373.0
149.90	389.0
151.90	261.0
152.90	298.0
153.80	287.0
155.00	1074.0
155.90	283.0
156.90	837.0
157.80	228.0
158.80	546.0
160.90	667.0
169.30	191.0
170.00	178.0
170.80	496.0
171.90	4394.0
173.00	4830.0
173.90	423424.0
174.90	30728.0
175.90	407104.0
176.90	25832.0
177.90	911.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	3361.0
37.00	20944.0
38.00	18024.0
39.00	7974.0
40.00	1548.0
41.10	225.0
41.80	103.0
43.10	314.0
44.00	3111.0
45.00	3884.0
46.10	425.0
47.00	5746.0
47.90	2657.0
49.00	17136.0
50.00	81560.0
51.00	25192.0
52.00	1175.0
52.90	323.0
53.80	172.0
55.00	1018.0
56.00	6877.0
57.00	11523.0
58.00	610.0
58.70	197.0
60.00	3651.0
61.00	21016.0
62.00	20384.0
63.00	16464.0
64.00	2618.0
65.00	2668.0
65.90	471.0
66.90	1027.0
68.00	44104.0
69.00	44824.0
70.00	3515.0
70.90	227.0
72.00	2442.0
73.00	19848.0
74.00	74608.0
75.00	219008.0
76.00	19360.0
77.00	2576.0
77.90	1874.0
78.90	13426.0
80.00	3419.0
80.90	13351.0
81.90	3099.0
83.00	343.0
85.90	513.0
87.00	20112.0
87.90	18888.0
90.90	1444.0
92.00	12430.0
93.00	19928.0
94.00	52672.0
95.00	439296.0
96.00	29272.0
97.10	692.0
102.80	258.0
103.90	1986.0
104.90	523.0
105.90	1819.0
106.80	596.0
107.90	157.0
110.00	390.0
110.90	442.0
111.90	410.0
112.90	430.0
114.80	424.0
115.90	1633.0
116.90	2923.0
117.90	1535.0
118.90	2520.0
122.70	119.0
123.10	140.0
123.80	278.0
124.90	230.0
125.90	255.0
127.10	209.0
127.90	1331.0
128.90	793.0
129.90	1601.0
130.90	689.0
133.70	112.0
134.90	909.0
135.80	149.0
136.80	836.0
139.20	133.0
139.90	373.0
140.90	4134.0
141.90	799.0
142.90	5525.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

144.00	225.0
144.90	995.0
145.90	648.0
146.80	359.0
147.90	1161.0
148.90	349.0
149.90	374.0
151.80	284.0
152.80	315.0
153.80	291.0
154.90	957.0
156.00	241.0
156.90	908.0
157.80	207.0
158.80	498.0
160.90	590.0
169.30	120.0
170.00	207.0
170.80	437.0
171.90	4003.0
173.00	4366.0
173.90	395968.0
174.90	28056.0
175.90	380800.0
176.90	23616.0
177.90	779.0
207.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

Scan 2793 (10.071 min): VV012724.D
BFB70

m/z	Abundance
35.80	123.0
37.90	166.0
40.00	1145.0
40.90	111.0
43.90	1025.0
45.20	101.0
48.60	104.0
55.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70