

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091322\
 Data File : VV027811.D
 Acq On : 13 Sep 2022 10:24
 Operator : SY/MD
 Sample : VSTDCCC0.5
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5287

Quant Time: Sep 14 02:29:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 10 02:33:14 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	4395	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.848	117	4078	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	2712	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.296	65	1388	0.509	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 102.000%	
4) 1,2-Dichloroethane-d4	5.019	65	1058	0.516	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	= 104.000%	
7) 1,2-Dichloropropane-d6	6.068	67	681	0.501	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 100.000%	
8) Toluene-d8	7.301	98	3759	0.500	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	= 100.000%	
10) 1,1,2,2-Tetrachloroeth...	10.216	84	580	0.498	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 100.000%	
Target Compounds						Qvalue
3) Vinyl chloride	1.296	62	1285	0.502	ug/L	97
6) Trichloroethene	5.901	95	1307	0.514	ug/L	94
9) 1,2-Dibromoethane	8.353	107	743	0.501	ug/L	100
12) 1,2,3-Trichloropropane	10.267	75	435	0.489	ug/L	97
13) 1,2-Dibromo-3-chloropr...	12.409	75	116	0.647	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091322\
Data File : VV027811.D
Acq On : 13 Sep 2022 10:24
Operator : SY/MD
Sample : VSTDCCC0.5
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5287

Quant Time: Sep 14 02:29:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 10 02:33:14 2022
Response via : Initial Calibration




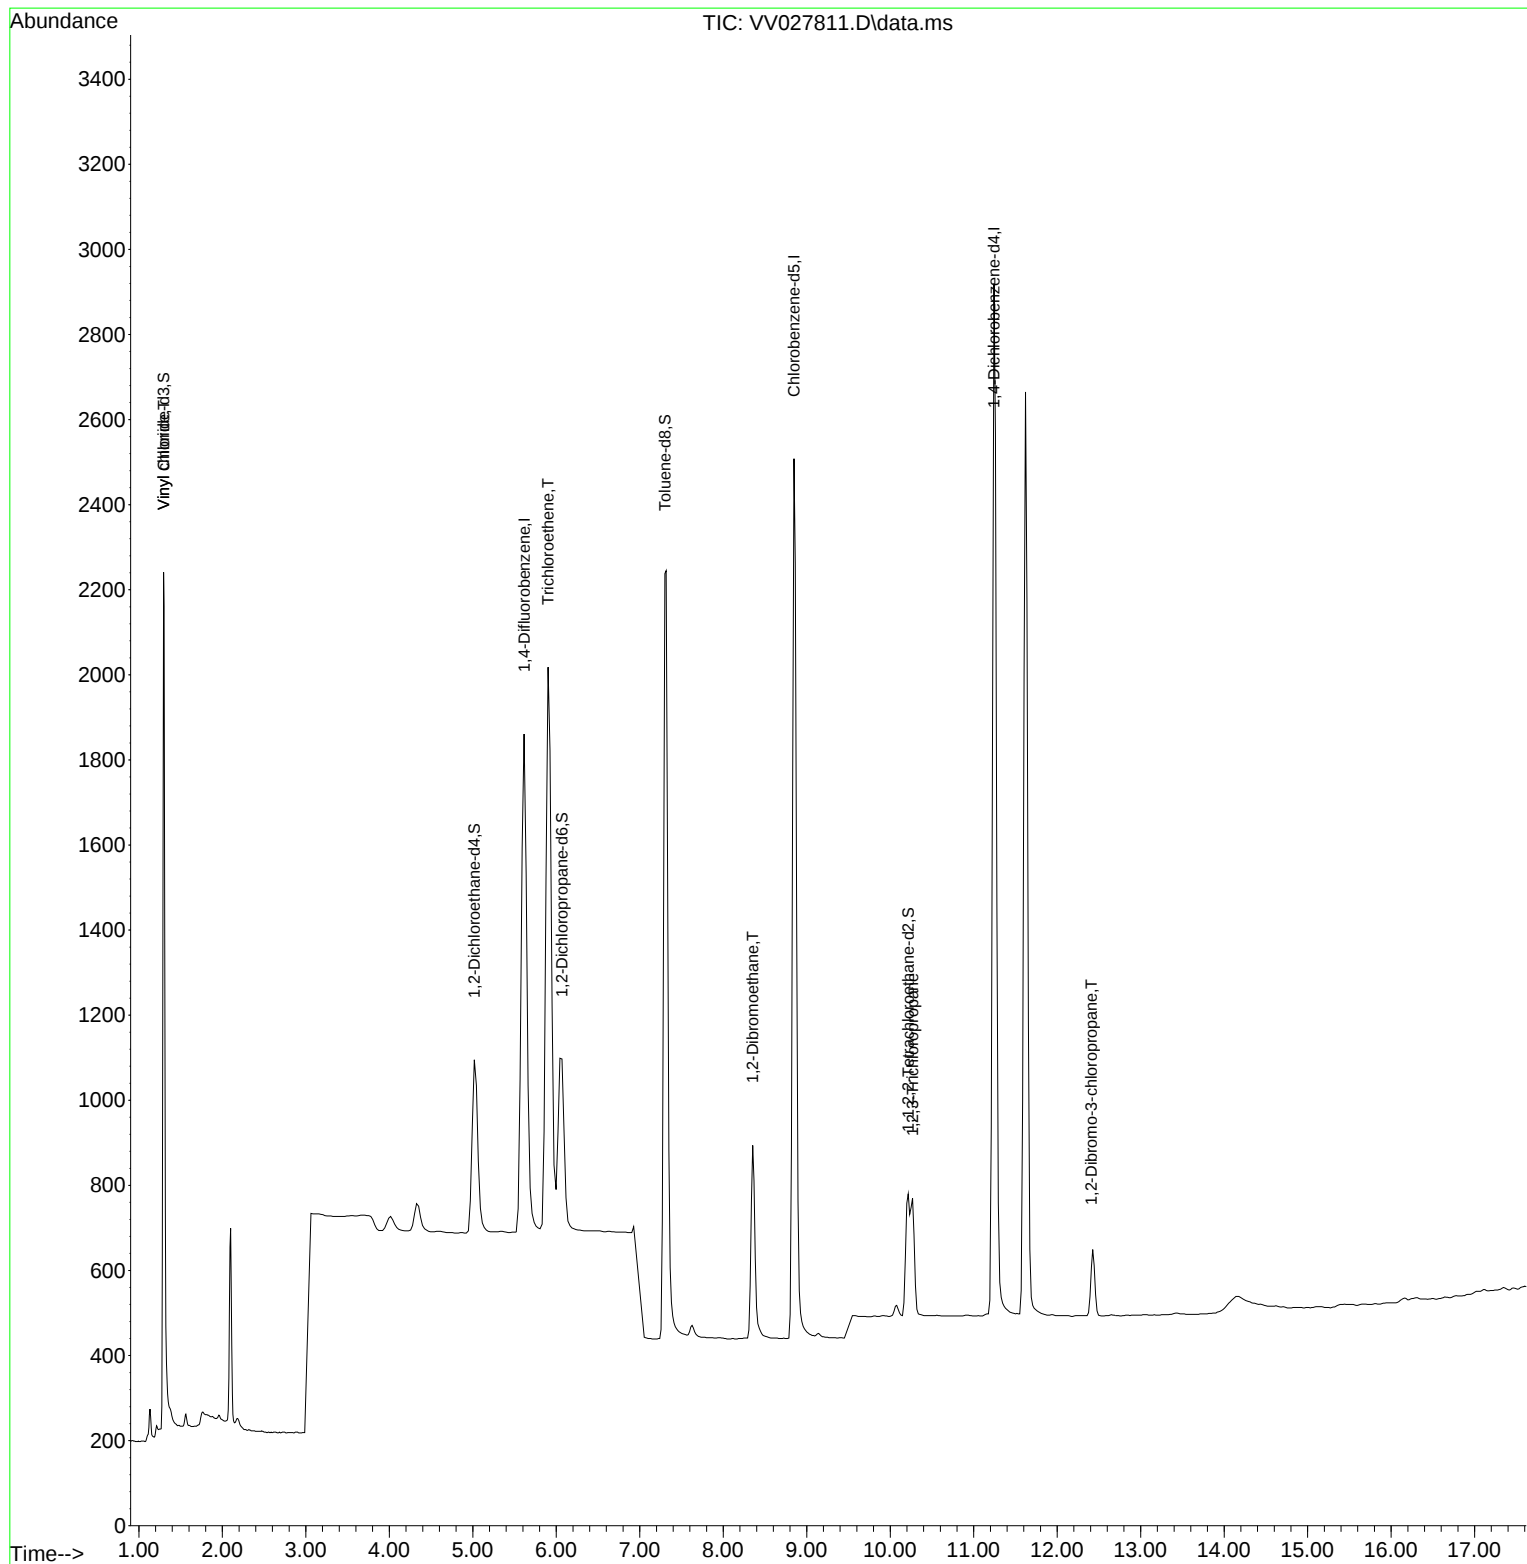


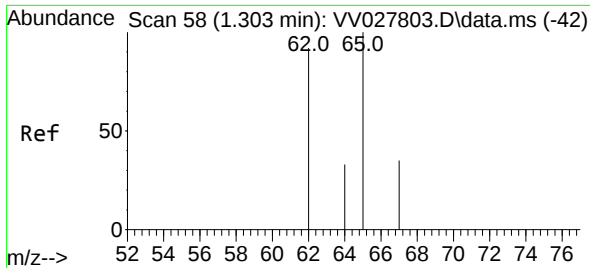

#3
 Vinyl chloride
 Concen: 0.502 ug/L
 RT: 1.296 min Scan# 51
 Delta R.T. -0.007 min
 Lab File: VV027811.D
 Acq: 13 Sep 2022 10:24




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5287


Tgt Ion: 62 Resp: 1285
 Ion Ratio Lower Upper
 62 100
 64 38.1 27.8 51.6

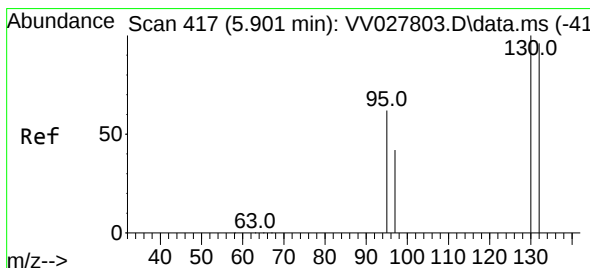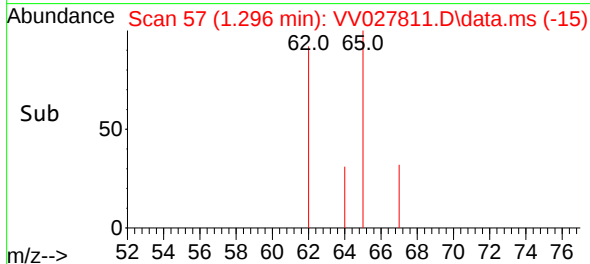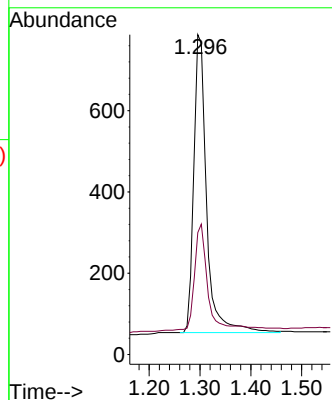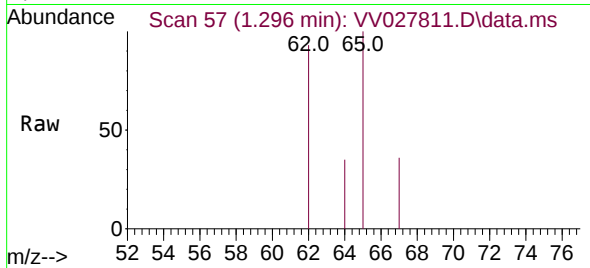

#6
 Trichloroethene
 Concen: 0.514 ug/L
 RT: 5.901 min Scan# 417
 Delta R.T. -0.024 min
 Lab File: VV027811.D
 Acq: 13 Sep 2022 10:24

Tgt Ion: 95 Resp: 1307
 Ion Ratio Lower Upper
 95 100
 97 71.0 50.6 94.0
 132 136.7 103.6 192.4
 130 144.5 104.9 194.7


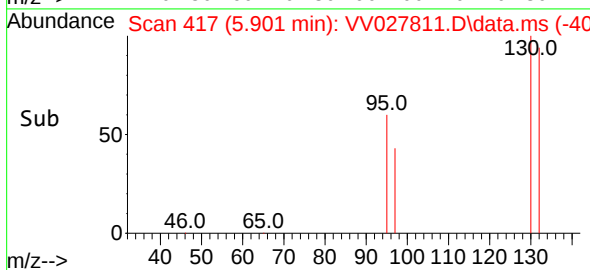
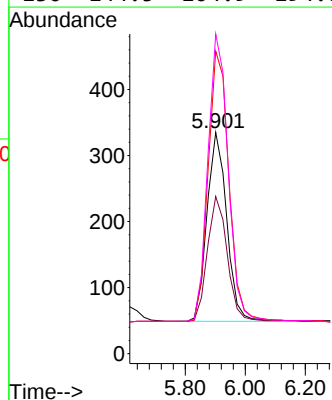
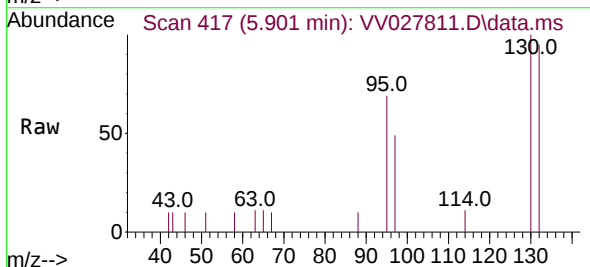


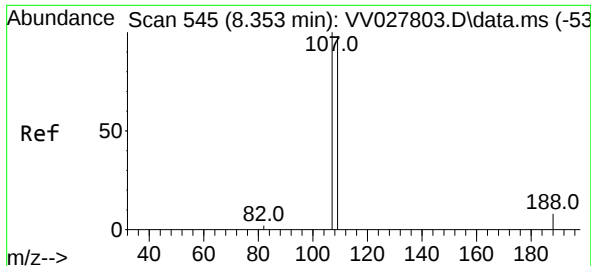

#9
1,2-Dibromoethane
Concen: 0.501 ug/L
RT: 8.353 min Scan# 545
Delta R.T. 0.000 min
Lab File: VV027811.D
Acq: 13 Sep 2022 10:24




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5287


Tgt Ion:107 Resp: 743
Ion Ratio Lower Upper
107 100
109 95.2 66.6 123.8
188 24.7 19.0 28.6

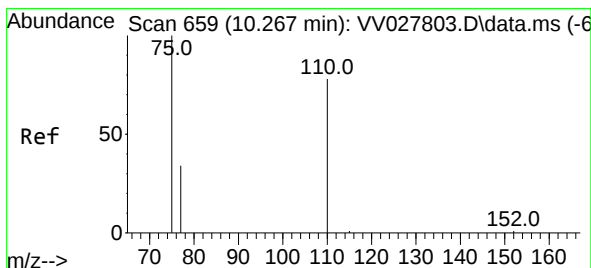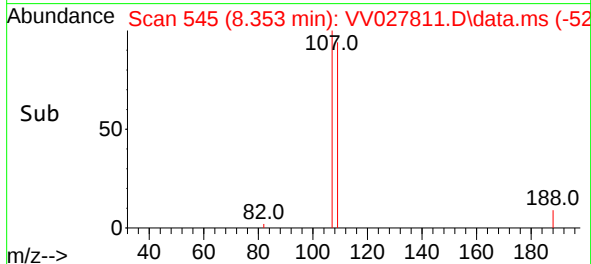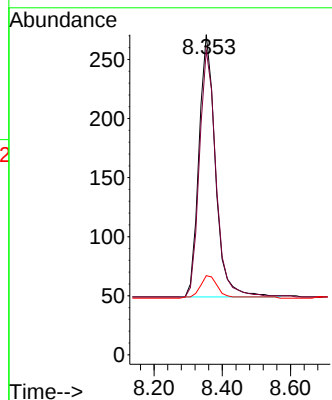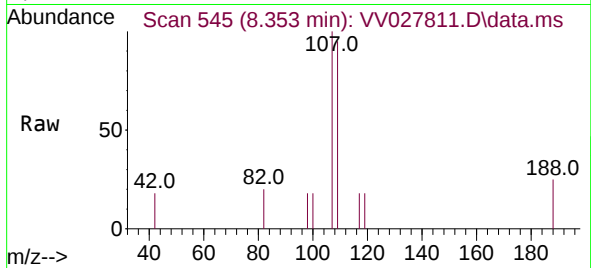

#12
1,2,3-Trichloropropane
Concen: 0.489 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV027811.D
Acq: 13 Sep 2022 10:24


Tgt Ion: 75 Resp: 435
Ion Ratio Lower Upper
75 100
110 69.4 55.5 83.3
77 37.2 26.2 39.2

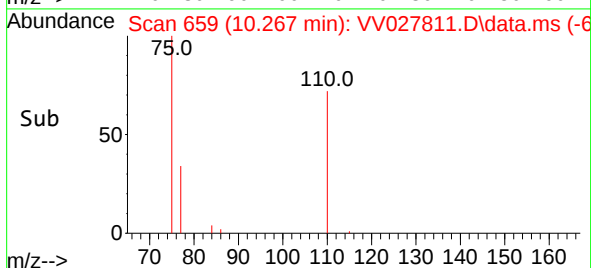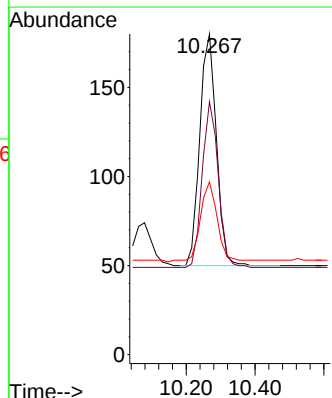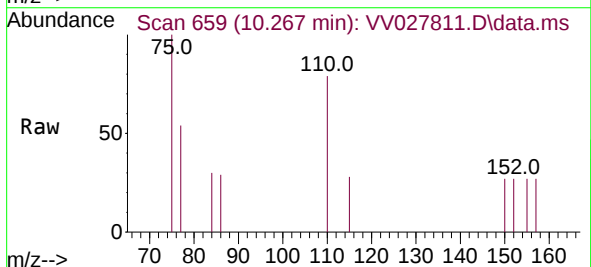

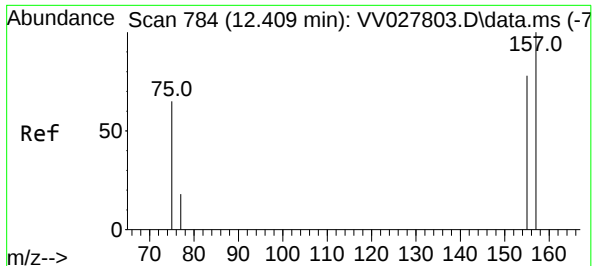

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.647 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. 0.000 min
 Lab File: VV027811.D
 Acq: 13 Sep 2022 10:24

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5287

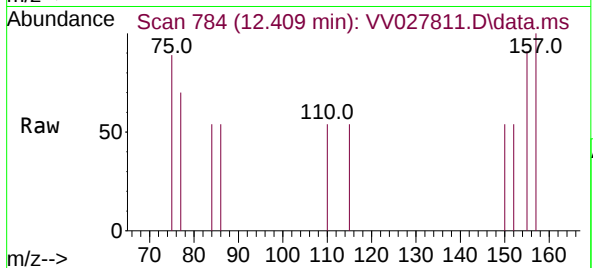

Tgt Ion:	75	Resp:	116
Ion	Ratio	Lower	Upper
75	100		
157	112.5	94.2	141.2
155	102.5	86.1	129.1

