

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091322\
 Data File : VV027812.D
 Acq On : 13 Sep 2022 11:42
 Operator : SY/MD
 Sample : VV0913WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK205

Quant Time: Sep 14 02:31:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 10 02:33:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	4258	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.848	117	3785	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	2588	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.296	65	1359	0.515	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.019	65	1039	0.523	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
7) 1,2-Dichloropropane-d6	6.068	67	697	0.553	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.301	98	3732	0.535	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
10) 1,1,2,2-Tetrachloroeth...	10.199	84	563	0.521	ug/L	-0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.375	75	6	0.035	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091322\
Data File : VV027812.D
Acq On : 13 Sep 2022 11:42
Operator : SY/MD
Sample : VV0913WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK205


Quant Time: Sep 14 02:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 10 02:33:14 2022
Response via : Initial Calibration

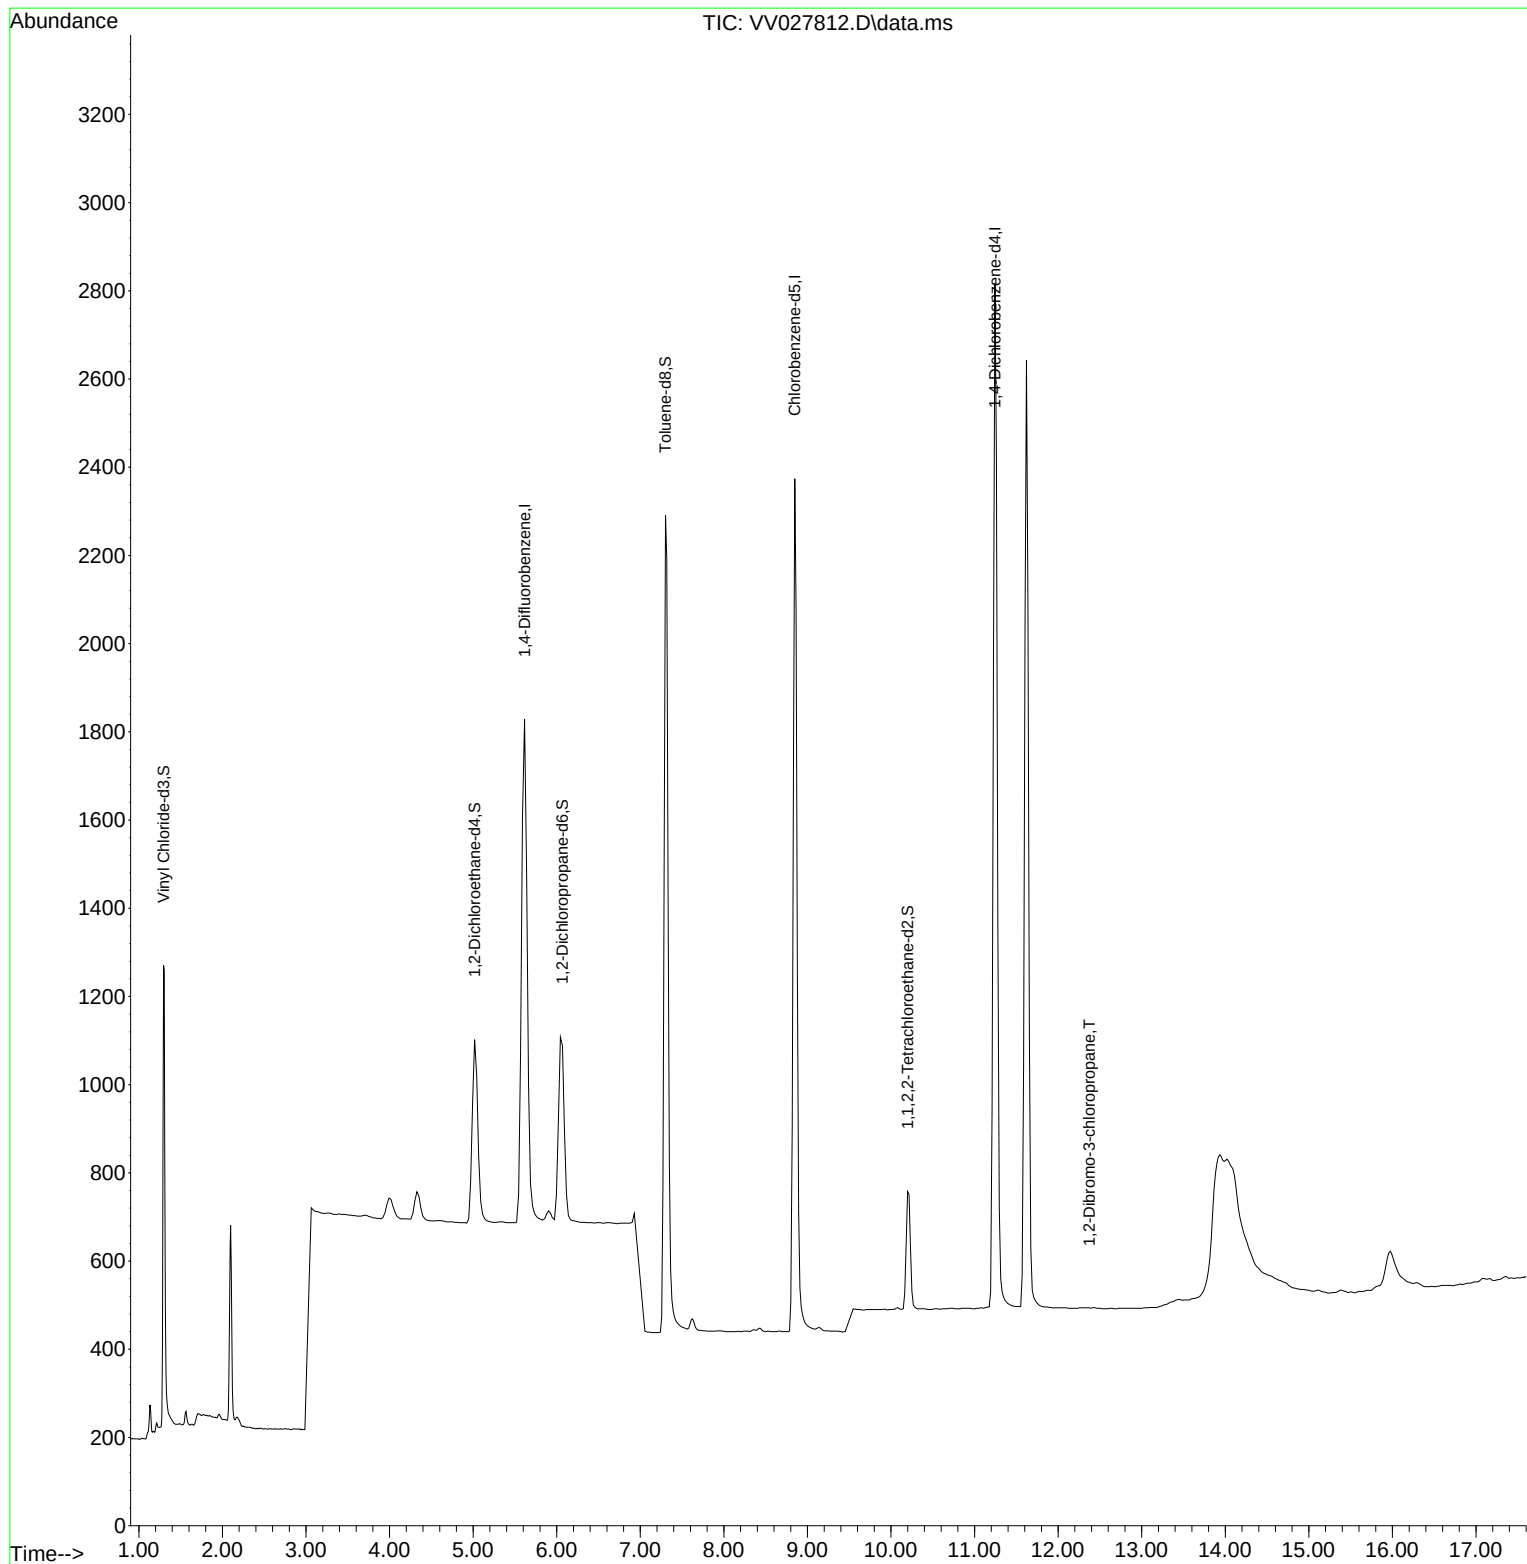

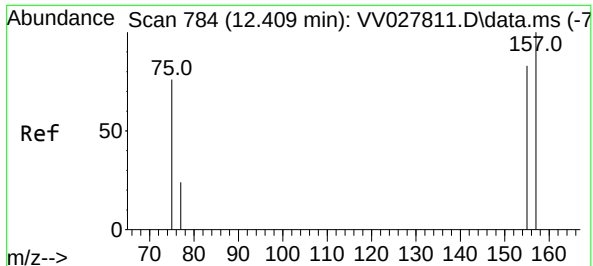

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.035 ug/L
 RT: 12.375 min Scan# 784
 Delta R.T. -0.034 min
 Lab File: VV027812.D
 Acq: 13 Sep 2022 11:42

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK205

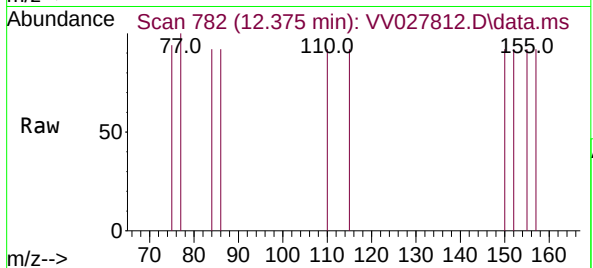

Tgt Ion: 75	Resp: 6
Ion Ratio	Lower Upper
75 100	
157 98.0	94.2 141.2
155 98.0	86.1 129.1

