
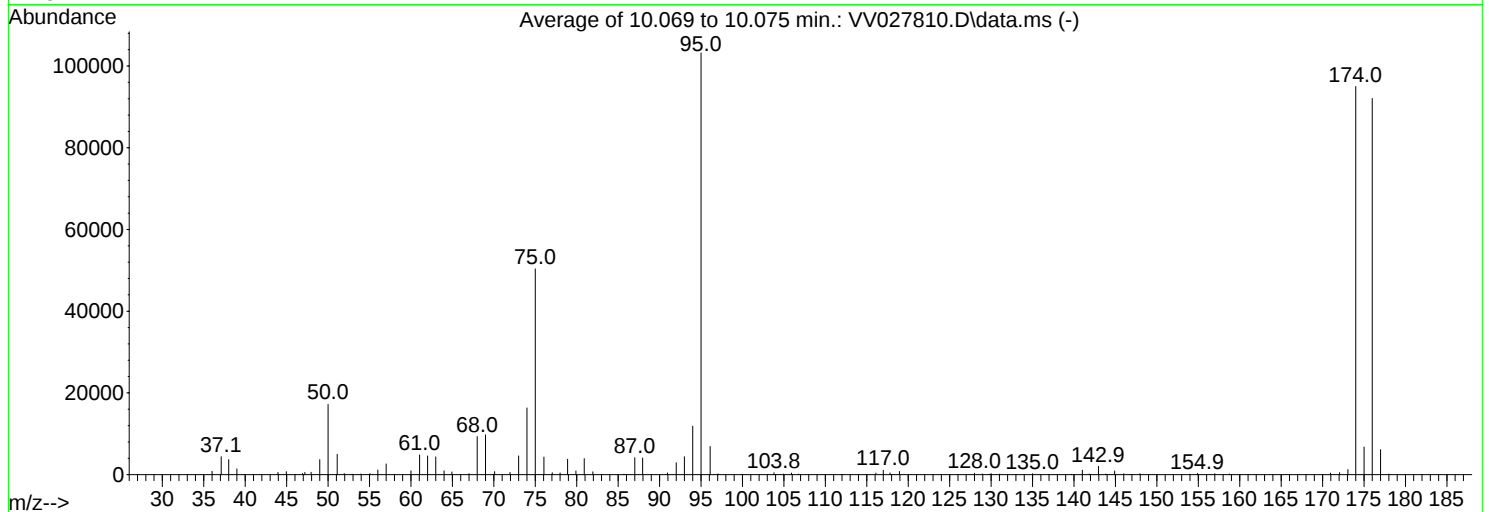


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091322\
Data File : VV027810.D
Acq On : 13 Sep 2022 09:51
Operator : SY/MD
Sample : BFB206
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB206

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
Title : TRACE VOA SOM01.0
Last Update : Sat Sep 10 02:33:14 2022

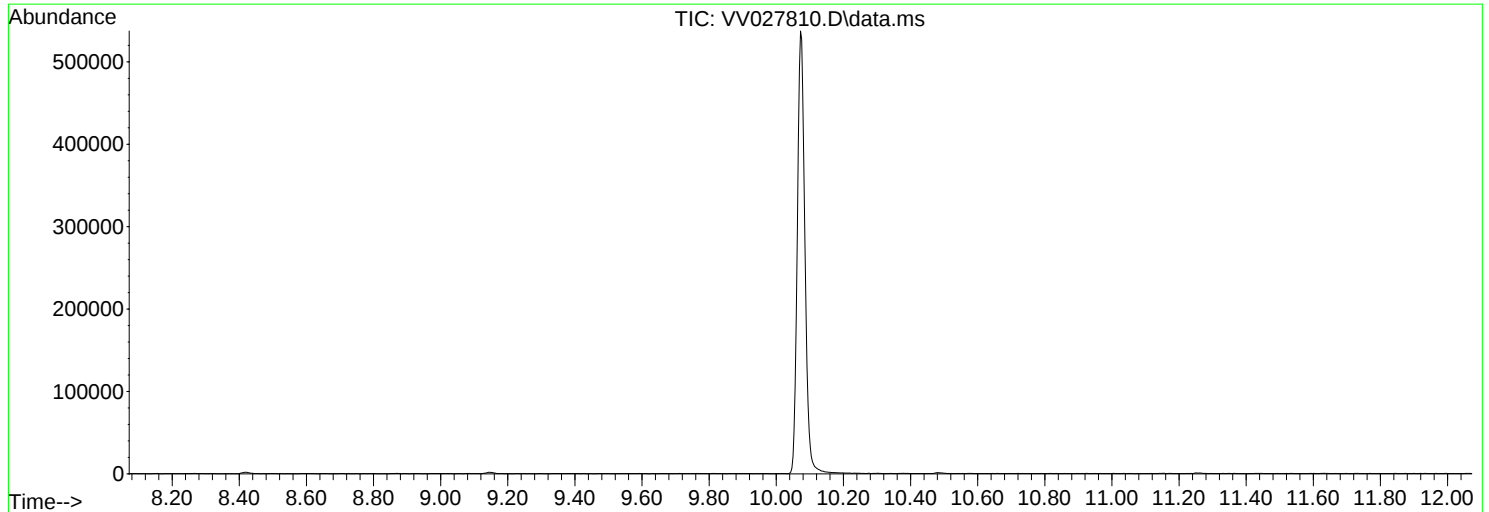

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	17200	PASS
75	95	30	80	48.8	50355	PASS
95	95	100	100	100.0	103229	PASS
96	95	5	9	6.7	6881	PASS
173	174	0.00	2	1.3	1250	PASS
174	95	50	120	92.0	94989	PASS
175	174	5	9	7.1	6786	PASS
176	174	95	101	96.9	92051	PASS
177	176	5	9	6.6	6118	PASS

Scan 2796 (10.030 min): VV027810.D\data.ms
BFB206

m/z	Abundance
40.00	159.0
44.00	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	746.0
37.10	3868.0
38.00	3485.0
39.00	1500.0
39.90	208.0
43.90	751.0
45.00	682.0
46.00	152.0
46.90	832.0
48.00	583.0
49.00	3425.0
50.00	16448.0
51.10	4707.0
52.00	270.0
52.90	153.0
54.00	138.0
55.00	222.0
56.00	1203.0
57.00	2508.0
58.00	120.0
60.00	1020.0
61.10	4683.0
62.00	4296.0
63.00	4363.0
64.00	908.0
65.00	618.0
67.10	220.0
68.00	9040.0
69.00	9433.0
70.10	762.0
71.90	569.0
73.00	4403.0
74.00	15824.0
75.00	48200.0
76.10	4035.0
77.00	463.0
77.90	344.0
78.90	3565.0
79.90	865.0
80.90	3568.0
81.90	588.0
85.60	105.0
87.00	4129.0
87.90	3875.0
90.90	455.0
92.00	2754.0
93.00	4276.0
94.00	11123.0
95.00	98632.0
96.10	6546.0
97.10	166.0
103.80	422.0
104.90	155.0
105.90	368.0
106.70	151.0
116.10	359.0
117.00	994.0
117.80	373.0
118.90	728.0
128.00	331.0
128.90	208.0
129.80	363.0
131.10	129.0
135.00	256.0
139.70	132.0
141.00	980.0
141.90	159.0
143.00	1909.0
143.80	109.0
144.90	932.0
146.00	242.0
148.00	251.0
154.10	101.0
154.90	313.0
157.00	232.0
158.80	163.0
171.00	382.0
172.00	444.0
173.10	1157.0
174.00	87752.0
175.00	6627.0
176.00	86416.0
177.00	6026.0
178.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	866.0
37.10	4612.0
38.00	3740.0
39.00	1423.0
39.90	246.0
43.90	710.0
44.90	767.0
46.10	137.0
47.20	797.0
48.00	622.0
49.00	3875.0
50.00	17888.0
51.10	5086.0
52.00	277.0
52.90	144.0
53.90	150.0
55.00	237.0
56.00	1151.0
57.00	2773.0
58.00	135.0
60.00	959.0
61.00	4869.0
62.00	4672.0
63.00	4525.0
64.00	974.0
64.90	715.0
67.00	262.0
68.00	9622.0
69.00	10050.0
70.10	776.0
72.00	564.0
73.00	4819.0
74.00	16960.0
75.00	52104.0
76.00	4506.0
77.10	508.0
78.00	455.0
78.90	3866.0
79.90	946.0
80.90	4046.0
82.00	734.0
85.70	102.0
87.00	4301.0
88.00	4208.0
91.00	472.0
92.00	3061.0
93.00	4542.0
94.00	12251.0
95.00	106984.0
96.10	7122.0
97.00	197.0
103.80	499.0
105.00	164.0
105.90	404.0
106.80	122.0
111.90	103.0
114.90	120.0
116.10	414.0
117.00	1105.0
117.80	434.0
118.90	828.0
128.00	390.0
129.00	219.0
130.00	411.0
131.10	163.0
135.00	247.0
136.90	112.0
139.70	114.0
141.00	1138.0
141.80	181.0
142.90	2076.0
143.90	173.0
144.90	920.0
146.00	264.0
146.80	101.0
148.00	255.0
153.90	103.0
154.90	332.0
157.00	257.0
158.70	165.0
171.00	420.0
172.10	537.0
173.00	1294.0
174.00	98512.0
175.00	7006.0
176.00	95448.0
177.00	6388.0
178.00	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	878.0
37.10	4724.0
38.00	3766.0
39.00	1269.0
39.90	298.0
44.00	633.0
44.90	736.0
47.20	827.0
47.90	564.0
49.00	3795.0
50.00	17264.0
51.10	5086.0
51.90	280.0
52.90	121.0
53.90	171.0
55.10	273.0
56.00	1095.0
57.00	2622.0
58.00	127.0
60.00	870.0
61.00	4859.0
62.00	4733.0
63.00	4132.0
64.00	978.0
64.90	721.0
66.90	265.0
68.00	9277.0
69.00	9810.0
70.10	734.0
72.00	536.0
73.00	4550.0
74.00	16186.0
75.00	50760.0
76.00	4377.0
77.10	478.0
78.10	513.0
78.90	3806.0
79.90	882.0
80.90	4179.0
81.90	778.0
85.80	119.0
87.00	4073.0
87.90	4128.0
91.00	409.0
92.00	2997.0
93.00	4400.0
94.00	12198.0
95.00	104072.0
96.10	6974.0
97.00	207.0
103.80	515.0
105.00	163.0
105.90	432.0
106.80	107.0
114.90	145.0
116.10	404.0
117.00	1089.0
117.80	507.0
119.00	835.0
128.00	385.0
129.00	214.0
130.00	429.0
131.00	185.0
135.00	187.0
136.90	146.0
141.00	1161.0
141.80	198.0
142.90	2081.0
143.90	207.0
144.90	838.0
146.00	224.0
147.90	249.0
153.80	114.0
154.90	286.0
157.00	274.0
158.70	175.0
170.90	422.0
172.10	562.0
173.00	1299.0
174.00	98704.0
175.00	6725.0
176.00	94288.0
177.00	5939.0
178.00	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206