

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032066.D
 Acq On : 13 Sep 2023 11:11
 Operator : SY/MD
 Sample : 04332-02ME
 Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 14 06:21:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	248387	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	239998	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	120820	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	58894	37.886	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.780%
7) Chloroethane-d5	1.503	69	19322	14.179	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	28.360%#
11) 1,1-Dichloroethene-d2	2.034	65	25194	34.612	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.220%
21) 2-Butanone-d5	3.802	46	100484	82.188	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.190%
24) Chloroform-d	4.246	84	116486	34.284	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.560%#
26) 1,2-Dichloroethane-d4	4.940	65	77454	34.350	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.700%#
32) Benzene-d6	4.953	84	243826	37.232	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.460%
36) 1,2-Dichloropropane-d6	5.989	67	83869	39.789	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	79.580%
41) Toluene-d8	7.246	98	215539	35.720	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	71.440%#
43) trans-1,3-Dichloroprop...	7.558	79	38430	35.176	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.360%
47) 2-Hexanone-d5	8.043	63	61542	95.259	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.260%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	106436	39.076	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.160%
66) 1,2-Dichlorobenzene-d4	11.567	152	82859	37.621	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.240%#
Target Compounds						
15) Methyl Acetate	2.381	43	2840	1.463	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032066.D
Acq On : 13 Sep 2023 11:11
Operator : SY/MD
Sample : 04332-02ME
Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 14 06:21:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 14 06:19:55 2023
Response via : Initial Calibration

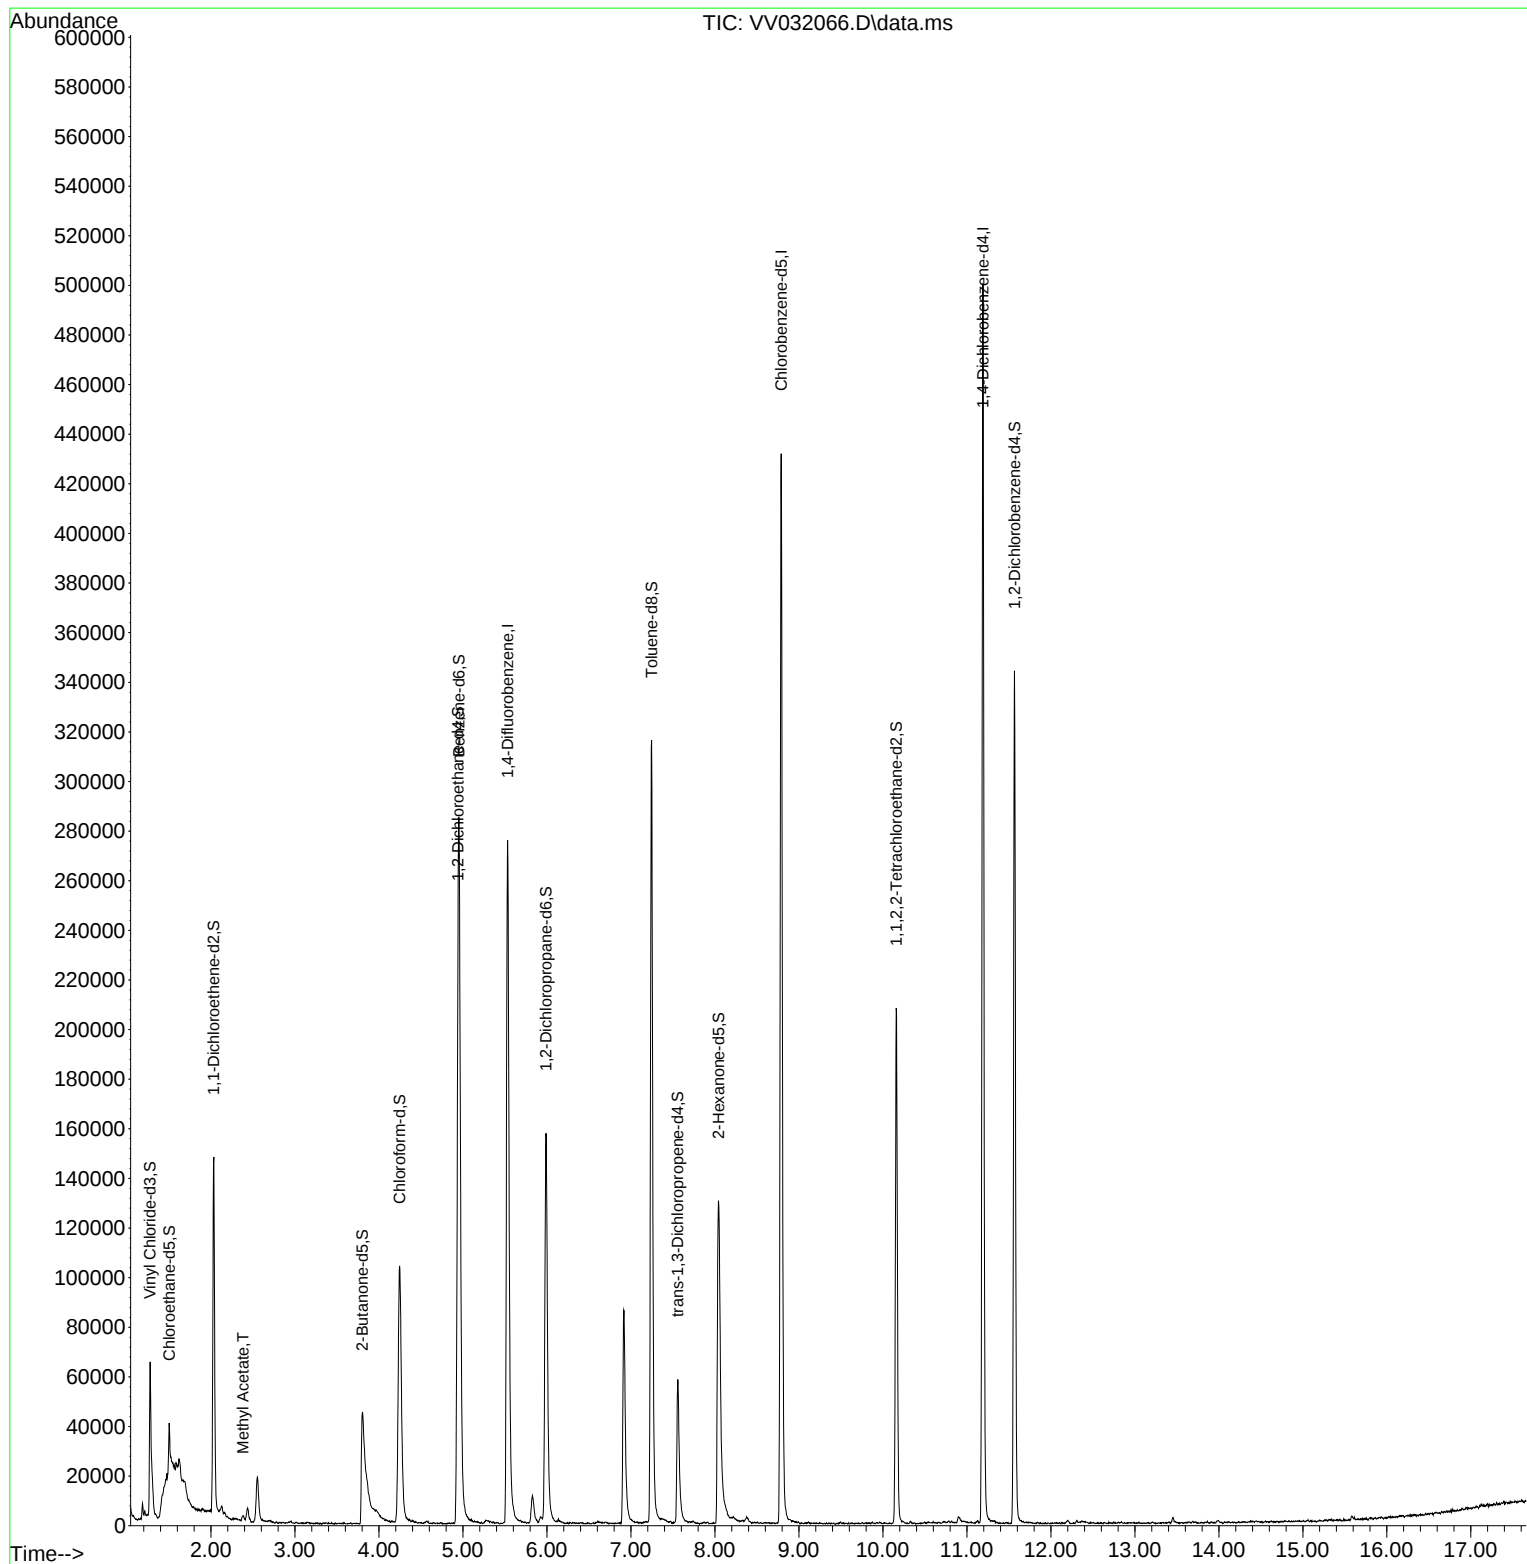

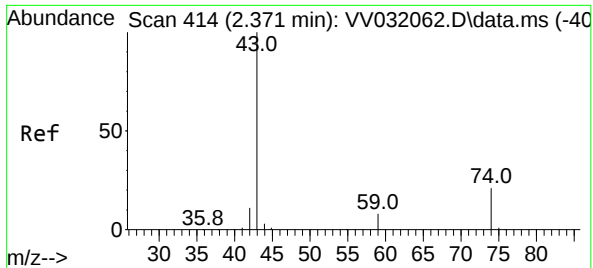

#15
Methyl Acetate
Concen: 1.463 ug/L
RT: 2.381 min Scan# 41
Delta R.T. 0.010 min
Lab File: VV032066.D
Acq: 13 Sep 2023 11:11

Instrument :
MSVOA_V
ClientSampleId :

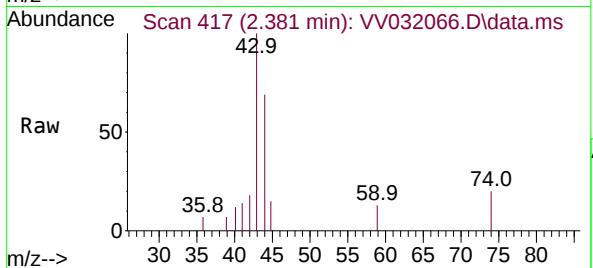

Tgt Ion: 43 Resp: 2840
Ion Ratio Lower Upper
43 100
74 21.8 17.9 26.9

