

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091323\
 Data File : VW032082.D
 Acq On : 13 Sep 2023 17:27
 Operator : SY/MD
 Sample : 04330-10ME
 Misc : 5.88g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 14 06:24:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	353228	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	336510	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	181341	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	64980	29.394	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	58.780%#
7) Chloroethane-d5	1.503	69	14658	7.564	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	15.120%#
11) 1,1-Dichloroethene-d2	2.031	65	27953	27.004	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.000%#
21) 2-Butanone-d5	3.809	46	135846	78.133	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.130%
24) Chloroform-d	4.249	84	140814	29.143	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	58.280%#
26) 1,2-Dichloroethane-d4	4.941	65	96034	29.949	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	59.900%#
32) Benzene-d6	4.957	84	290944	31.685	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	63.380%#
36) 1,2-Dichloropropane-d6	5.992	67	99442	33.646	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	67.300%#
41) Toluene-d8	7.246	98	255253	30.169	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	60.340%#
43) trans-1,3-Dichloroprop...	7.558	79	46022	30.043	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.080%
47) 2-Hexanone-d5	8.047	63	86321	95.293	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.290%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	136716	35.797	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	71.600%
66) 1,2-Dichlorobenzene-d4	11.567	152	106355	32.173	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.340%#
Target Compounds						
39) cis-1,3-Dichloropropene	6.921	75	2724	0.611	ug/L	Qvalue # 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032082.D
Acq On : 13 Sep 2023 17:27
Operator : SY/MD
Sample : 04330-10ME
Misc : 5.88g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 14 06:24:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 14 06:19:55 2023
Response via : Initial Calibration

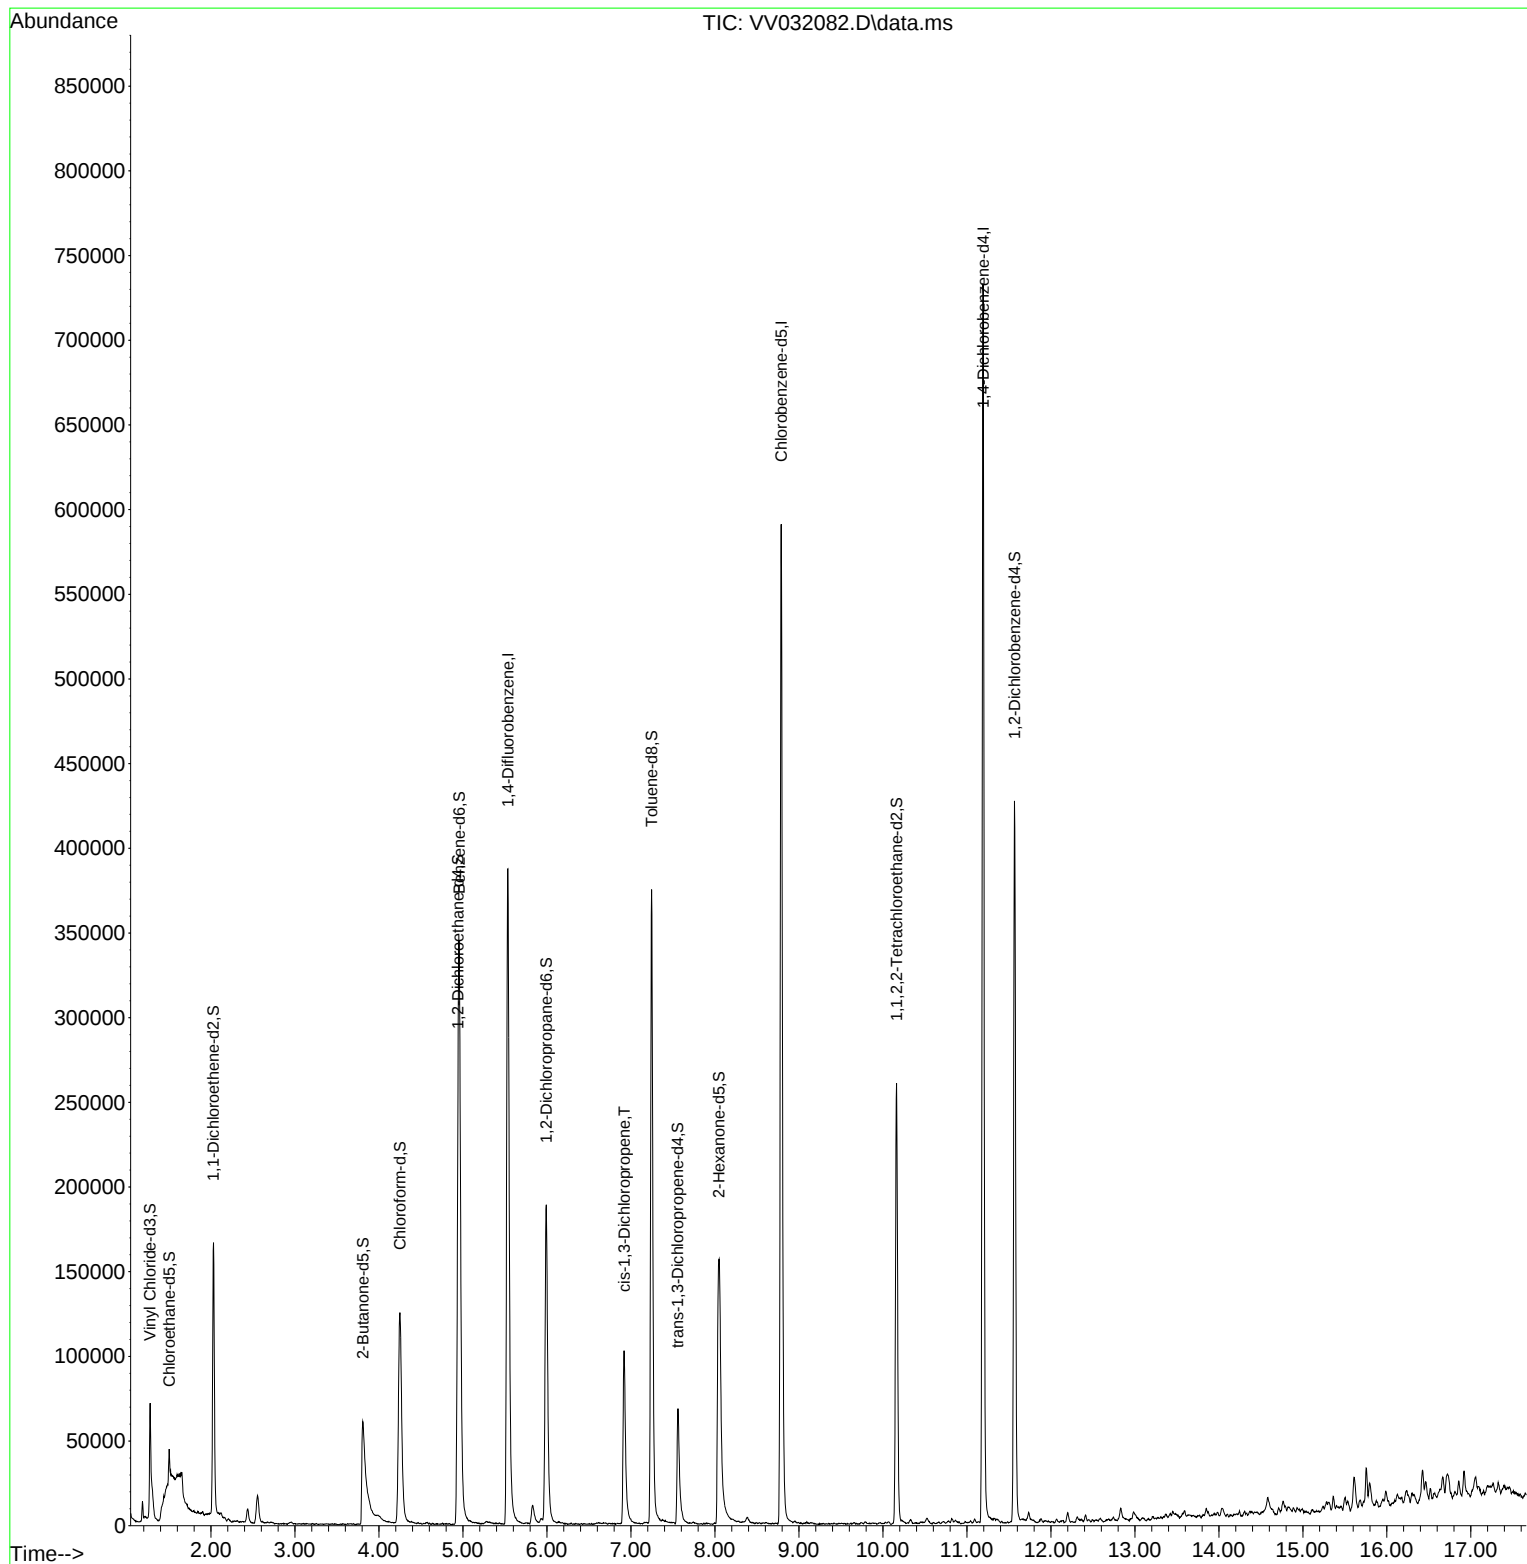

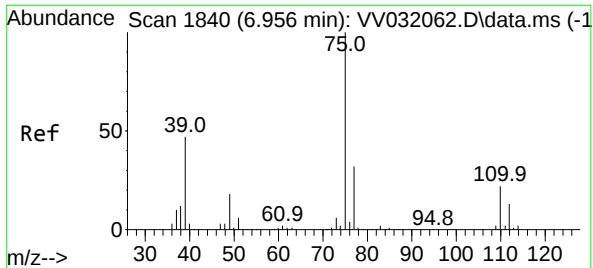

#39
 cis-1,3-Dichloropropene
 Concen: 0.611 ug/L
 RT: 6.921 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV032082.D
 Acq: 13 Sep 2023 17:27

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 2724
 Ion Ratio Lower Upper
 75 100
 77 54.7 21.4 39.8#

