




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032072.D
 Acq On : 13 Sep 2023 13:31
 Operator : SY/MD
 Sample : 04387-04ME
 Misc : 3.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6ME

Manual IntegrationsAPPROVED

Quant Time: Sep 14 06:22:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2023
 Supervised By :Semsettin Yesilyurt 09/18/2023

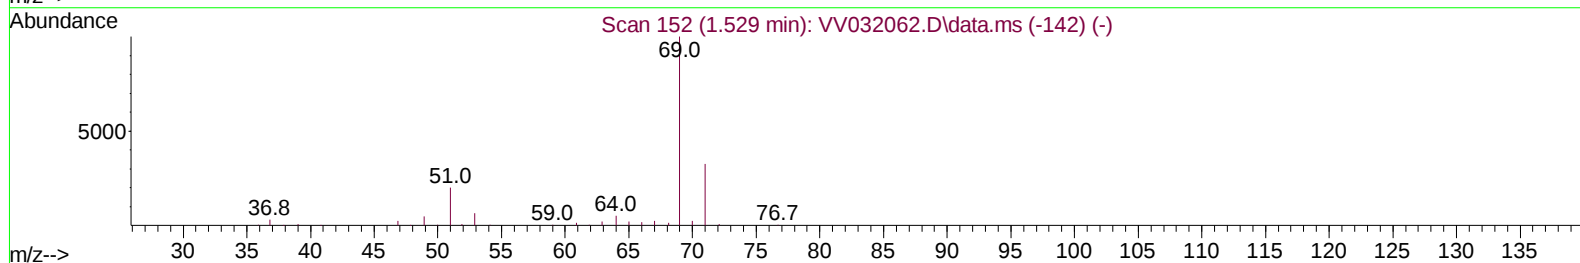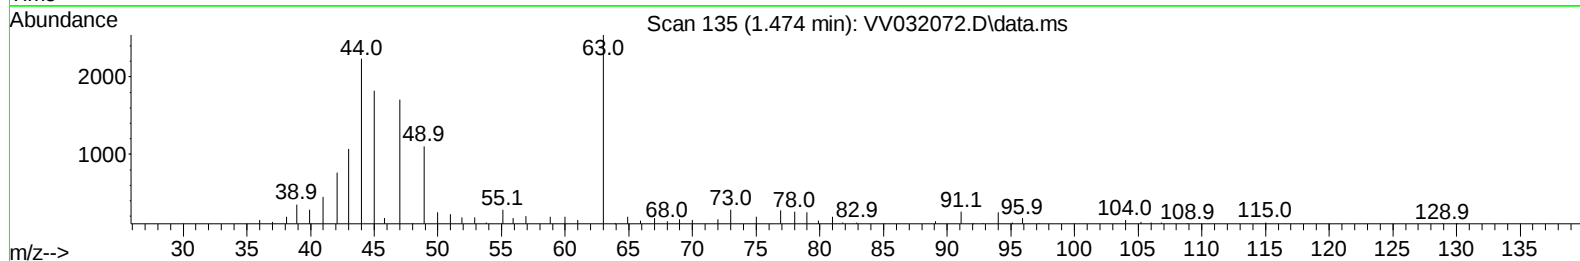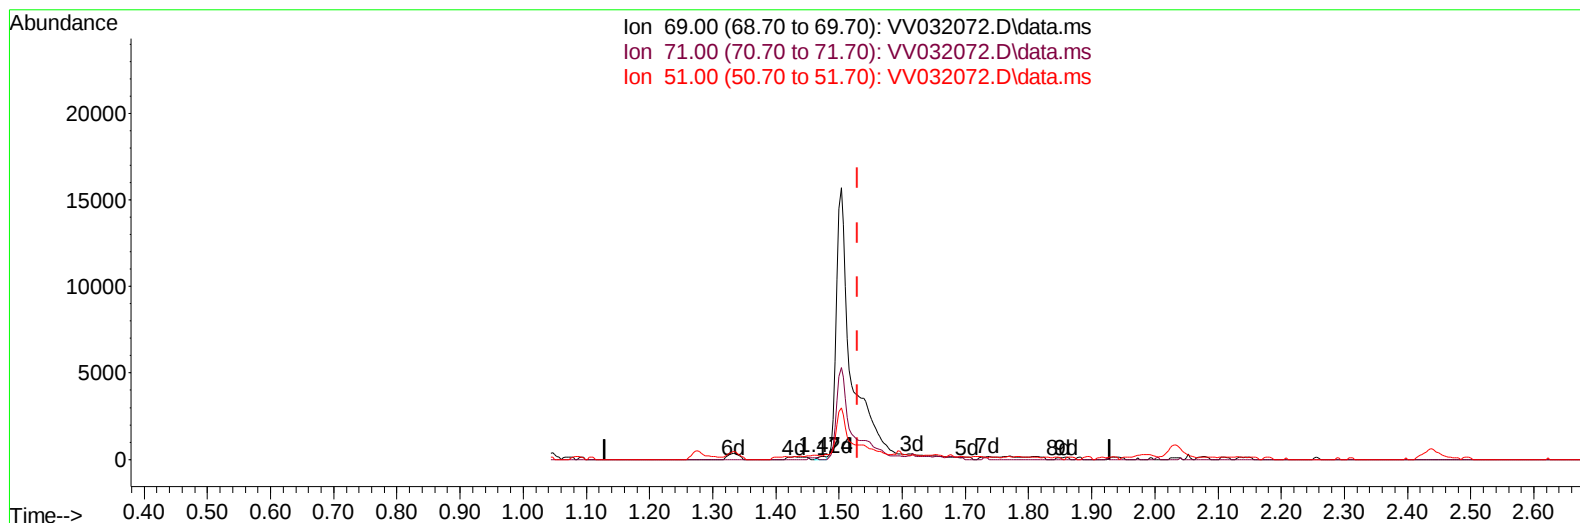

TIC: VV032072.D\data.ms

(7) Chloroethane-d5 (S)

1.474min (-0.055) 0.09 ug/L

response 164

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	37.80
51.00	25.40	18.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032072.D
 Acq On : 13 Sep 2023 13:31
 Operator : SY/MD
 Sample : 04387-04ME
 Misc : 3.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6ME

Manual IntegrationsAPPROVED

Quant Time: Sep 14 06:22:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2023
 Supervised By :Semsettin Yesilyurt 09/18/2023

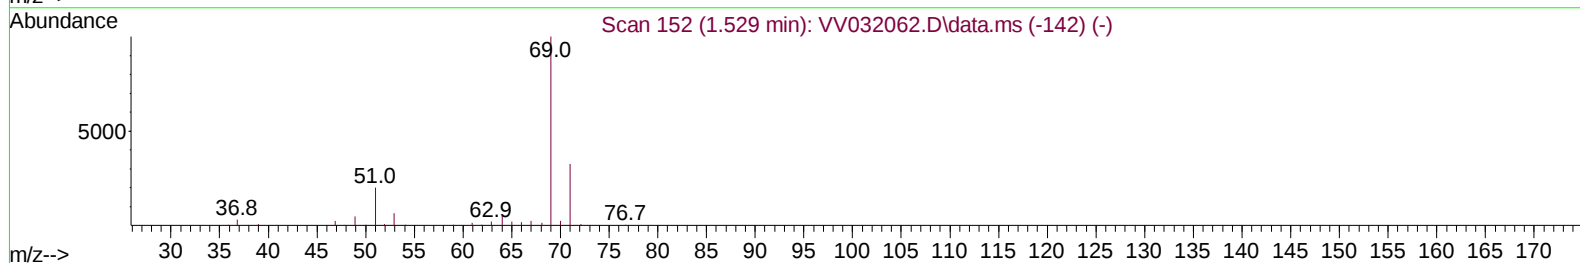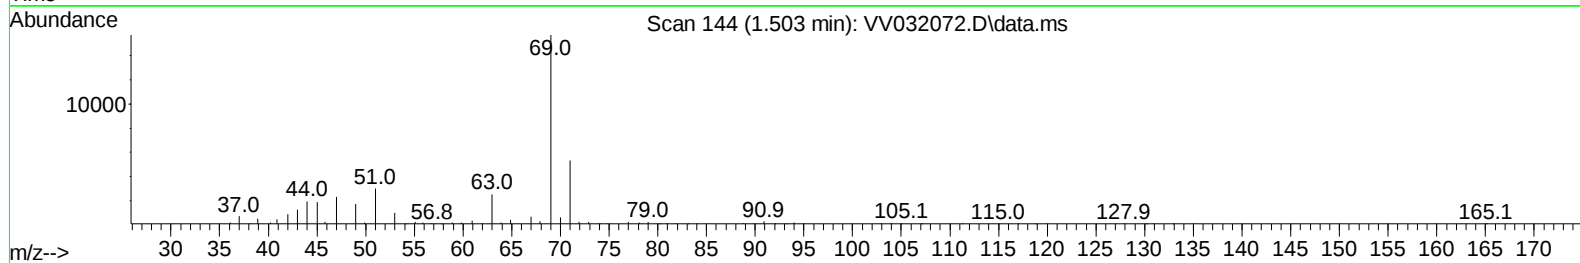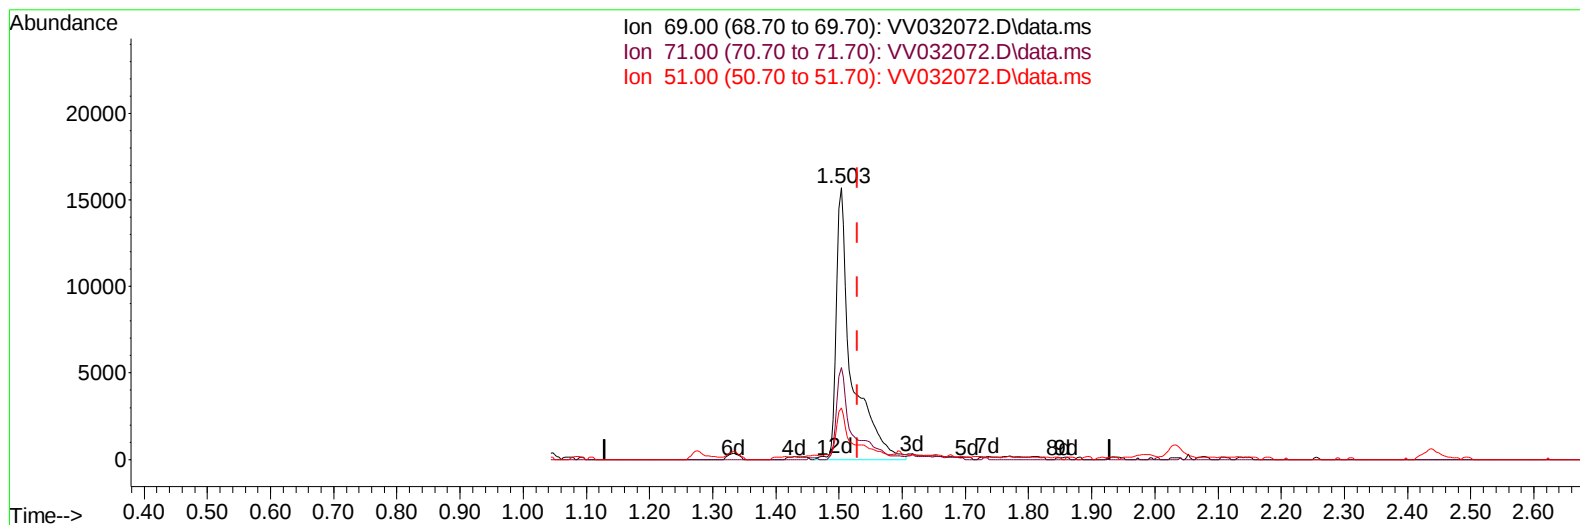

TIC: VV032072.D\data.ms

(7) Chloroethane-d5 (S)

1.503min (-0.026) 15.09 ug/L m

response 26486

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.23#
51.00	25.40	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032072.D
 Acq On : 13 Sep 2023 13:31
 Operator : SY/MD
 Sample : 04387-04ME
 Misc : 3.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2023
 Supervised By :Semsettin Yesilyurt 09/18/2023

Quant Time: Sep 14 06:22:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	319950	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	311170	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	163702	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	85467	42.683	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	85.360%		
7) Chloroethane-d5	1.503	69	26486m	15.089	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130	Recovery =	30.180%#		
11) 1,1-Dichloroethene-d2	2.034	65	35434	37.792	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery =	75.580%		
21) 2-Butanone-d5	3.805	46	164114	104.209	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery =	104.210%		
24) Chloroform-d	4.249	84	171901	39.277	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	78.560%		
26) 1,2-Dichloroethane-d4	4.940	65	115358	39.717	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	79.440%		
32) Benzene-d6	4.957	84	355934	41.919	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	83.840%		
36) 1,2-Dichloropropane-d6	5.992	67	125013	45.743	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	91.480%		
41) Toluene-d8	7.246	98	314054	40.142	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	80.280%		
43) trans-1,3-Dichloroprop...	7.558	79	56481	39.873	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	79.740%		
47) 2-Hexanone-d5	8.043	63	101249	120.874	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery =	120.870%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	164457	46.567	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	93.140%		
66) 1,2-Dichlorobenzene-d4	11.567	152	127846	42.841	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	85.680%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032072.D
Acq On : 13 Sep 2023 13:31
Operator : SY/MD
Sample : 04387-04ME
Misc : 3.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6ME

Manual IntegrationsAPPROVED

Quant Time: Sep 14 06:22:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 14 06:19:55 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2023
Supervised By :Semsettin Yesilyurt 09/18/2023

