

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032075.D
 Acq On : 13 Sep 2023 14:42
 Operator : SY/MD
 Sample : 04387-08ME
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4ME

Quant Time: Sep 14 06:23:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 14 06:19:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	244843	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	240080	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	127764	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	70913	46.278	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.560%
7) Chloroethane-d5	1.503	69	20490	15.254	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	30.500%#
11) 1,1-Dichloroethene-d2	2.031	65	29433	41.021	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.040%
21) 2-Butanone-d5	3.805	46	134201	111.355	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.360%
24) Chloroform-d	4.249	84	141584	42.274	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.540%
26) 1,2-Dichloroethane-d4	4.940	65	96187	43.276	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.560%
32) Benzene-d6	4.957	84	293849	44.855	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.720%
36) 1,2-Dichloropropane-d6	5.992	67	102613	48.665	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.320%
41) Toluene-d8	7.246	98	258918	42.894	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.780%
43) trans-1,3-Dichloroprop...	7.558	79	46385	42.442	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.880%
47) 2-Hexanone-d5	8.046	63	85681	132.577	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	132.580%#
56) 1,1,2,2-Tetrachloroeth...	10.162	84	137871	50.599	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	11.567	152	106430	45.696	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.400%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.381	43	28153	14.716	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032075.D
Acq On : 13 Sep 2023 14:42
Operator : SY/MD
Sample : 04387-08ME
Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4ME

Quant Time: Sep 14 06:23:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 14 06:19:55 2023
Response via : Initial Calibration

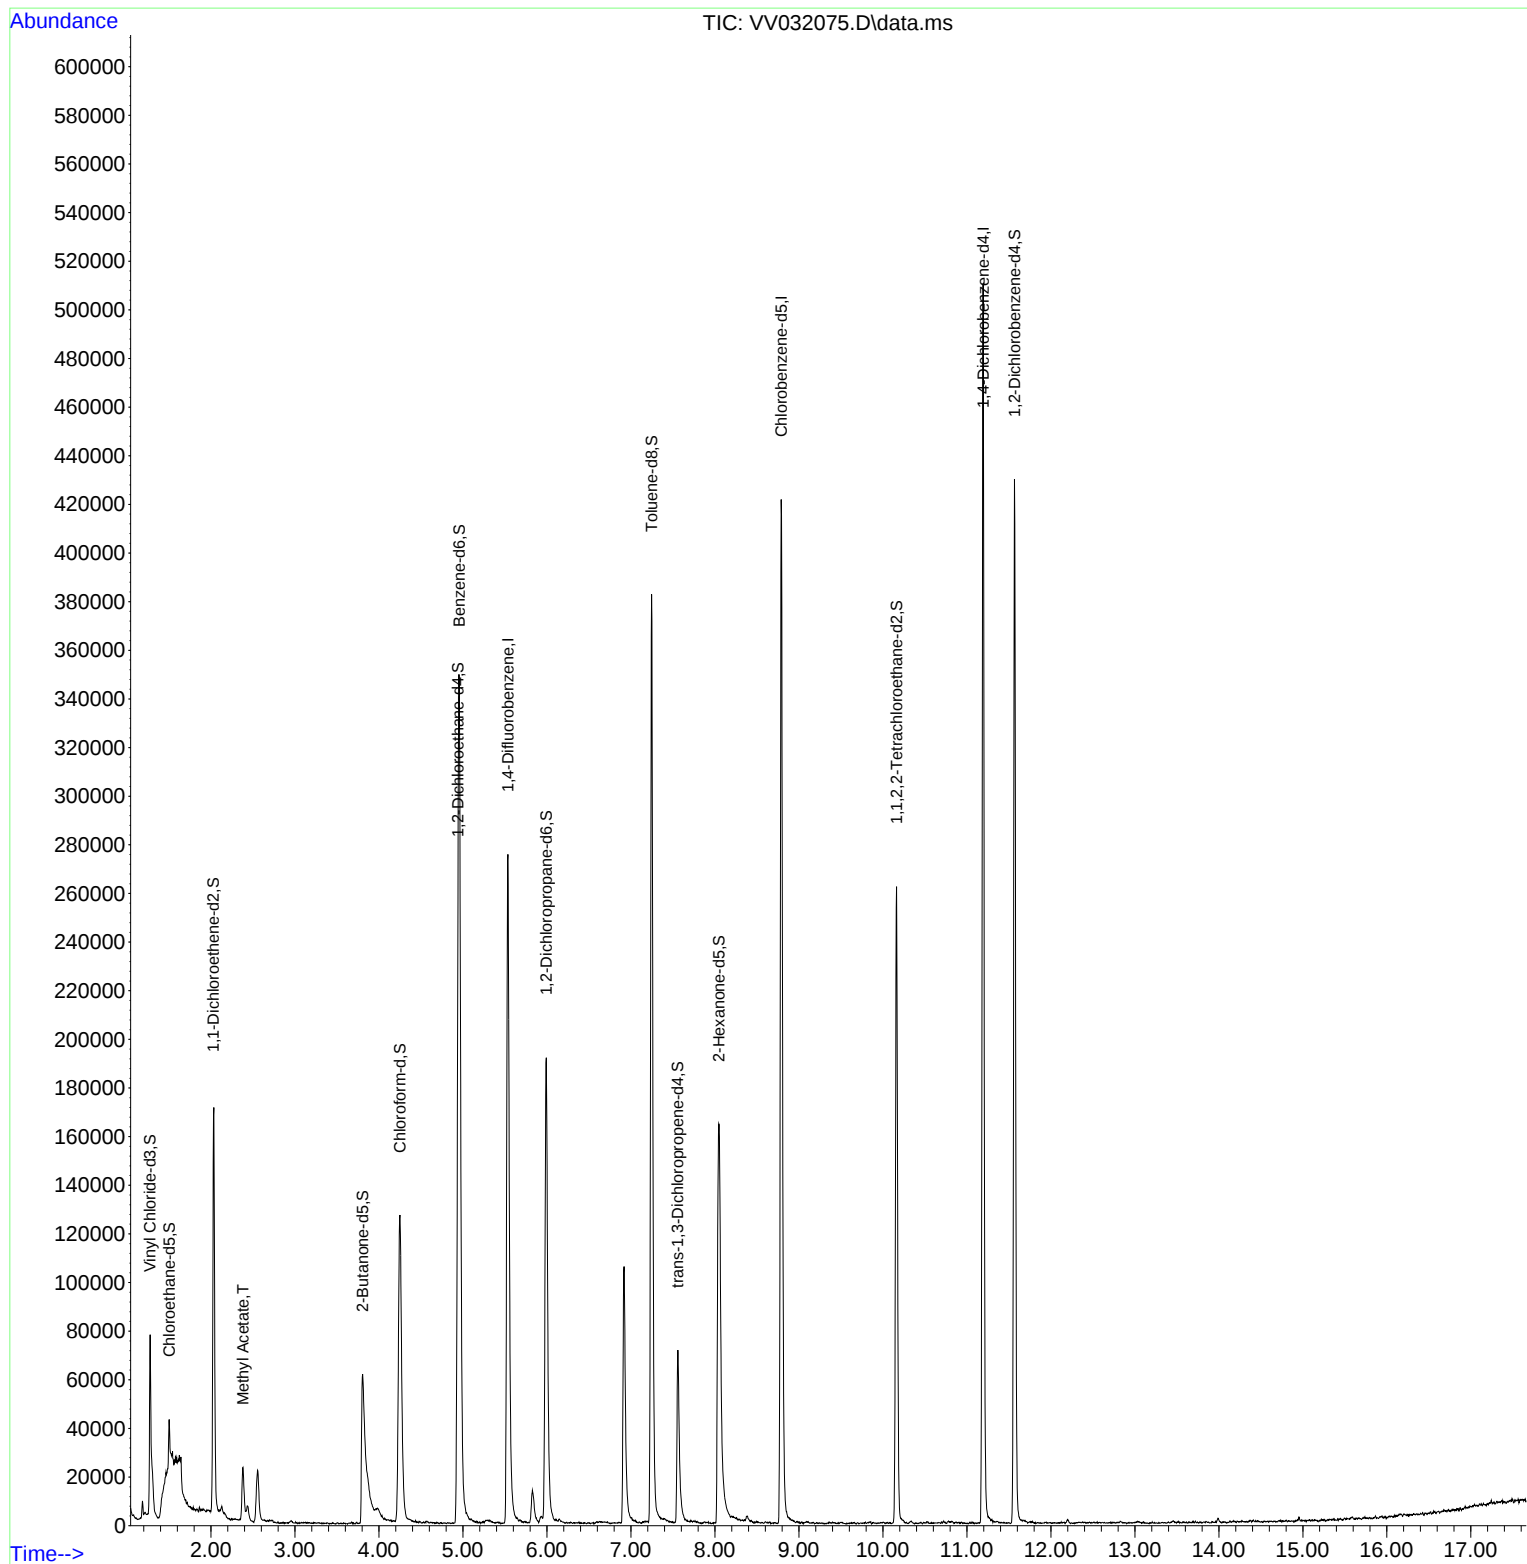

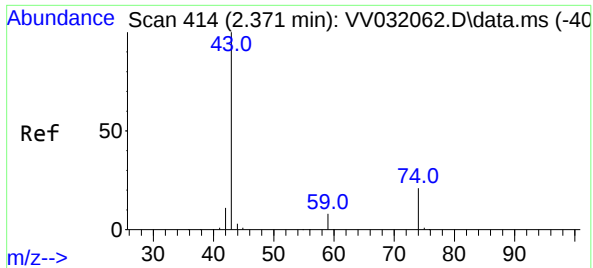

#15
Methyl Acetate
Concen: 14.716 ug/L
RT: 2.381 min Scan# 41
Delta R.T. 0.010 min
Lab File: VV032075.D
Acq: 13 Sep 2023 14:42

Instrument :
MSVOA_V
ClientSampleId :
C0AB4ME

Tgt Ion: 43 Resp: 28153
Ion Ratio Lower Upper
43 100
74 22.5 17.9 26.9

