

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032063.D
 Acq On : 13 Sep 2023 09:47
 Operator : SY/MD
 Sample : VV0913MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	97471	104835	13.69%	1.668%
2	1.529	146	152	166	rVB	82651	97947	12.79%	1.559%
3	2.056	308	316	331	rBV	152659	220167	28.76%	3.504%
4	2.446	429	437	448	rBV3	6549	11035	1.44%	0.176%
5	2.818	551	553	555	rBV	416	178	0.02%	0.003%
6	2.880	570	572	575	rVB2	369	214	0.03%	0.003%
7	2.963	595	598	600	rBV2	494	375	0.05%	0.006%
8	2.976	600	602	607	rVB2	757	423	0.06%	0.007%
9	3.118	644	646	649	rVV3	533	372	0.05%	0.006%
10	3.156	656	658	661	rBV3	304	186	0.02%	0.003%
11	3.191	667	669	671	rBV	451	243	0.03%	0.004%
12	3.214	673	676	679	rBV3	449	313	0.04%	0.005%
13	3.291	695	700	702	rBV2	326	298	0.04%	0.005%
14	3.368	721	724	727	rBV	297	214	0.03%	0.003%
15	3.474	753	757	758	rBV3	318	217	0.03%	0.003%
16	3.497	760	764	767	rVV2	399	290	0.04%	0.005%
17	3.523	767	772	775	rVB3	463	414	0.05%	0.007%
18	3.574	786	788	797	rVB4	401	548	0.07%	0.009%
19	3.645	806	810	814	rBV3	636	494	0.06%	0.008%
20	3.677	816	820	824	rVB3	435	398	0.05%	0.006%
21	3.741	837	840	841	rBV	379	217	0.03%	0.003%
22	3.790	844	855	892	rBV2	72822	216286	28.25%	3.442%
23	4.195	979	981	982	rBV	507	285	0.04%	0.005%
24	4.249	983	998	1026	rVV	114342	295372	38.58%	4.701%
25	4.571	1095	1098	1099	rBV2	727	389	0.05%	0.006%
26	4.706	1137	1140	1143	rBV	379	252	0.03%	0.004%
27	4.796	1166	1168	1171	rVB2	561	293	0.04%	0.005%
28	4.822	1171	1176	1182	rBV4	481	494	0.06%	0.008%
29	4.873	1186	1192	1194	rBV3	463	413	0.05%	0.007%
30	4.957	1202	1218	1249	rBV2	288745	765573	100.00%	12.184%
31	5.352	1339	1341	1345	rBV4	439	297	0.04%	0.005%
32	5.384	1349	1351	1354	rVB2	597	296	0.04%	0.005%
33	5.535	1386	1398	1420	rBV	259834	544166	71.08%	8.660%
34	5.831	1477	1490	1508	rBV2	12034	27863	3.64%	0.443%
35	5.989	1525	1539	1559	rBV	169800	358284	46.80%	5.702%
36	6.233	1613	1615	1619	rVB3	432	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032063.D
 Acq On : 13 Sep 2023 09:47
 Operator : SY/MD
 Sample : VV0913MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.291	1630	1633	1638	rVB4	430	367	0.05%	0.006%
38	6.420	1670	1673	1677	rBV2	500	270	0.04%	0.004%
39	6.574	1714	1721	1727	rBV3	536	692	0.09%	0.011%
40	6.680	1750	1754	1759	rVB4	555	606	0.08%	0.010%
41	6.709	1759	1763	1767	rBV3	558	500	0.07%	0.008%
42	6.825	1797	1799	1803	rBV	263	182	0.02%	0.003%
43	6.854	1803	1808	1809	rBV2	255	208	0.03%	0.003%
44	6.915	1817	1827	1849	rBV	93258	178285	23.29%	2.837%
45	7.108	1885	1887	1889	rBV2	324	208	0.03%	0.003%
46	7.246	1918	1930	1962	rBV	330295	600386	78.42%	9.555%
47	7.555	2016	2026	2053	rBV	62949	120070	15.68%	1.911%
48	7.867	2120	2123	2126	rBV3	313	226	0.03%	0.004%
49	7.915	2136	2138	2141	rBV2	453	242	0.03%	0.004%
50	8.027	2163	2173	2213	rBV	187100	379188	49.53%	6.035%
51	8.606	2350	2353	2356	rBV3	344	210	0.03%	0.003%
52	8.690	2377	2379	2388	rVB	720	536	0.07%	0.009%
53	8.725	2388	2390	2392	rBV2	299	196	0.03%	0.003%
54	8.786	2397	2409	2434	rBV	402814	677028	88.43%	10.775%
55	9.085	2496	2502	2515	rBV7	1573	2175	0.28%	0.035%
56	9.265	2550	2558	2561	rBV4	486	488	0.06%	0.008%
57	9.448	2612	2615	2620	rVB3	270	187	0.02%	0.003%
58	9.481	2620	2625	2626	rBV2	1003	738	0.10%	0.012%
59	9.600	2660	2662	2665	rVB3	558	228	0.03%	0.004%
60	9.635	2669	2673	2678	rVV3	382	414	0.05%	0.007%
61	9.776	2713	2717	2718	rBV3	353	221	0.03%	0.004%
62	9.979	2777	2780	2783	rBV3	308	220	0.03%	0.004%
63	10.018	2790	2792	2795	rBV	437	216	0.03%	0.003%
64	10.156	2821	2835	2860	rBV	220062	357196	46.66%	5.685%
65	10.323	2883	2887	2890	rVV3	342	312	0.04%	0.005%
66	10.484	2932	2937	2947	rVB5	1575	2437	0.32%	0.039%
67	10.587	2966	2969	2972	rBV2	482	227	0.03%	0.004%
68	10.651	2985	2989	2992	rBV2	370	263	0.03%	0.004%
69	10.741	3014	3017	3023	rVB2	464	390	0.05%	0.006%
70	10.770	3023	3026	3029	rBV	639	356	0.05%	0.006%
71	10.860	3047	3054	3058	rBV3	1582	1966	0.26%	0.031%
72	10.969	3083	3088	3091	rBV3	380	394	0.05%	0.006%
73	10.995	3092	3096	3101	rVB4	316	329	0.04%	0.005%
74	11.021	3101	3104	3105	rBV2	333	179	0.02%	0.003%
75	11.127	3132	3137	3145	rVB7	2149	2973	0.39%	0.047%
76	11.188	3145	3156	3180	rBV	435514	684783	89.45%	10.898%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032063.D
 Acq On : 13 Sep 2023 09:47
 Operator : SY/MD
 Sample : VV0913MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.387	3214	3218	3221	rBV	254	203	0.03%	0.003%
78	11.410	3222	3225	3231	rVB3	567	508	0.07%	0.008%
79	11.455	3235	3239	3241	rBV	401	277	0.04%	0.004%
80	11.564	3260	3273	3290	rBV	338427	543150	70.95%	8.644%
81	11.763	3331	3335	3336	rBV	281	184	0.02%	0.003%
82	11.873	3367	3369	3372	rVB	386	195	0.03%	0.003%
83	12.034	3414	3419	3420	rBV2	376	313	0.04%	0.005%
84	12.140	3448	3452	3454	rBV2	290	194	0.03%	0.003%
85	12.185	3463	3466	3467	rBV2	487	296	0.04%	0.005%
86	12.239	3481	3483	3487	rBV	333	225	0.03%	0.004%
87	12.593	3587	3593	3601	rVB6	2852	4454	0.58%	0.071%
88	12.632	3601	3605	3610	rBV3	414	394	0.05%	0.006%
89	12.796	3653	3656	3660	rBV3	426	384	0.05%	0.006%
90	12.841	3665	3670	3672	rBV2	664	560	0.07%	0.009%
91	12.882	3680	3683	3686	rBV4	483	383	0.05%	0.006%
92	13.107	3751	3753	3756	rVB2	638	263	0.03%	0.004%
93	13.130	3758	3760	3765	rVB2	424	265	0.03%	0.004%
94	13.204	3777	3783	3794	rVB4	5645	8153	1.06%	0.130%
95	13.445	3849	3858	3875	rBV	26718	44259	5.78%	0.704%
96	13.628	3913	3915	3918	rBV2	355	192	0.03%	0.003%
97	13.689	3926	3934	3948	rVB4	7641	11560	1.51%	0.184%
98	13.767	3955	3958	3961	rBV	475	294	0.04%	0.005%
99	13.821	3972	3975	3977	rBV2	394	199	0.03%	0.003%
100	14.310	4124	4127	4131	rBV4	547	444	0.06%	0.007%




Sum of corrected areas: 6283334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032063.D
Acq On : 13 Sep 2023 09:47
Operator : SY/MD
Sample : VV0913MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

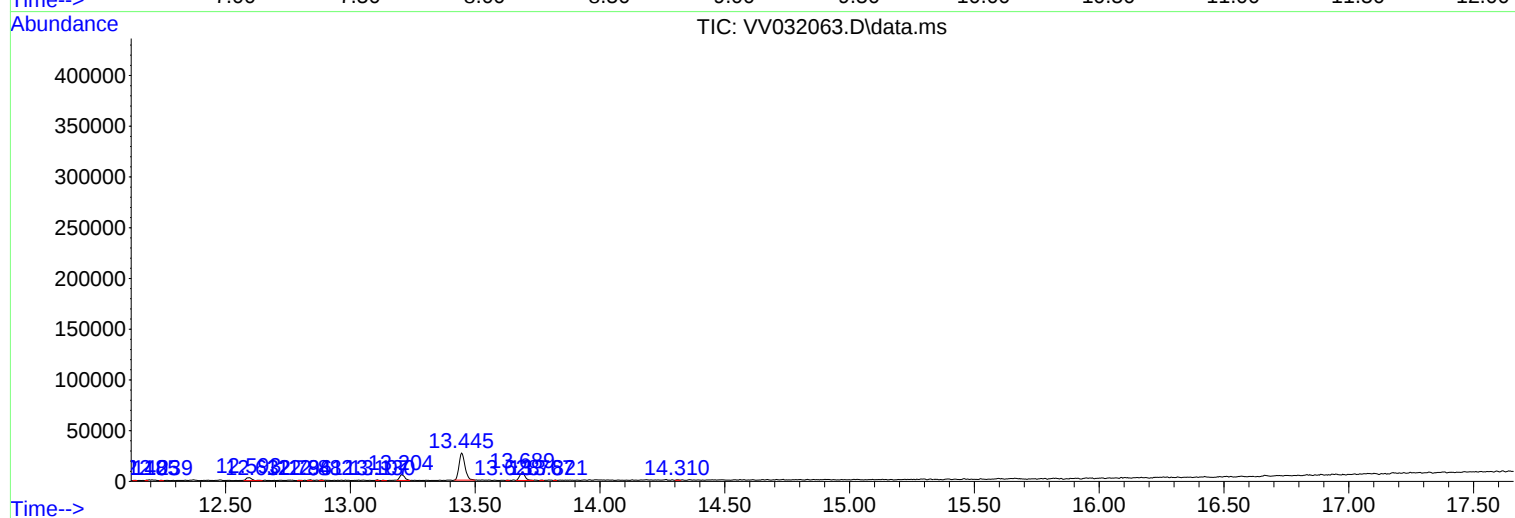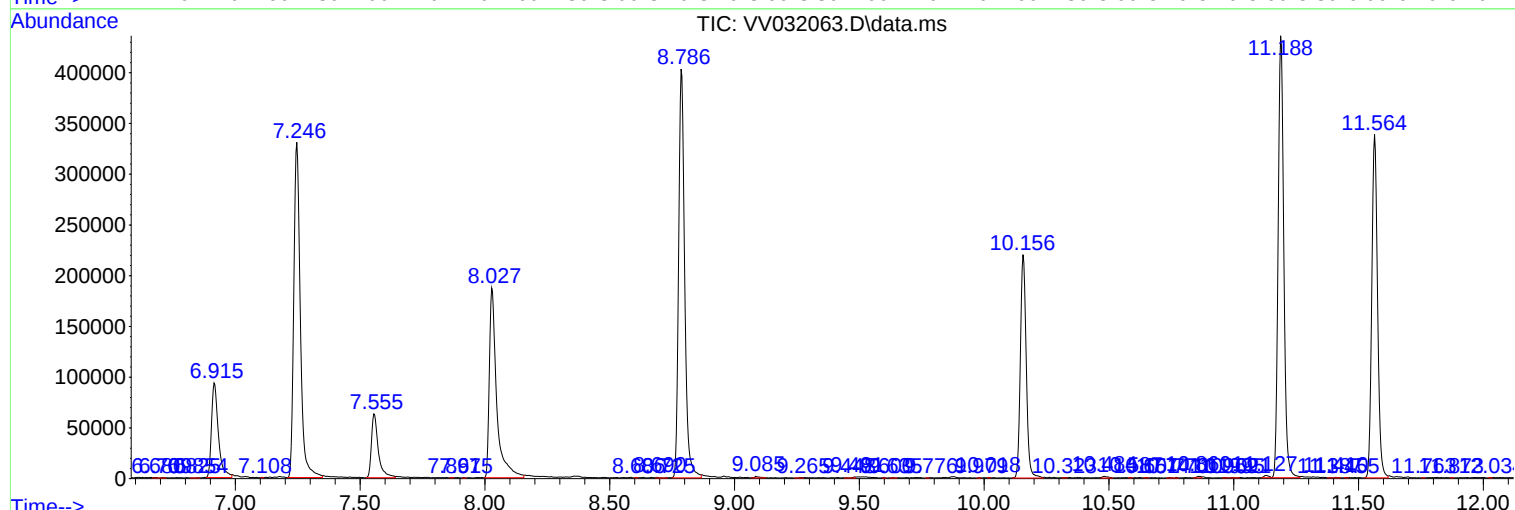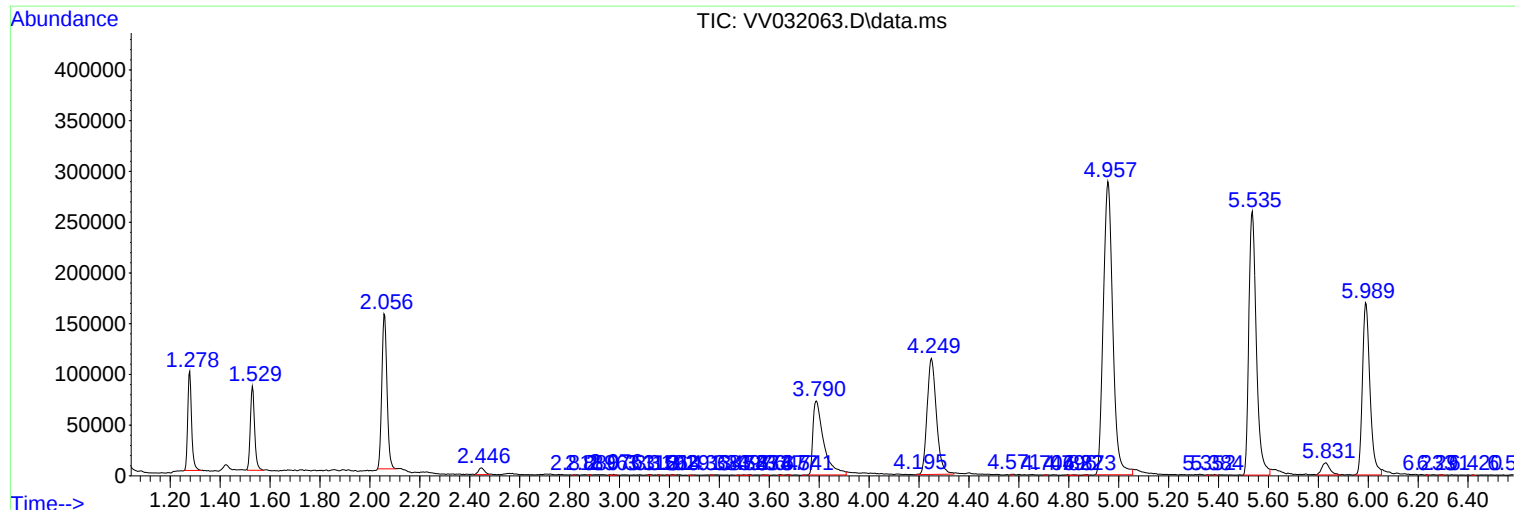

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032063.D
Acq On : 13 Sep 2023 09:47
Operator : SY/MD
Sample : VV0913MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032063.D
Acq On : 13 Sep 2023 09:47
Operator : SY/MD
Sample : VV0913MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc