

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032065.D
 Acq On : 13 Sep 2023 10:32
 Operator : SY/MD
 Sample : 04332-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	92170	98328	13.62%	1.650%
2	1.529	146	152	167	rVB	75200	90879	12.59%	1.525%
3	2.060	308	317	330	rBV	142190	206388	28.59%	3.464%
4	2.632	494	495	497	rBV	588	250	0.03%	0.004%
5	2.764	533	536	537	rBV	340	198	0.03%	0.003%
6	2.854	561	564	566	rBV2	407	307	0.04%	0.005%
7	2.966	595	599	600	rBV3	350	197	0.03%	0.003%
8	3.134	648	651	654	rBV	473	304	0.04%	0.005%
9	3.159	657	659	662	rVB2	630	335	0.05%	0.006%
10	3.175	662	664	666	rBV2	409	220	0.03%	0.004%
11	3.208	670	674	676	rBV2	344	232	0.03%	0.004%
12	3.224	677	679	683	rBV	274	213	0.03%	0.004%
13	3.310	703	706	709	rVV	296	224	0.03%	0.004%
14	3.339	713	715	719	rVB2	345	182	0.03%	0.003%
15	3.481	755	759	762	rVB3	667	467	0.06%	0.008%
16	3.516	765	770	772	rBV2	325	202	0.03%	0.003%
17	3.603	795	797	800	rVV2	426	217	0.03%	0.004%
18	3.725	830	835	837	rBV2	296	268	0.04%	0.004%
19	3.748	840	842	844	rBV	375	195	0.03%	0.003%
20	3.793	845	856	891	rBV2	76804	229128	31.75%	3.846%
21	4.252	984	999	1029	rBV	108852	279513	38.73%	4.691%
22	4.635	1115	1118	1119	rBV2	484	277	0.04%	0.005%
23	4.719	1142	1144	1146	rVB	481	194	0.03%	0.003%
24	4.896	1194	1199	1202	rBV2	454	453	0.06%	0.008%
25	4.960	1202	1219	1242	rBV2	273976	721769	100.00%	12.114%
26	5.317	1327	1330	1332	rBV2	365	188	0.03%	0.003%
27	5.400	1353	1356	1358	rBV	525	375	0.05%	0.006%
28	5.458	1372	1374	1376	rBV2	321	181	0.03%	0.003%
29	5.539	1386	1399	1440	rBV	243380	525310	72.78%	8.817%
30	5.828	1479	1489	1508	rBV2	12504	28196	3.91%	0.473%
31	5.912	1513	1515	1521	rBV5	291	266	0.04%	0.004%
32	5.992	1527	1540	1566	rBV	162050	348670	48.31%	5.852%
33	6.246	1616	1619	1621	rBV	373	231	0.03%	0.004%
34	6.307	1634	1638	1641	rBV3	447	356	0.05%	0.006%
35	6.323	1641	1643	1647	rBV2	360	260	0.04%	0.004%
36	6.458	1682	1685	1687	rVV	510	334	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032065.D
 Acq On : 13 Sep 2023 10:32
 Operator : SY/MD
 Sample : 04332-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.526	1702	1706	1709	rBV2	697	483	0.07%	0.008%
38	6.709	1759	1763	1765	rVB2	373	234	0.03%	0.004%
39	6.738	1768	1772	1774	rBV2	333	255	0.04%	0.004%
40	6.773	1780	1783	1792	rVB3	621	628	0.09%	0.011%
41	6.825	1792	1799	1802	rBV3	403	477	0.07%	0.008%
42	6.918	1816	1828	1854	rBV	88665	172415	23.89%	2.894%
43	7.246	1919	1930	1969	rBV	310715	568228	78.73%	9.537%
44	7.558	2018	2027	2054	rBV	59739	113726	15.76%	1.909%
45	7.793	2097	2100	2102	rBV2	348	219	0.03%	0.004%
46	7.805	2102	2104	2106	rBV	628	317	0.04%	0.005%
47	7.982	2156	2159	2164	rBV4	469	317	0.04%	0.005%
48	8.030	2164	2174	2206	rBV	188060	382458	52.99%	6.419%
49	8.182	2217	2221	2231	rVB	7552	7301	1.01%	0.123%
50	8.339	2267	2270	2272	rBV4	649	491	0.07%	0.008%
51	8.365	2272	2278	2287	rVV4	2613	4504	0.62%	0.076%
52	8.426	2291	2297	2300	rBV5	665	544	0.08%	0.009%
53	8.493	2313	2318	2320	rBV3	651	606	0.08%	0.010%
54	8.564	2336	2340	2343	rBV4	415	459	0.06%	0.008%
55	8.606	2350	2353	2354	rBV2	332	185	0.03%	0.003%
56	8.680	2373	2376	2380	rBV3	308	261	0.04%	0.004%
57	8.789	2399	2410	2441	rBV	384578	643275	89.12%	10.797%
58	9.040	2485	2488	2489	rBV	373	194	0.03%	0.003%
59	9.127	2512	2515	2517	rBV2	342	254	0.04%	0.004%
60	9.191	2534	2535	2539	rVB2	521	303	0.04%	0.005%
61	9.477	2622	2624	2626	rBV2	302	195	0.03%	0.003%
62	9.519	2635	2637	2645	rVB5	607	615	0.09%	0.010%
63	9.564	2648	2651	2653	rBV2	302	208	0.03%	0.003%
64	9.735	2702	2704	2708	rBV	330	174	0.02%	0.003%
65	9.754	2708	2710	2715	rVB2	558	290	0.04%	0.005%
66	9.783	2715	2719	2720	rBV2	443	249	0.03%	0.004%
67	9.870	2744	2746	2748	rBV2	423	173	0.02%	0.003%
68	9.895	2752	2754	2759	rVB3	379	226	0.03%	0.004%
69	9.918	2759	2761	2768	rBV4	383	265	0.04%	0.004%
70	10.037	2796	2798	2801	rVB2	350	175	0.02%	0.003%
71	10.101	2816	2818	2824	rVV2	432	358	0.05%	0.006%
72	10.156	2824	2835	2858	rVV	215630	348976	48.35%	5.857%
73	10.300	2877	2880	2882	rBV	386	225	0.03%	0.004%
74	10.403	2907	2912	2914	rBV	467	380	0.05%	0.006%
75	10.458	2926	2929	2934	rVB2	368	260	0.04%	0.004%
76	10.725	3010	3012	3018	rVB3	383	321	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032065.D
 Acq On : 13 Sep 2023 10:32
 Operator : SY/MD
 Sample : 04332-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.757	3018	3022	3025	rBV2	358	299	0.04%	0.005%
78	10.812	3036	3039	3043	rVB3	456	287	0.04%	0.005%
79	10.860	3050	3054	3055	rBV	401	275	0.04%	0.005%
80	11.088	3122	3125	3127	rBV	278	200	0.03%	0.003%
81	11.188	3145	3156	3176	rBV	406139	643739	89.19%	10.805%
82	11.464	3239	3242	3244	rBV2	321	214	0.03%	0.004%
83	11.564	3260	3273	3297	rBV	328580	517628	71.72%	8.688%
84	11.760	3330	3334	3337	rBV4	437	410	0.06%	0.007%
85	11.857	3360	3364	3367	rBV2	468	398	0.06%	0.007%
86	11.921	3381	3384	3390	rBV2	332	350	0.05%	0.006%
87	11.989	3401	3405	3409	rBV2	338	255	0.04%	0.004%
88	12.014	3409	3413	3416	rBV2	460	371	0.05%	0.006%
89	12.072	3429	3431	3434	rBV2	385	276	0.04%	0.005%
90	12.181	3461	3465	3466	rBV2	312	173	0.02%	0.003%
91	12.297	3499	3501	3505	rBV2	308	188	0.03%	0.003%
92	12.358	3518	3520	3524	rBV2	402	345	0.05%	0.006%
93	12.644	3607	3609	3614	rBV3	400	340	0.05%	0.006%
94	13.281	3805	3807	3812	rBV2	431	285	0.04%	0.005%
95	13.355	3828	3830	3834	rBV	428	226	0.03%	0.004%
96	13.378	3834	3837	3838	rBV2	370	216	0.03%	0.004%
97	13.451	3855	3860	3869	rVB3	2713	3685	0.51%	0.062%
98	14.152	4076	4078	4084	rVB3	719	431	0.06%	0.007%
99	14.365	4142	4144	4145	rBV2	582	262	0.04%	0.004%
100	14.905	4309	4312	4317	rBV4	735	655	0.09%	0.011%




Sum of corrected areas: 5958039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032065.D
Acq On : 13 Sep 2023 10:32
Operator : SY/MD
Sample : 04332-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

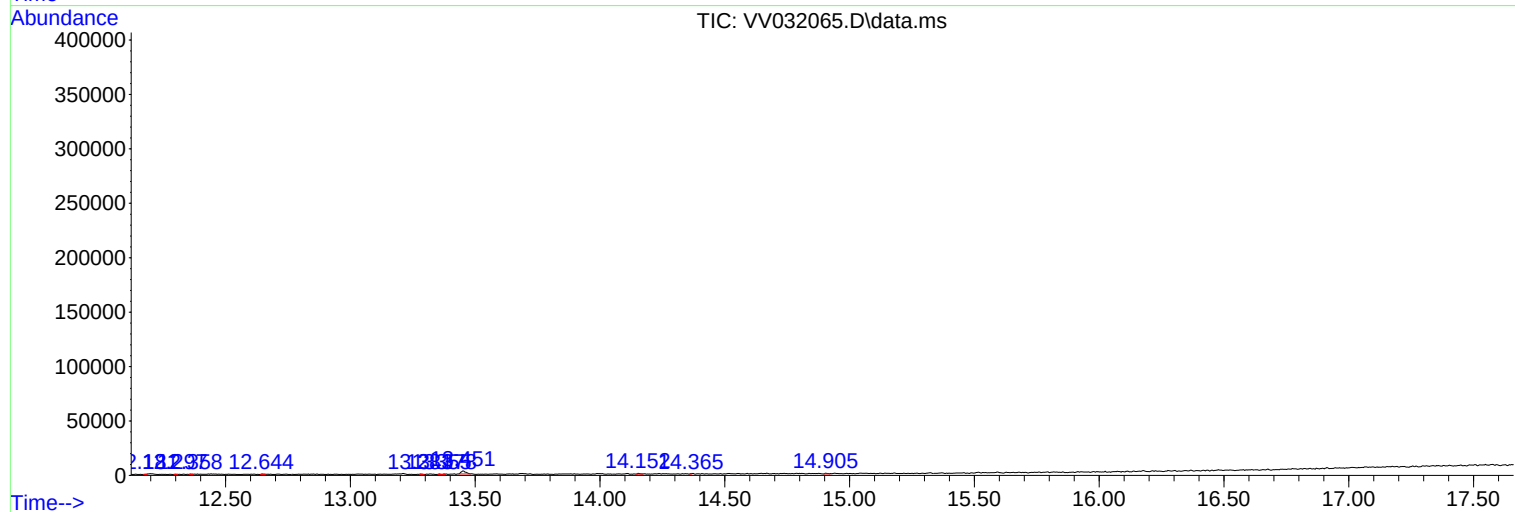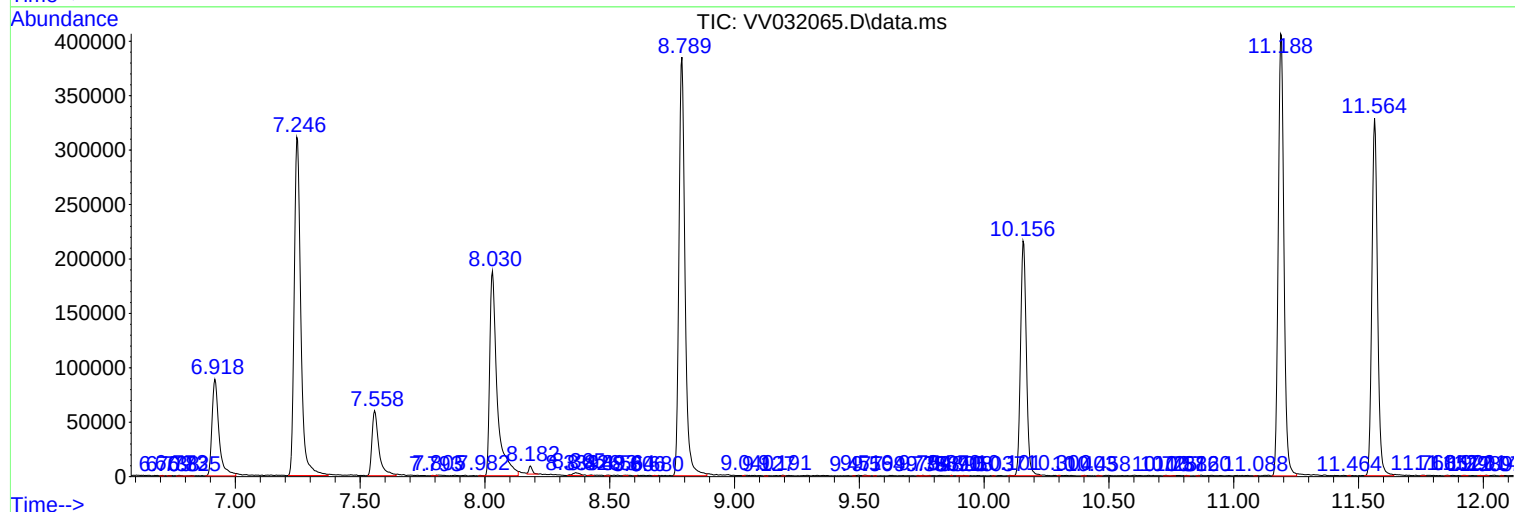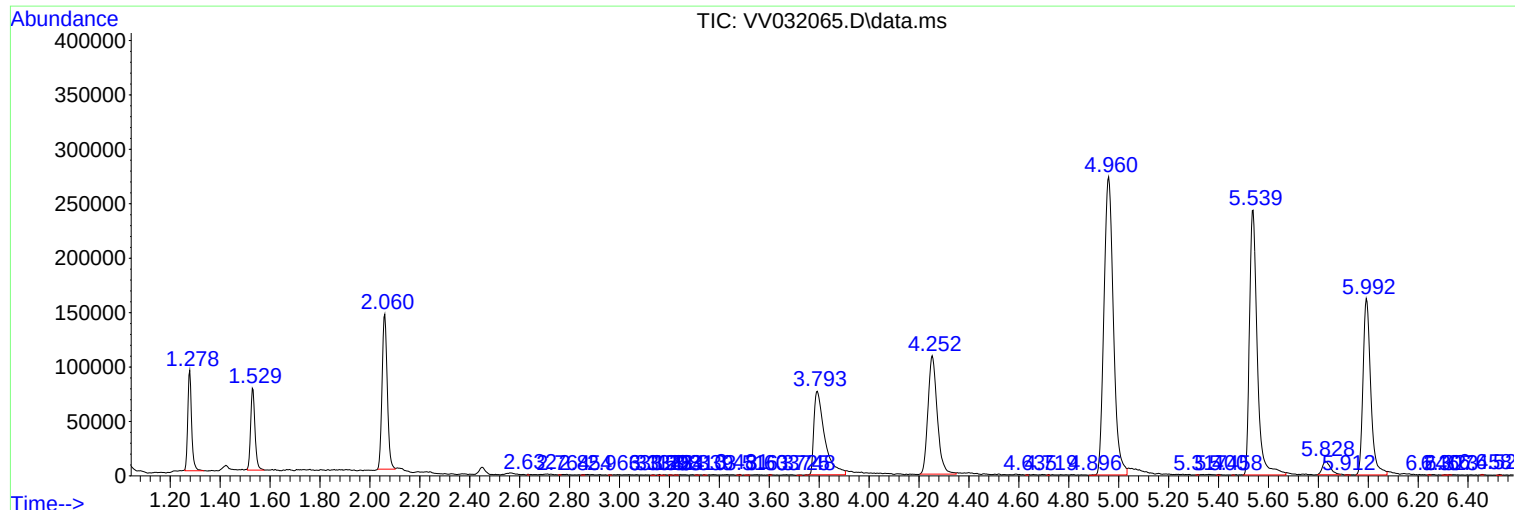

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032065.D
Acq On : 13 Sep 2023 10:32
Operator : SY/MD
Sample : 04332-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032065.D
Acq On : 13 Sep 2023 10:32
Operator : SY/MD
Sample : 04332-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------