

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032066.D
 Acq On : 13 Sep 2023 11:11
 Operator : SY/MD
 Sample : 04332-02ME
 Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

Signal : TIC: VV032066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	50	rBV	5856	5561	0.72%	0.091%
2	1.275	67	73	93	rVB	61585	91954	11.90%	1.497%
3	2.034	300	309	326	rVB	142735	208629	27.00%	3.397%
4	2.551	460	470	487	rVB	17468	35624	4.61%	0.580%
5	2.818	549	553	555	rBV5	507	373	0.05%	0.006%
6	3.098	637	640	642	rVB2	456	250	0.03%	0.004%
7	3.143	652	654	657	rBV4	486	328	0.04%	0.005%
8	3.304	702	704	707	rVB3	371	209	0.03%	0.003%
9	3.333	710	713	717	rBV2	469	411	0.05%	0.007%
10	3.397	730	733	735	rBV2	483	223	0.03%	0.004%
11	3.481	757	759	763	rBV2	537	347	0.04%	0.006%
12	3.510	763	768	769	rBV	226	190	0.02%	0.003%
13	3.587	789	792	797	rVB4	461	281	0.04%	0.005%
14	3.693	821	825	828	rBV	362	360	0.05%	0.006%
15	3.805	850	860	898	rBV	44808	176612	22.85%	2.876%
16	4.246	981	997	1022	rBV2	103017	279477	36.16%	4.551%
17	4.645	1118	1121	1123	rBV2	495	311	0.04%	0.005%
18	4.731	1144	1148	1151	rBV3	523	436	0.06%	0.007%
19	4.799	1166	1169	1172	rVB3	268	171	0.02%	0.003%
20	4.818	1172	1175	1176	rBV	385	224	0.03%	0.004%
21	4.950	1200	1216	1248	rBV2	284730	737318	95.41%	12.006%
22	5.243	1304	1307	1309	rBV2	316	193	0.02%	0.003%
23	5.532	1385	1397	1435	rBV	274944	596414	77.18%	9.711%
24	5.828	1477	1489	1504	rBV3	10888	25689	3.32%	0.418%
25	5.927	1512	1520	1526	rBV8	2262	4346	0.56%	0.071%
26	5.989	1528	1539	1569	rVB	156417	341560	44.20%	5.562%
27	6.272	1624	1627	1635	rBV6	667	755	0.10%	0.012%
28	6.304	1635	1637	1641	rBV2	497	373	0.05%	0.006%
29	6.394	1663	1665	1668	rBV3	396	329	0.04%	0.005%
30	6.464	1684	1687	1690	rBV4	335	202	0.03%	0.003%
31	6.484	1690	1693	1694	rBV3	450	226	0.03%	0.004%
32	6.542	1708	1711	1713	rBV3	287	224	0.03%	0.004%
33	6.580	1718	1723	1724	rBV2	536	337	0.04%	0.005%
34	6.606	1729	1731	1734	rVB3	633	482	0.06%	0.008%
35	6.664	1746	1749	1754	rBV4	512	379	0.05%	0.006%
36	6.776	1782	1784	1787	rVB2	297	169	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091323\
 Data File : VW032066.D
 Acq On : 13 Sep 2023 11:11
 Operator : SY/MD
 Sample : 04332-02ME
 Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.815	1793	1796	1799	rBV2	375	212	0.03%	0.003%
38	6.915	1814	1827	1851	rBV2	86105	178437	23.09%	2.905%
39	7.246	1919	1930	1958	rBV	314725	574940	74.40%	9.362%
40	7.558	2018	2027	2055	rBV	57236	115136	14.90%	1.875%
41	7.828	2108	2111	2114	rBV2	436	386	0.05%	0.006%
42	7.847	2114	2117	2120	rVV2	352	278	0.04%	0.005%
43	7.979	2154	2158	2159	rBV2	465	278	0.04%	0.005%
44	8.043	2167	2178	2213	rBV2	129955	343332	44.43%	5.590%
45	8.448	2301	2304	2306	rBV3	542	327	0.04%	0.005%
46	8.657	2367	2369	2372	rVB2	382	194	0.03%	0.003%
47	8.789	2398	2410	2438	rBV	431071	743906	96.26%	12.113%
48	9.021	2479	2482	2483	rBV	380	206	0.03%	0.003%
49	9.078	2497	2500	2503	rVB2	453	274	0.04%	0.004%
50	9.095	2503	2505	2506	rBV2	388	185	0.02%	0.003%
51	9.114	2509	2511	2515	rVV3	602	367	0.05%	0.006%
52	9.130	2515	2516	2519	rVB	435	171	0.02%	0.003%
53	9.204	2537	2539	2541	rBV3	380	171	0.02%	0.003%
54	9.246	2549	2552	2555	rBV3	456	270	0.03%	0.004%
55	9.329	2576	2578	2582	rVB	433	194	0.03%	0.003%
56	9.352	2582	2585	2587	rBV	367	210	0.03%	0.003%
57	9.390	2592	2597	2599	rBV	474	352	0.05%	0.006%
58	9.451	2613	2616	2618	rBV	294	172	0.02%	0.003%
59	9.480	2623	2625	2626	rBV2	389	193	0.02%	0.003%
60	9.519	2635	2637	2640	rBV	360	197	0.03%	0.003%
61	9.532	2640	2641	2644	rVB2	497	201	0.03%	0.003%
62	9.590	2656	2659	2663	rVB	439	192	0.02%	0.003%
63	9.615	2663	2667	2671	rBV3	403	380	0.05%	0.006%
64	9.741	2703	2706	2708	rBV2	280	188	0.02%	0.003%
65	9.754	2708	2710	2715	rVB3	555	431	0.06%	0.007%
66	9.873	2742	2747	2752	rBV5	667	669	0.09%	0.011%
67	9.927	2759	2764	2766	rBV2	476	383	0.05%	0.006%
68	10.072	2806	2809	2811	rBV	269	165	0.02%	0.003%
69	10.159	2823	2836	2857	rBV	207766	338044	43.74%	5.504%
70	10.461	2928	2930	2934	rBV3	327	204	0.03%	0.003%
71	10.525	2947	2950	2952	rBV2	570	381	0.05%	0.006%
72	10.599	2971	2973	2976	rVB3	506	208	0.03%	0.003%
73	10.898	3060	3066	3069	rBV8	2385	2791	0.36%	0.045%
74	11.104	3128	3130	3134	rBV2	566	560	0.07%	0.009%
75	11.191	3146	3157	3178	rBV	499409	772792	100.00%	12.583%
76	11.348	3204	3206	3209	rBV3	431	220	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032066.D
 Acq On : 13 Sep 2023 11:11
 Operator : SY/MD
 Sample : 04332-02ME
 Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.390	3217	3219	3222	rBV3	390	185	0.02%	0.003%
78	11.439	3232	3234	3238	rVB3	396	200	0.03%	0.003%
79	11.461	3238	3241	3242	rBV2	411	207	0.03%	0.003%
80	11.567	3259	3274	3294	rBV	343791	539978	69.87%	8.792%
81	11.905	3377	3379	3383	rVB2	372	242	0.03%	0.004%
82	11.930	3383	3387	3389	rBV	455	258	0.03%	0.004%
83	11.966	3394	3398	3404	rBV5	505	568	0.07%	0.009%
84	12.101	3438	3440	3446	rVB2	617	439	0.06%	0.007%
85	12.130	3446	3449	3453	rBV	714	518	0.07%	0.008%
86	12.310	3497	3505	3508	rBV3	1284	1583	0.20%	0.026%
87	12.371	3518	3524	3528	rBV6	771	940	0.12%	0.015%
88	12.464	3550	3553	3555	rBV2	409	222	0.03%	0.004%
89	12.474	3555	3556	3560	rVB2	515	206	0.03%	0.003%
90	12.635	3602	3606	3610	rBV2	582	575	0.07%	0.009%
91	12.744	3636	3640	3642	rBV2	622	400	0.05%	0.007%
92	13.040	3727	3732	3735	rBV3	569	456	0.06%	0.007%
93	13.094	3747	3749	3753	rBV2	323	218	0.03%	0.004%
94	13.307	3813	3815	3817	rVB2	403	164	0.02%	0.003%
95	13.323	3817	3820	3822	rBV3	416	321	0.04%	0.005%
96	13.455	3853	3861	3865	rBV6	2314	3161	0.41%	0.051%
97	13.528	3881	3884	3886	rBV2	409	264	0.03%	0.004%
98	13.831	3975	3978	3980	rBV3	493	331	0.04%	0.005%
99	13.946	4012	4014	4018	rVB2	394	176	0.02%	0.003%
100	13.979	4019	4024	4025	rBV2	848	711	0.09%	0.012%




Sum of corrected areas: 6141487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032066.D
Acq On : 13 Sep 2023 11:11
Operator : SY/MD
Sample : 04332-02ME
Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COACOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

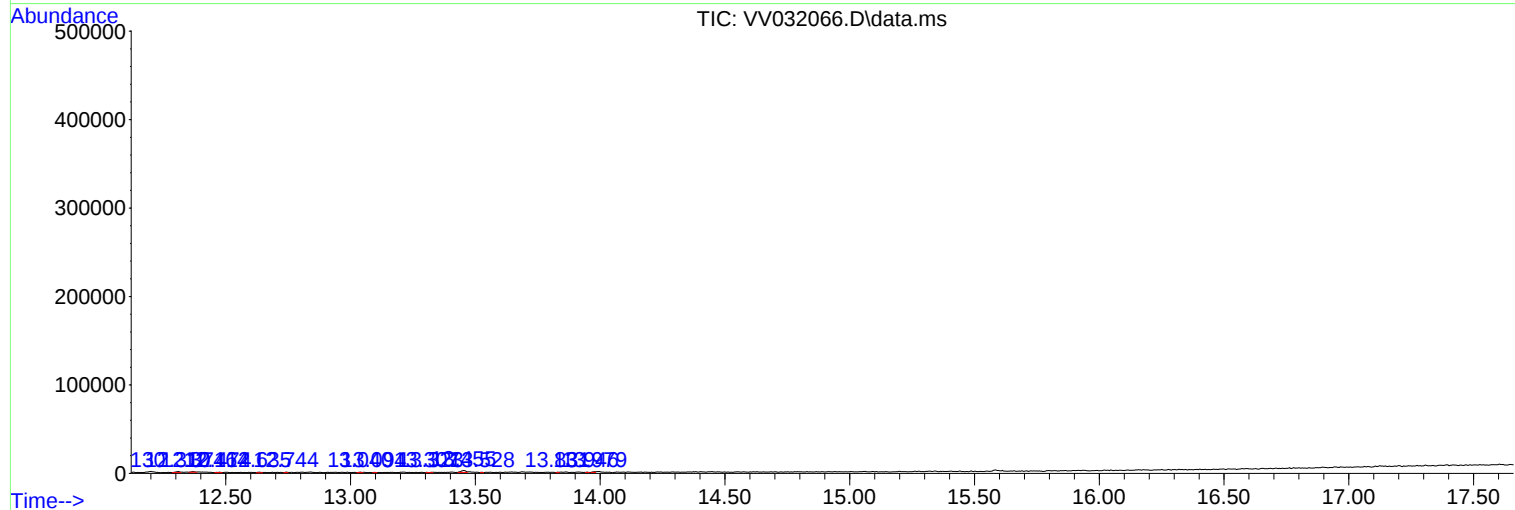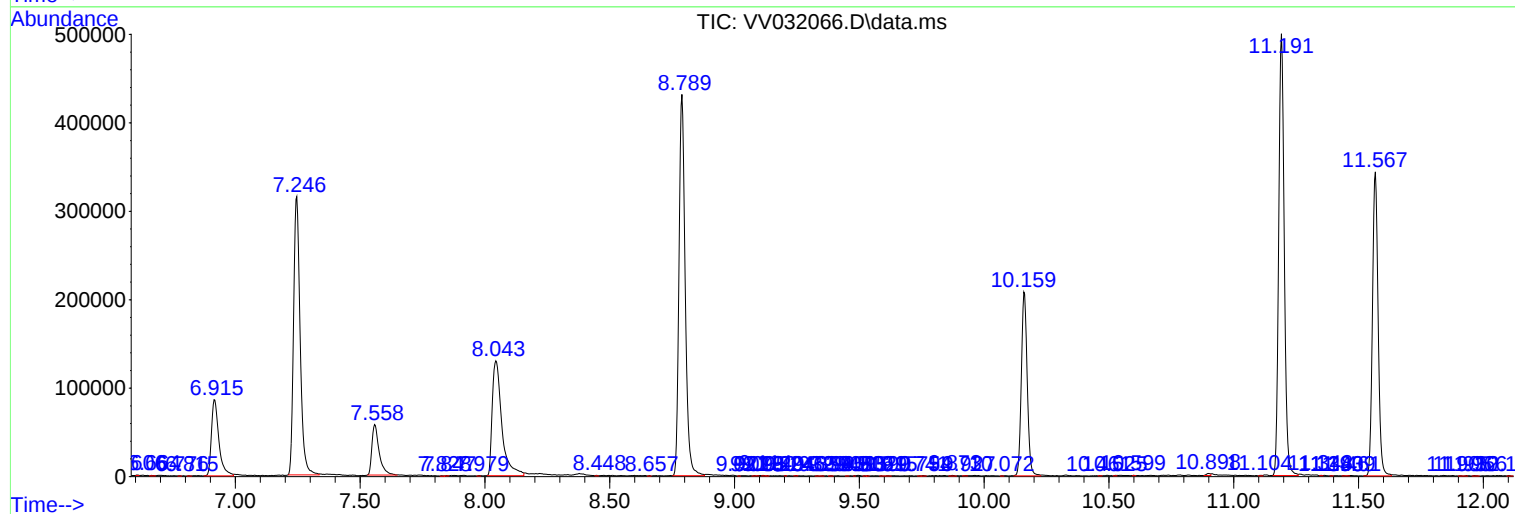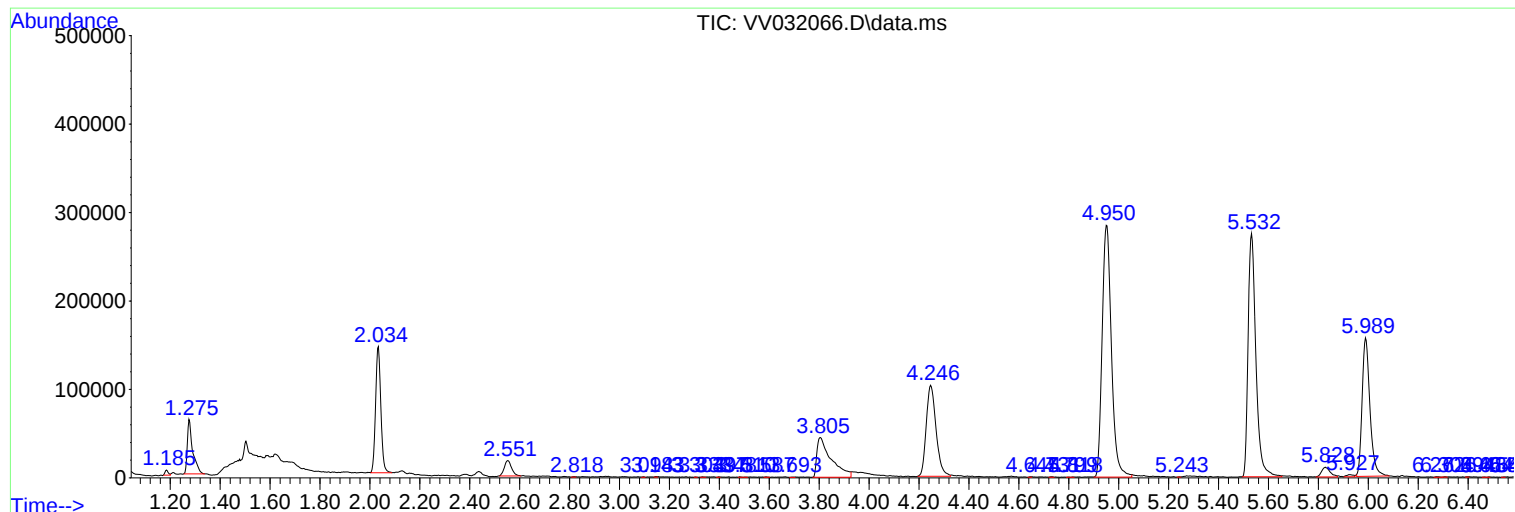

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032066.D
Acq On : 13 Sep 2023 11:11
Operator : SY/MD
Sample : 04332-02ME
Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032066.D
Acq On : 13 Sep 2023 11:11
Operator : SY/MD
Sample : 04332-02ME
Misc : 2.66g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc