

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032069.D
 Acq On : 13 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04332-09ME
 Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	50	rBV	7014	6215	0.78%	0.102%
2	1.275	67	73	95	rVB	59231	92646	11.66%	1.518%
3	2.031	300	308	321	rVB	136993	196433	24.73%	3.218%
4	2.838	556	559	561	rBV2	509	353	0.04%	0.006%
5	3.015	611	614	617	rBV3	703	464	0.06%	0.008%
6	3.056	623	627	629	rBV2	381	340	0.04%	0.006%
7	3.105	638	642	646	rBV3	429	448	0.06%	0.007%
8	3.269	689	693	694	rBV2	368	269	0.03%	0.004%
9	3.314	703	707	710	rVB4	394	346	0.04%	0.006%
10	3.433	741	744	746	rBV2	458	273	0.03%	0.004%
11	3.481	754	759	760	rBV3	266	204	0.03%	0.003%
12	3.497	762	764	768	rVV2	386	204	0.03%	0.003%
13	3.529	771	774	776	rVB2	455	289	0.04%	0.005%
14	3.542	776	778	780	rBV	292	176	0.02%	0.003%
15	3.597	790	795	797	rBV3	351	274	0.03%	0.004%
16	3.680	817	821	823	rBV3	451	287	0.04%	0.005%
17	3.738	837	839	841	rBV2	366	187	0.02%	0.003%
18	3.777	848	851	852	rBV2	395	181	0.02%	0.003%
19	3.809	852	861	895	rBV	45481	167843	21.13%	2.750%
20	4.249	984	998	1027	rVB	101689	273085	34.37%	4.474%
21	4.481	1068	1070	1073	rVB3	680	310	0.04%	0.005%
22	4.497	1073	1075	1077	rBV3	704	388	0.05%	0.006%
23	4.542	1087	1089	1091	rBV2	388	206	0.03%	0.003%
24	4.597	1102	1106	1112	rBV5	608	565	0.07%	0.009%
25	4.790	1163	1166	1168	rBV2	443	235	0.03%	0.004%
26	4.854	1183	1186	1189	rBV2	851	494	0.06%	0.008%
27	4.953	1201	1217	1248	rBV2	281558	722599	90.96%	11.840%
28	5.288	1310	1321	1325	rBV5	1290	2682	0.34%	0.044%
29	5.388	1350	1352	1354	rBV2	394	224	0.03%	0.004%
30	5.426	1361	1364	1372	rVB4	643	579	0.07%	0.009%
31	5.474	1376	1379	1381	rBV	276	180	0.02%	0.003%
32	5.535	1384	1398	1428	rBV	280134	613550	77.23%	10.053%
33	5.831	1479	1490	1510	rVB5	10036	25747	3.24%	0.422%
34	5.992	1529	1540	1568	rVB	155171	335290	42.20%	5.494%
35	6.297	1633	1635	1637	rBV2	511	281	0.04%	0.005%
36	6.310	1637	1639	1643	rVB3	419	269	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032069.D
 Acq On : 13 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04332-09ME
 Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.371	1652	1658	1661	rBV3	419	428	0.05%	0.007%
38	6.388	1661	1663	1666	rBV2	678	418	0.05%	0.007%
39	6.429	1672	1676	1677	rBV3	591	325	0.04%	0.005%
40	6.458	1684	1685	1689	rVB2	439	194	0.02%	0.003%
41	6.490	1689	1695	1698	rBV2	588	501	0.06%	0.008%
42	6.545	1708	1712	1714	rBV	457	372	0.05%	0.006%
43	6.587	1721	1725	1727	rBV3	420	359	0.05%	0.006%
44	6.831	1798	1801	1802	rBV2	385	192	0.02%	0.003%
45	6.918	1817	1828	1856	rBV	85337	176276	22.19%	2.888%
46	7.246	1918	1930	1956	rBV	307767	565103	71.13%	9.259%
47	7.561	2018	2028	2047	rBV	56864	115130	14.49%	1.886%
48	7.973	2152	2156	2160	rVB3	417	421	0.05%	0.007%
49	7.995	2160	2163	2166	rBV2	426	341	0.04%	0.006%
50	8.043	2168	2178	2210	rBV	134427	349918	44.05%	5.733%
51	8.545	2333	2334	2338	rBV2	291	198	0.02%	0.003%
52	8.677	2371	2375	2376	rBV2	309	187	0.02%	0.003%
53	8.789	2398	2410	2433	rBV	447988	766974	96.54%	12.567%
54	9.085	2497	2502	2504	rBV2	447	316	0.04%	0.005%
55	9.140	2516	2519	2521	rBV2	425	210	0.03%	0.003%
56	9.153	2521	2523	2527	rBV2	375	284	0.04%	0.005%
57	9.233	2546	2548	2551	rBV2	431	240	0.03%	0.004%
58	9.323	2572	2576	2580	rBV4	478	424	0.05%	0.007%
59	9.346	2580	2583	2586	rBV2	365	224	0.03%	0.004%
60	9.461	2615	2619	2626	rVB4	513	531	0.07%	0.009%
61	9.497	2626	2630	2631	rBV2	524	320	0.04%	0.005%
62	9.567	2649	2652	2654	rVB3	611	376	0.05%	0.006%
63	9.645	2673	2676	2678	rBV2	396	251	0.03%	0.004%
64	9.702	2692	2694	2701	rVB3	268	235	0.03%	0.004%
65	9.738	2701	2705	2710	rBV4	731	870	0.11%	0.014%
66	9.828	2729	2733	2735	rBV2	269	221	0.03%	0.004%
67	9.870	2742	2746	2747	rBV	548	322	0.04%	0.005%
68	9.931	2762	2765	2767	rBV3	511	239	0.03%	0.004%
69	9.956	2771	2773	2777	rVV2	304	183	0.02%	0.003%
70	10.011	2786	2790	2794	rBV4	580	516	0.06%	0.008%
71	10.114	2818	2822	2824	rBV3	419	329	0.04%	0.005%
72	10.162	2824	2837	2858	rBV	206825	342626	43.13%	5.614%
73	10.413	2911	2915	2917	rBV2	244	193	0.02%	0.003%
74	10.436	2920	2922	2927	rVB3	297	237	0.03%	0.004%
75	10.465	2929	2931	2934	rBV2	319	237	0.03%	0.004%
76	10.519	2945	2948	2949	rBV	579	302	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032069.D
 Acq On : 13 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04332-09ME
 Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.600	2970	2973	2975	rBV4	737	386	0.05%	0.006%
78	10.648	2986	2988	2991	rBV2	594	334	0.04%	0.005%
79	10.847	3048	3050	3052	rBV2	459	219	0.03%	0.004%
80	11.111	3130	3132	3135	rBV3	561	402	0.05%	0.007%
81	11.191	3145	3157	3178	rBV	510378	794438	100.00%	13.017%
82	11.500	3249	3253	3255	rBV3	508	381	0.05%	0.006%
83	11.567	3262	3274	3295	rBV	337197	530843	66.82%	8.698%
84	11.915	3380	3382	3385	rBV	436	279	0.04%	0.005%
85	12.104	3439	3441	3446	rVB2	553	377	0.05%	0.006%
86	12.127	3446	3448	3451	rBV	447	228	0.03%	0.004%
87	12.149	3451	3455	3458	rBV3	302	256	0.03%	0.004%
88	12.310	3501	3505	3507	rBV2	334	239	0.03%	0.004%
89	12.349	3511	3517	3521	rBV3	581	642	0.08%	0.011%
90	12.554	3579	3581	3583	rBV2	347	178	0.02%	0.003%
91	12.625	3601	3603	3606	rVB2	482	219	0.03%	0.004%
92	12.680	3617	3620	3623	rBV2	379	231	0.03%	0.004%
93	12.699	3623	3626	3628	rBV2	408	295	0.04%	0.005%
94	13.181	3773	3776	3780	rVB3	447	282	0.04%	0.005%
95	13.201	3780	3782	3783	rBV	498	186	0.02%	0.003%
96	13.243	3792	3795	3797	rBV2	426	335	0.04%	0.005%
97	13.313	3814	3817	3820	rBV3	574	410	0.05%	0.007%
98	13.358	3828	3831	3834	rBV2	610	382	0.05%	0.006%
99	13.400	3841	3844	3847	rBV2	603	373	0.05%	0.006%
100	13.680	3930	3931	3932	rBV	564	202	0.03%	0.003%




Sum of corrected areas: 6103256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032069.D
Acq On : 13 Sep 2023 12:21
Operator : SY/MD
Sample : 04332-09ME
Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

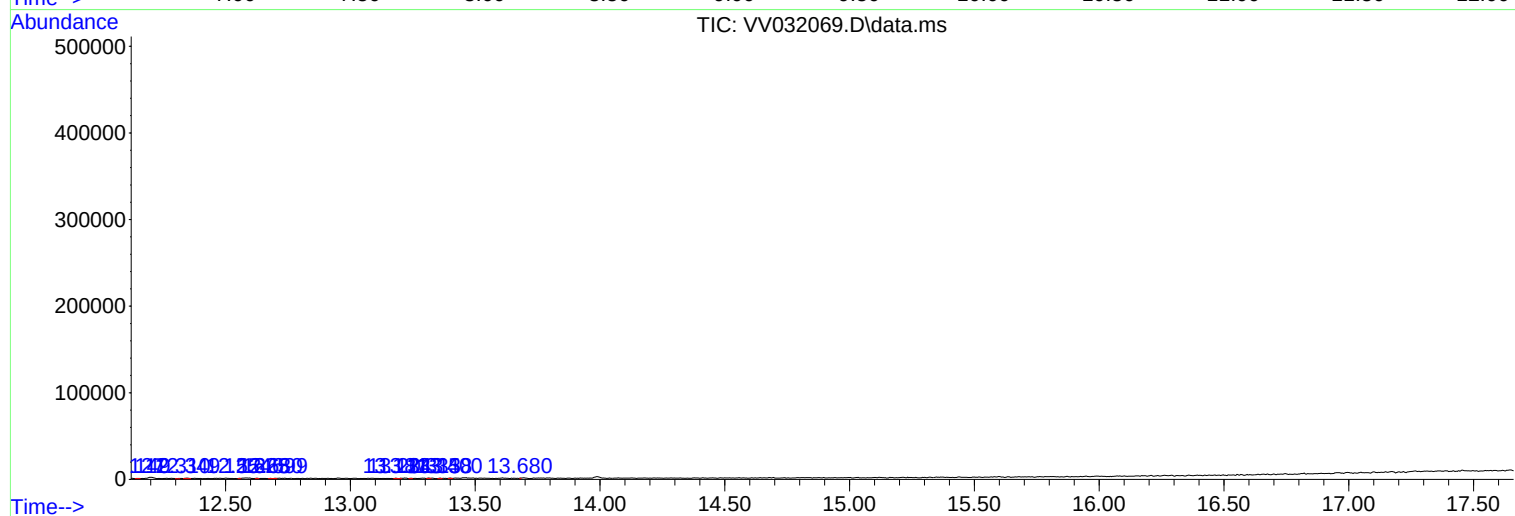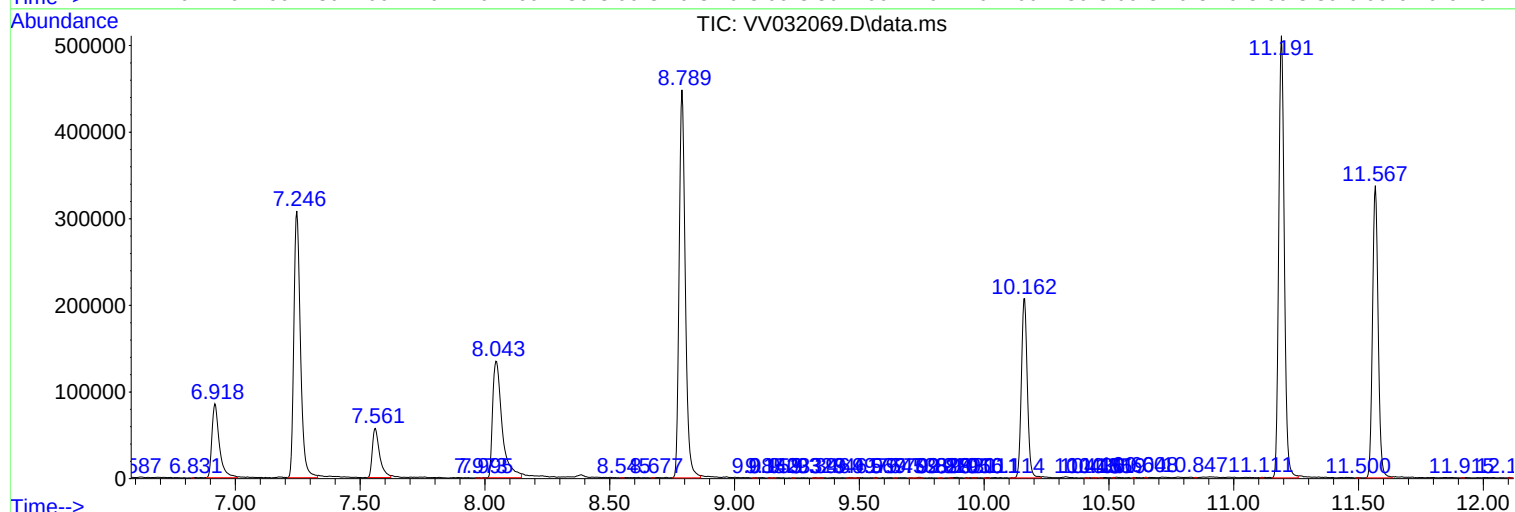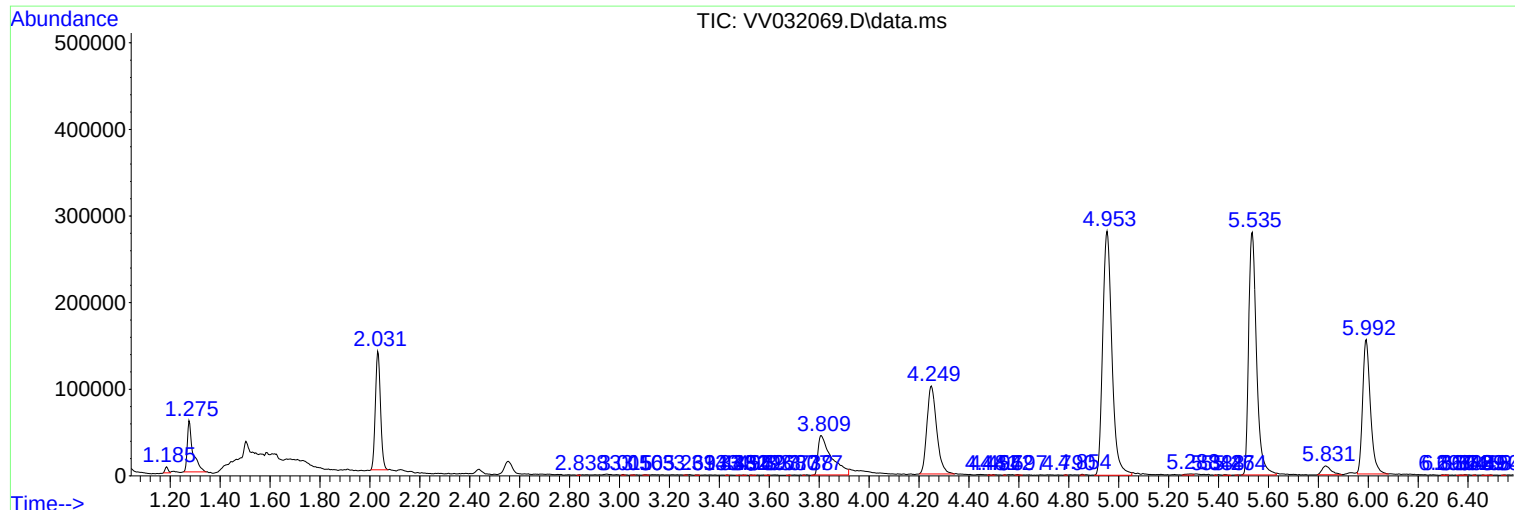

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032069.D
Acq On : 13 Sep 2023 12:21
Operator : SY/MD
Sample : 04332-09ME
Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032069.D
Acq On : 13 Sep 2023 12:21
Operator : SY/MD
Sample : 04332-09ME
Misc : 0.46g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc