

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032070.D
 Acq On : 13 Sep 2023 12:44
 Operator : SY/MD
 Sample : 04332-15ME
 Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	50	rBV	5995	5511	0.69%	0.091%
2	1.275	67	73	91	rBV	59182	88270	11.06%	1.453%
3	2.034	301	309	324	rVB	134779	196375	24.61%	3.232%
4	2.847	559	562	568	rBV3	687	561	0.07%	0.009%
5	2.876	568	571	573	rBV3	525	283	0.04%	0.005%
6	2.989	603	606	609	rVB3	666	459	0.06%	0.008%
7	3.372	723	725	729	rVV4	447	239	0.03%	0.004%
8	3.394	729	732	734	rVB3	436	262	0.03%	0.004%
9	3.462	751	753	756	rBV2	343	250	0.03%	0.004%
10	3.500	761	765	768	rBV4	506	436	0.05%	0.007%
11	3.536	773	776	778	rBV2	233	128	0.02%	0.002%
12	3.577	785	789	790	rBV2	532	339	0.04%	0.006%
13	3.725	833	835	836	rBV2	339	140	0.02%	0.002%
14	3.741	837	840	843	rVV3	387	281	0.04%	0.005%
15	3.809	852	861	899	rBV	45280	174153	21.82%	2.866%
16	4.249	983	998	1024	rBV	101178	270941	33.95%	4.459%
17	4.478	1067	1069	1072	rBV4	432	227	0.03%	0.004%
18	4.677	1129	1131	1134	rBV2	204	118	0.01%	0.002%
19	4.761	1156	1157	1159	rVV	428	181	0.02%	0.003%
20	4.786	1162	1165	1169	rVB3	455	322	0.04%	0.005%
21	4.815	1169	1174	1176	rBV2	513	376	0.05%	0.006%
22	4.880	1190	1194	1196	rBV2	471	324	0.04%	0.005%
23	4.953	1202	1217	1258	rBV2	280776	714825	89.56%	11.763%
24	5.214	1296	1298	1301	rBV2	455	258	0.03%	0.004%
25	5.275	1309	1317	1319	rBV7	1667	2127	0.27%	0.035%
26	5.429	1364	1365	1367	rBV2	397	130	0.02%	0.002%
27	5.535	1385	1398	1430	rBV	281987	613183	76.83%	10.091%
28	5.728	1456	1458	1461	rVB3	626	256	0.03%	0.004%
29	5.828	1478	1489	1510	rBV3	11179	27856	3.49%	0.458%
30	5.992	1529	1540	1569	rVB	151094	329461	41.28%	5.422%
31	6.243	1615	1618	1620	rVB2	507	222	0.03%	0.004%
32	6.288	1629	1632	1633	rBV	239	141	0.02%	0.002%
33	6.320	1638	1642	1646	rBV3	433	422	0.05%	0.007%
34	6.400	1664	1667	1669	rBV2	439	256	0.03%	0.004%
35	6.416	1669	1672	1673	rBV2	326	199	0.02%	0.003%
36	6.458	1681	1685	1687	rBV3	894	669	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032070.D
 Acq On : 13 Sep 2023 12:44
 Operator : SY/MD
 Sample : 04332-15ME
 Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.529	1704	1707	1708	rBV	278	172	0.02%	0.003%
38	6.822	1796	1798	1799	rBV	327	122	0.02%	0.002%
39	6.847	1804	1806	1807	rBV2	385	168	0.02%	0.003%
40	6.918	1818	1828	1863	rBV2	82443	172352	21.60%	2.836%
41	7.085	1878	1880	1884	rBV3	528	323	0.04%	0.005%
42	7.246	1918	1930	1957	rBV	308334	560226	70.19%	9.219%
43	7.561	2018	2028	2057	rBV	55455	113999	14.28%	1.876%
44	7.738	2078	2083	2087	rBV5	943	1169	0.15%	0.019%
45	7.802	2101	2103	2106	rBV2	449	270	0.03%	0.004%
46	7.870	2123	2124	2126	rBV	436	171	0.02%	0.003%
47	7.963	2150	2153	2155	rBV2	384	249	0.03%	0.004%
48	8.047	2168	2179	2222	rBV	129709	350266	43.89%	5.764%
49	8.564	2338	2340	2343	rBV2	498	232	0.03%	0.004%
50	8.657	2365	2369	2370	rBV	510	330	0.04%	0.005%
51	8.686	2376	2378	2380	rVB2	432	168	0.02%	0.003%
52	8.703	2380	2383	2387	rBV2	550	328	0.04%	0.005%
53	8.789	2399	2410	2438	rBV	439837	770335	96.52%	12.677%
54	9.011	2477	2479	2486	rVB4	680	664	0.08%	0.011%
55	9.066	2493	2496	2497	rBV2	555	273	0.03%	0.004%
56	9.156	2519	2524	2526	rBV2	523	452	0.06%	0.007%
57	9.233	2542	2548	2552	rBV3	569	552	0.07%	0.009%
58	9.252	2552	2554	2556	rVV2	267	119	0.01%	0.002%
59	9.297	2565	2568	2570	rBV	243	151	0.02%	0.002%
60	9.313	2570	2573	2576	rVB	319	187	0.02%	0.003%
61	9.339	2576	2581	2584	rBV4	474	436	0.05%	0.007%
62	9.403	2600	2601	2605	rBV	216	138	0.02%	0.002%
63	9.484	2623	2626	2629	rBV2	633	424	0.05%	0.007%
64	9.596	2655	2661	2663	rBV3	471	488	0.06%	0.008%
65	9.609	2663	2665	2668	rVB3	535	235	0.03%	0.004%
66	9.651	2676	2678	2681	rBV2	498	343	0.04%	0.006%
67	9.719	2695	2699	2701	rBV3	396	357	0.04%	0.006%
68	9.754	2708	2710	2712	rBV	251	123	0.02%	0.002%
69	9.854	2738	2741	2745	rVB2	574	341	0.04%	0.006%
70	9.873	2745	2747	2750	rBV3	516	302	0.04%	0.005%
71	9.953	2770	2772	2774	rBV3	318	130	0.02%	0.002%
72	9.973	2774	2778	2781	rVB3	531	489	0.06%	0.008%
73	10.162	2826	2837	2854	rBV	199630	329536	41.29%	5.423%
74	10.317	2883	2885	2887	rBV2	325	185	0.02%	0.003%
75	10.333	2887	2890	2897	rVB7	1296	1691	0.21%	0.028%
76	10.362	2897	2899	2903	rBV	350	299	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032070.D
 Acq On : 13 Sep 2023 12:44
 Operator : SY/MD
 Sample : 04332-15ME
 Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.384	2904	2906	2909	rVB2	358	158	0.02%	0.003%
78	10.407	2911	2913	2916	rVB3	439	238	0.03%	0.004%
79	10.474	2930	2934	2936	rBV2	617	519	0.07%	0.009%
80	10.600	2970	2973	2974	rBV	330	167	0.02%	0.003%
81	10.664	2991	2993	2995	rBV3	695	327	0.04%	0.005%
82	10.722	3004	3011	3018	rVB6	1146	1584	0.20%	0.026%
83	10.776	3023	3028	3031	rBV3	1095	1079	0.14%	0.018%
84	10.905	3060	3068	3079	rBV8	2629	5917	0.74%	0.097%
85	11.124	3131	3136	3138	rBV3	683	584	0.07%	0.010%
86	11.191	3146	3157	3178	rBV	510272	798109	100.00%	13.134%
87	11.442	3233	3235	3236	rBV	324	142	0.02%	0.002%
88	11.493	3249	3251	3253	rVB	432	151	0.02%	0.002%
89	11.567	3262	3274	3298	rBV	326922	524029	65.66%	8.624%
90	11.837	3355	3358	3359	rBV2	350	166	0.02%	0.003%
91	11.979	3398	3402	3405	rBV3	585	440	0.06%	0.007%
92	12.571	3581	3586	3592	rBV5	724	884	0.11%	0.015%
93	12.953	3701	3705	3709	rBV3	571	596	0.07%	0.010%
94	12.995	3714	3718	3723	rBV5	517	602	0.08%	0.010%
95	13.124	3754	3758	3762	rBV3	589	485	0.06%	0.008%
96	13.210	3783	3785	3786	rBV2	435	229	0.03%	0.004%
97	13.387	3836	3840	3841	rBV	366	263	0.03%	0.004%
98	13.419	3848	3850	3854	rVB4	540	326	0.04%	0.005%
99	13.673	3925	3929	3931	rBV2	551	426	0.05%	0.007%
100	14.316	4127	4129	4132	rBV	492	331	0.04%	0.005%




Sum of corrected areas: 6076728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032070.D
Acq On : 13 Sep 2023 12:44
Operator : SY/MD
Sample : 04332-15ME
Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

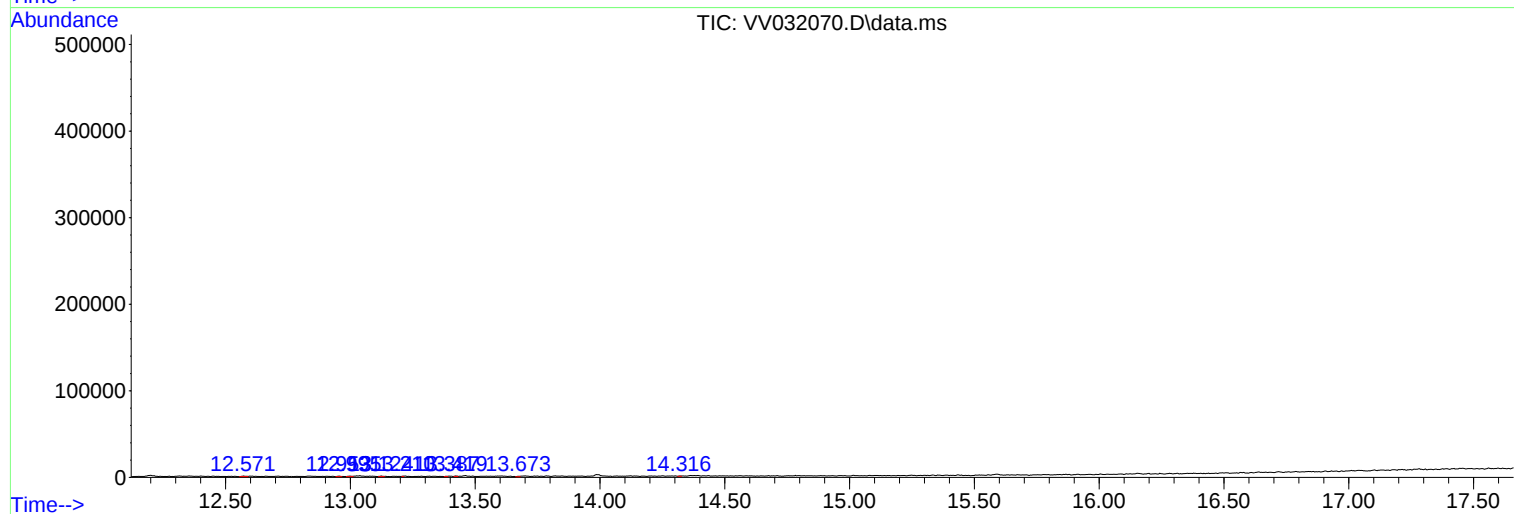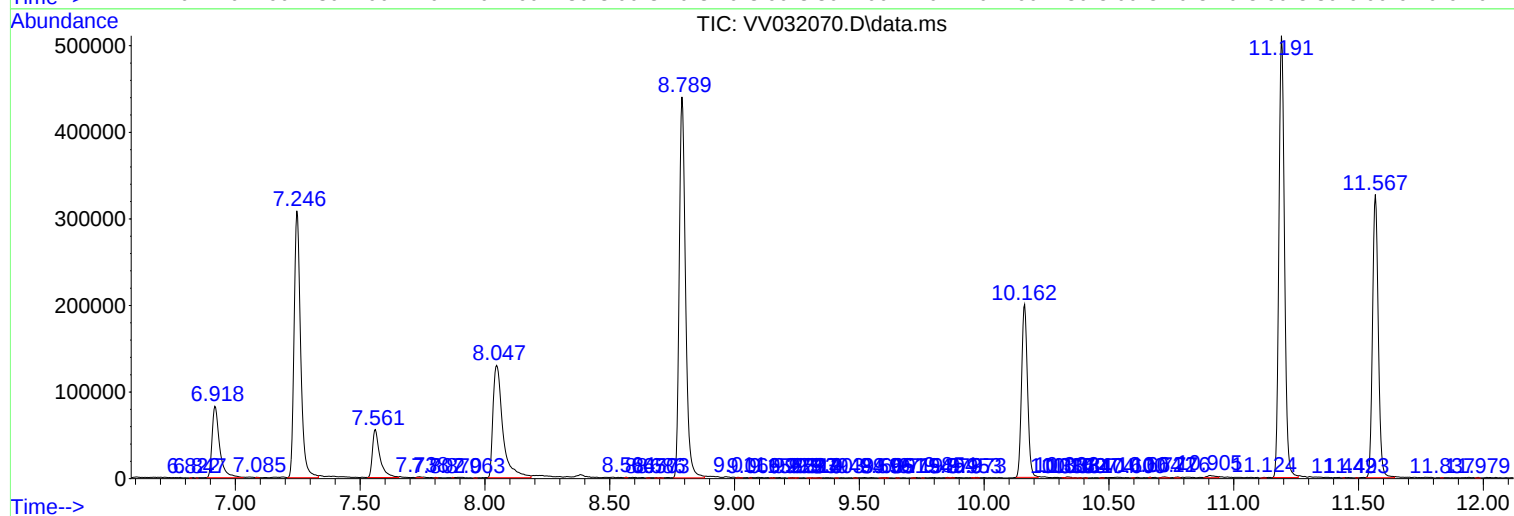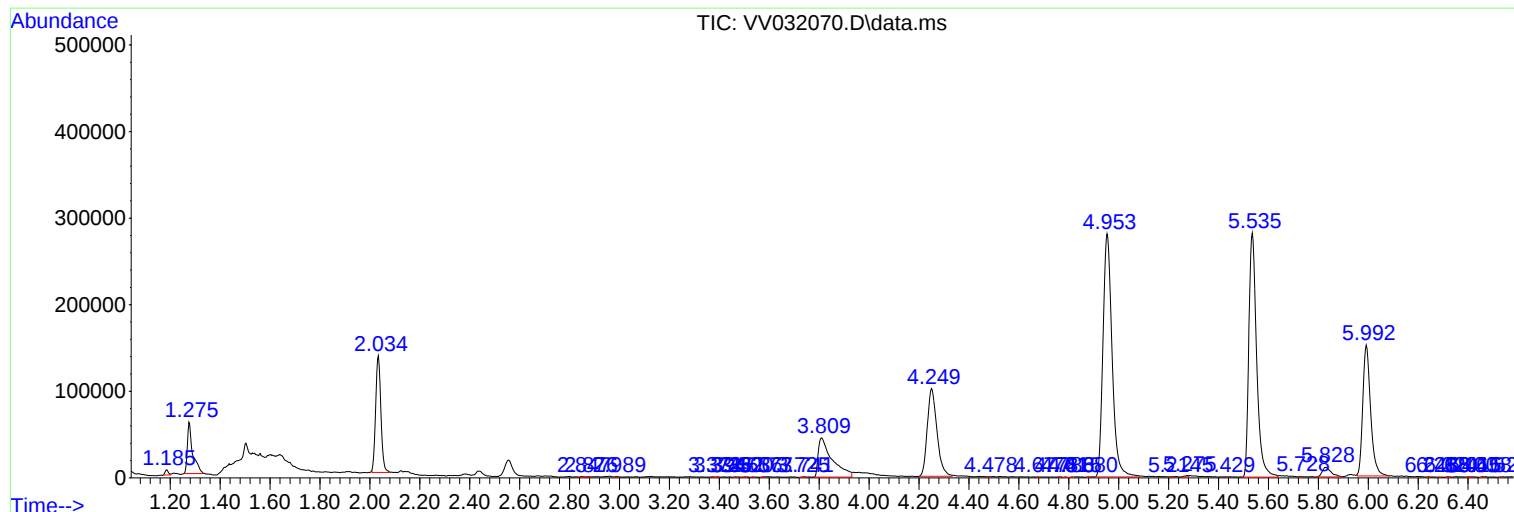

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032070.D
Acq On : 13 Sep 2023 12:44
Operator : SY/MD
Sample : 04332-15ME
Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032070.D
Acq On : 13 Sep 2023 12:44
Operator : SY/MD
Sample : 04332-15ME
Misc : 2.42g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc