

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032071.D
 Acq On : 13 Sep 2023 13:08
 Operator : SY/MD
 Sample : 04332-22ME
 Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	50	rBV	9106	8109	1.05%	0.133%
2	1.275	67	73	94	rVB	58619	91610	11.87%	1.502%
3	2.031	300	308	326	rVB	137201	200320	25.96%	3.285%
4	2.793	543	545	547	rBV	470	271	0.04%	0.004%
5	2.854	562	564	566	rBV	776	409	0.05%	0.007%
6	3.153	653	657	660	rBV3	709	625	0.08%	0.010%
7	3.268	690	693	696	rVV3	465	280	0.04%	0.005%
8	3.371	722	725	728	rBV2	528	331	0.04%	0.005%
9	3.535	774	776	783	rVB4	541	499	0.06%	0.008%
10	3.567	783	786	790	rBV2	487	369	0.05%	0.006%
11	3.584	790	791	794	rBV	306	147	0.02%	0.002%
12	3.670	811	818	822	rBV4	505	634	0.08%	0.010%
13	3.776	848	851	852	rBV	355	186	0.02%	0.003%
14	3.809	852	861	901	rBV2	46844	182219	23.61%	2.988%
15	4.249	984	998	1026	rBV	101642	271935	35.24%	4.459%
16	4.500	1072	1076	1077	rBV2	409	272	0.04%	0.004%
17	4.622	1112	1114	1116	rBV	343	185	0.02%	0.003%
18	4.744	1148	1152	1154	rBV	726	409	0.05%	0.007%
19	4.764	1154	1158	1161	rVB2	614	448	0.06%	0.007%
20	4.783	1161	1164	1169	rBV	733	516	0.07%	0.008%
21	4.863	1187	1189	1194	rVB2	548	384	0.05%	0.006%
22	4.889	1194	1197	1200	rBV3	325	170	0.02%	0.003%
23	4.953	1200	1217	1246	rBV2	282437	730702	94.68%	11.981%
24	5.188	1287	1290	1293	rBV2	526	370	0.05%	0.006%
25	5.220	1297	1300	1302	rBV	319	189	0.02%	0.003%
26	5.230	1302	1303	1304	rBV	383	142	0.02%	0.002%
27	5.394	1352	1354	1357	rVB4	678	349	0.05%	0.006%
28	5.410	1357	1359	1362	rBV2	378	257	0.03%	0.004%
29	5.426	1362	1364	1368	rVB3	498	311	0.04%	0.005%
30	5.535	1386	1398	1431	rBV	276317	596014	77.23%	9.773%
31	5.828	1478	1489	1510	rBV4	11621	28042	3.63%	0.460%
32	5.992	1528	1540	1570	rVB	154727	341990	44.32%	5.608%
33	6.281	1627	1630	1632	rBV2	506	404	0.05%	0.007%
34	6.291	1632	1633	1638	rVV3	769	490	0.06%	0.008%
35	6.362	1653	1655	1657	rVB	380	150	0.02%	0.002%
36	6.391	1659	1664	1668	rBV5	747	903	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091323\
 Data File : VW032071.D
 Acq On : 13 Sep 2023 13:08
 Operator : SY/MD
 Sample : 04332-22ME
 Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.538	1708	1710	1713	rBV	417	237	0.03%	0.004%
38	6.583	1721	1724	1725	rBV2	455	284	0.04%	0.005%
39	6.918	1816	1828	1849	rBV2	86688	175676	22.76%	2.881%
40	7.117	1888	1890	1892	rBV2	407	248	0.03%	0.004%
41	7.178	1904	1909	1915	rVB6	801	1056	0.14%	0.017%
42	7.246	1918	1930	1958	rBV	313548	574090	74.39%	9.413%
43	7.522	2014	2016	2018	rBV2	500	280	0.04%	0.005%
44	7.561	2018	2028	2054	rVV	57544	118518	15.36%	1.943%
45	7.799	2101	2102	2107	rVB2	375	236	0.03%	0.004%
46	7.821	2107	2109	2112	rVB2	414	248	0.03%	0.004%
47	7.972	2153	2156	2157	rBV2	342	185	0.02%	0.003%
48	7.989	2157	2161	2163	rBV4	500	469	0.06%	0.008%
49	8.046	2168	2179	2213	rBV2	139446	360044	46.65%	5.904%
50	8.561	2337	2339	2341	rBV2	421	232	0.03%	0.004%
51	8.686	2375	2378	2382	rVB2	658	433	0.06%	0.007%
52	8.738	2389	2394	2396	rBV2	410	401	0.05%	0.007%
53	8.789	2399	2410	2432	rBV	430006	742430	96.20%	12.174%
54	9.079	2498	2500	2503	rBV2	504	274	0.04%	0.004%
55	9.098	2503	2506	2508	rBV2	510	286	0.04%	0.005%
56	9.133	2515	2517	2520	rBV3	377	178	0.02%	0.003%
57	9.204	2537	2539	2542	rVB2	540	277	0.04%	0.005%
58	9.226	2542	2546	2549	rBV3	518	342	0.04%	0.006%
59	9.255	2552	2555	2558	rBV2	508	328	0.04%	0.005%
60	9.307	2568	2571	2572	rBV2	434	194	0.03%	0.003%
61	9.313	2572	2573	2577	rVB2	830	366	0.05%	0.006%
62	9.361	2584	2588	2591	rVB2	368	218	0.03%	0.004%
63	9.378	2591	2593	2596	rBV	334	220	0.03%	0.004%
64	9.500	2627	2631	2633	rBV	545	415	0.05%	0.007%
65	9.513	2633	2635	2641	rVB2	544	436	0.06%	0.007%
66	9.580	2653	2656	2659	rBV3	547	331	0.04%	0.005%
67	9.622	2664	2669	2671	rBV2	355	283	0.04%	0.005%
68	9.693	2686	2691	2693	rBV4	577	443	0.06%	0.007%
69	9.741	2703	2706	2709	rBV2	568	439	0.06%	0.007%
70	10.008	2782	2789	2793	rVB4	599	734	0.10%	0.012%
71	10.033	2793	2797	2799	rBV2	563	379	0.05%	0.006%
72	10.162	2825	2837	2857	rBV	206265	342625	44.40%	5.618%
73	10.287	2874	2876	2880	rBV4	305	223	0.03%	0.004%
74	10.332	2886	2890	2897	rVV4	944	1240	0.16%	0.020%
75	10.368	2899	2901	2905	rVB	351	151	0.02%	0.002%
76	10.416	2913	2916	2918	rBV3	424	289	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032071.D
 Acq On : 13 Sep 2023 13:08
 Operator : SY/MD
 Sample : 04332-22ME
 Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.487	2934	2938	2940	rBV2	595	477	0.06%	0.008%
78	10.525	2945	2950	2952	rBV4	558	551	0.07%	0.009%
79	10.709	3003	3007	3010	rBV3	789	648	0.08%	0.011%
80	11.004	3098	3099	3101	rBV	318	152	0.02%	0.002%
81	11.049	3110	3113	3116	rBV2	522	443	0.06%	0.007%
82	11.191	3146	3157	3176	rBV	498871	771725	100.00%	12.654%
83	11.567	3260	3274	3292	rBV	333896	533301	69.11%	8.745%
84	11.885	3370	3373	3376	rBV3	423	262	0.03%	0.004%
85	11.914	3380	3382	3389	rVB4	442	344	0.04%	0.006%
86	11.972	3394	3400	3403	rBV4	481	520	0.07%	0.009%
87	12.049	3421	3424	3426	rBV3	456	279	0.04%	0.005%
88	12.175	3461	3463	3465	rBV2	572	321	0.04%	0.005%
89	12.262	3488	3490	3493	rBV3	507	253	0.03%	0.004%
90	12.297	3497	3501	3502	rBV2	497	274	0.04%	0.004%
91	12.307	3502	3504	3505	rBV2	554	202	0.03%	0.003%
92	12.577	3586	3588	3591	rBV	385	239	0.03%	0.004%
93	12.647	3608	3610	3614	rVB2	634	350	0.05%	0.006%
94	12.937	3696	3700	3701	rBV	411	262	0.03%	0.004%
95	13.014	3722	3724	3725	rBV	726	329	0.04%	0.005%
96	13.162	3768	3770	3771	rBV	495	195	0.03%	0.003%
97	13.188	3777	3778	3782	rBV3	376	240	0.03%	0.004%
98	13.252	3795	3798	3803	rVB3	468	367	0.05%	0.006%
99	13.307	3813	3815	3818	rBV2	431	270	0.03%	0.004%
100	14.229	4099	4102	4104	rBV3	521	301	0.04%	0.005%

Sum of corrected areas: 6098684




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032071.D
Acq On : 13 Sep 2023 13:08
Operator : SY/MD
Sample : 04332-22ME
Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

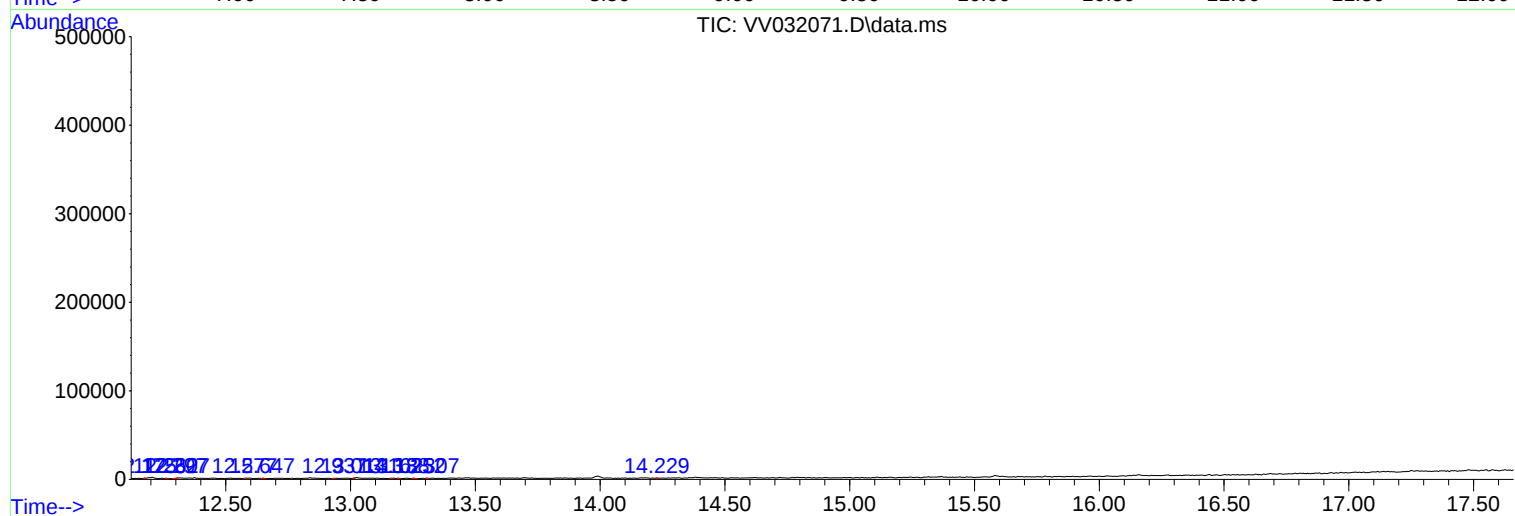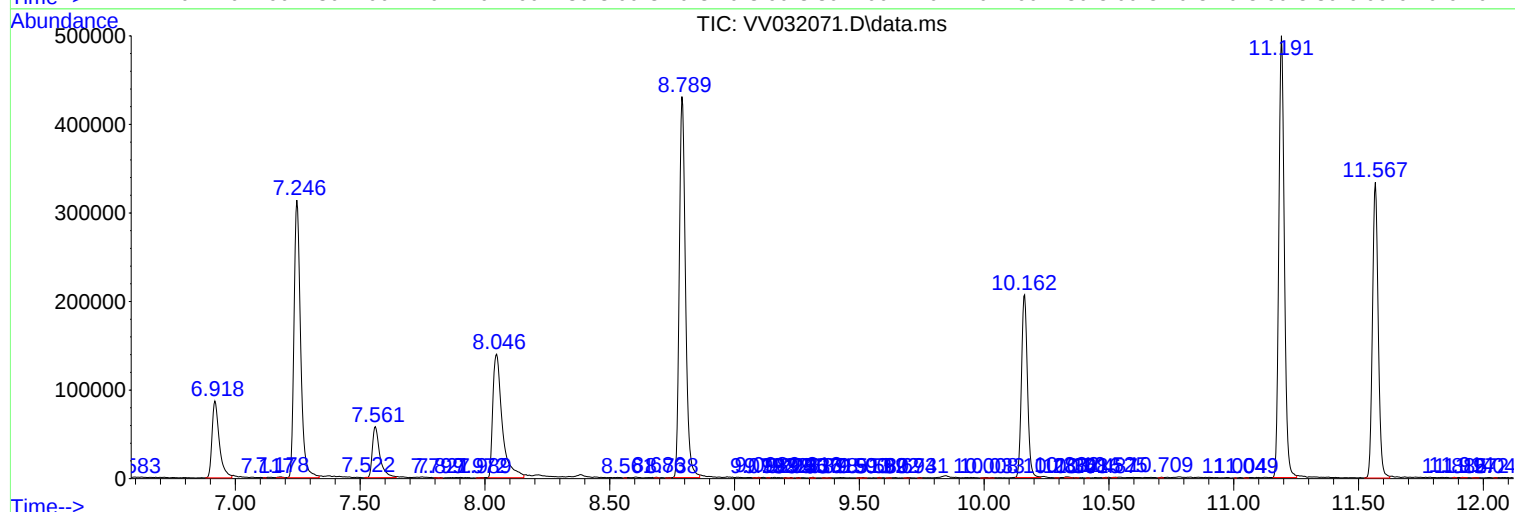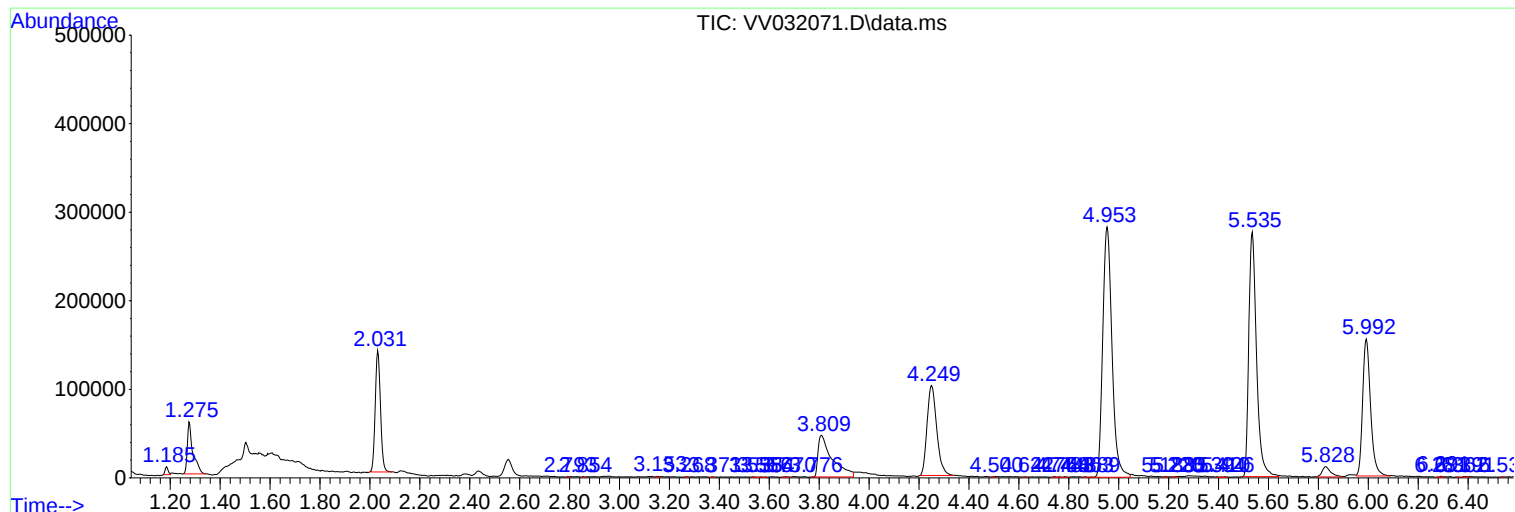

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032071.D
Acq On : 13 Sep 2023 13:08
Operator : SY/MD
Sample : 04332-22ME
Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032071.D
Acq On : 13 Sep 2023 13:08
Operator : SY/MD
Sample : 04332-22ME
Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------