

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032075.D
 Acq On : 13 Sep 2023 14:42
 Operator : SY/MD
 Sample : 04387-08ME
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	49	rBV	6343	5322	0.60%	0.074%
2	1.275	67	73	102	rVB	75370	118471	13.37%	1.656%
3	2.034	301	309	326	rVB	166022	243377	27.47%	3.403%
4	2.381	409	417	427	rBV	20690	35590	4.02%	0.498%
5	2.555	461	471	491	rVB	20642	44259	4.99%	0.619%
6	2.822	552	554	558	rBV2	272	177	0.02%	0.002%
7	2.863	565	567	570	rVB	519	275	0.03%	0.004%
8	3.008	610	612	617	rVB3	571	311	0.04%	0.004%
9	3.050	621	625	627	rVB3	533	278	0.03%	0.004%
10	3.076	627	633	636	rBV5	498	455	0.05%	0.006%
11	3.223	677	679	681	rBV3	437	181	0.02%	0.003%
12	3.330	709	712	714	rBV3	347	194	0.02%	0.003%
13	3.346	714	717	720	rBV3	364	245	0.03%	0.003%
14	3.416	738	739	741	rBV	251	104	0.01%	0.001%
15	3.449	747	749	751	rBV2	323	133	0.02%	0.002%
16	3.500	760	765	767	rBV2	493	459	0.05%	0.006%
17	3.580	787	790	794	rBV3	494	363	0.04%	0.005%
18	3.609	797	799	804	rVB	328	270	0.03%	0.004%
19	3.638	804	808	810	rBV3	456	431	0.05%	0.006%
20	3.670	814	818	819	rVV3	440	338	0.04%	0.005%
21	3.690	822	824	826	rBV2	501	196	0.02%	0.003%
22	3.725	832	835	836	rBV	415	225	0.03%	0.003%
23	3.805	851	860	902	rBV	61193	228412	25.78%	3.194%
24	4.249	984	998	1028	rVB	125052	333667	37.65%	4.665%
25	4.477	1067	1069	1070	rBV	648	248	0.03%	0.003%
26	4.686	1130	1134	1140	rBV5	480	546	0.06%	0.008%
27	4.735	1146	1149	1152	rBV4	583	469	0.05%	0.007%
28	4.821	1172	1176	1179	rBV3	481	385	0.04%	0.005%
29	4.876	1191	1193	1196	rVB2	369	172	0.02%	0.002%
30	4.892	1196	1198	1200	rBV	310	135	0.02%	0.002%
31	4.953	1201	1217	1243	rBV2	349062	886130	100.00%	12.390%
32	5.194	1291	1292	1294	rBV2	400	136	0.02%	0.002%
33	5.387	1350	1352	1354	rBV	434	222	0.03%	0.003%
34	5.452	1370	1372	1374	rBV	255	114	0.01%	0.002%
35	5.535	1384	1398	1430	rBV	274943	592964	66.92%	8.291%
36	5.828	1478	1489	1508	rBV3	13238	31471	3.55%	0.440%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091323\
 Data File : VW032075.D
 Acq On : 13 Sep 2023 14:42
 Operator : SY/MD
 Sample : 04387-08ME
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	5.992	1528	1540	1571	rVB	190081	414468	46.77%	5.795%
38	6.394	1664	1665	1667	rBV	309	108	0.01%	0.002%
39	6.442	1678	1680	1681	rBV	342	177	0.02%	0.002%
40	6.526	1704	1706	1709	rBV2	270	228	0.03%	0.003%
41	6.555	1714	1715	1717	rVB2	586	192	0.02%	0.003%
42	6.571	1717	1720	1721	rBV2	346	213	0.02%	0.003%
43	6.590	1721	1726	1727	rBV2	658	525	0.06%	0.007%
44	6.760	1777	1779	1781	rBV2	317	156	0.02%	0.002%
45	6.918	1818	1828	1853	rBV	105329	214199	24.17%	2.995%
46	7.140	1894	1897	1899	rBV2	713	520	0.06%	0.007%
47	7.246	1918	1930	1964	rBV	381737	701773	79.20%	9.812%
48	7.558	2018	2027	2054	rBV	70817	142914	16.13%	1.998%
49	8.046	2168	2179	2223	rBV	164074	461454	52.08%	6.452%
50	8.468	2308	2310	2311	rBV	381	127	0.01%	0.002%
51	8.477	2311	2313	2316	rVV3	438	266	0.03%	0.004%
52	8.628	2358	2360	2364	rBV2	474	255	0.03%	0.004%
53	8.683	2373	2377	2381	rVB3	357	322	0.04%	0.005%
54	8.706	2381	2384	2386	rBV	422	369	0.04%	0.005%
55	8.789	2399	2410	2439	rBV	421034	749800	84.62%	10.484%
56	9.034	2481	2486	2489	rBV5	781	794	0.09%	0.011%
57	9.210	2538	2541	2547	rVB3	472	396	0.04%	0.006%
58	9.297	2566	2568	2570	rVB	231	110	0.01%	0.002%
59	9.310	2570	2572	2576	rBV	250	168	0.02%	0.002%
60	9.333	2576	2579	2580	rBV	301	151	0.02%	0.002%
61	9.400	2598	2600	2605	rBV2	532	418	0.05%	0.006%
62	9.490	2624	2628	2631	rBV4	607	586	0.07%	0.008%
63	9.571	2651	2653	2656	rBV2	488	305	0.03%	0.004%
64	9.590	2657	2659	2662	rVV3	254	170	0.02%	0.002%
65	9.644	2672	2676	2678	rBV4	504	334	0.04%	0.005%
66	9.699	2688	2693	2697	rBV4	645	708	0.08%	0.010%
67	9.886	2747	2751	2755	rVV3	551	519	0.06%	0.007%
68	9.934	2763	2766	2768	rBV2	252	163	0.02%	0.002%
69	10.040	2797	2799	2800	rBV	364	156	0.02%	0.002%
70	10.075	2808	2810	2813	rBV2	405	255	0.03%	0.004%
71	10.088	2813	2814	2817	rVB2	524	183	0.02%	0.003%
72	10.162	2824	2837	2860	rBV	261633	438300	49.46%	6.128%
73	10.384	2903	2906	2909	rBV	406	335	0.04%	0.005%
74	10.435	2919	2922	2924	rBV3	317	222	0.03%	0.003%
75	10.484	2933	2937	2939	rBV2	642	487	0.05%	0.007%
76	10.522	2947	2949	2950	rBV2	661	353	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032075.D
 Acq On : 13 Sep 2023 14:42
 Operator : SY/MD
 Sample : 04387-08ME
 Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.577	2962	2966	2968	rBV3	410	248	0.03%	0.003%
78	10.696	3000	3003	3007	rBV3	694	486	0.05%	0.007%
79	10.725	3007	3012	3017	rVV3	871	886	0.10%	0.012%
80	10.779	3022	3029	3032	rBV4	991	1210	0.14%	0.017%
81	10.853	3050	3052	3053	rBV4	281	95	0.01%	0.001%
82	10.966	3083	3087	3090	rBV4	420	315	0.04%	0.004%
83	11.037	3102	3109	3114	rBV2	760	820	0.09%	0.011%
84	11.062	3114	3117	3120	rVV4	710	488	0.06%	0.007%
85	11.078	3120	3122	3125	rVB2	637	282	0.03%	0.004%
86	11.095	3125	3127	3130	rBV	510	393	0.04%	0.005%
87	11.120	3133	3135	3138	rBV4	398	234	0.03%	0.003%
88	11.194	3146	3158	3176	rBV	509674	800888	90.38%	11.198%
89	11.567	3262	3274	3296	rBV	429270	683056	77.08%	9.551%
90	12.017	3412	3414	3417	rBV	298	196	0.02%	0.003%
91	12.178	3461	3464	3465	rBV2	495	322	0.04%	0.005%
92	12.242	3481	3484	3490	rBV3	297	285	0.03%	0.004%
93	12.268	3490	3492	3494	rBV2	257	100	0.01%	0.001%
94	12.487	3557	3560	3562	rBV2	456	336	0.04%	0.005%
95	12.728	3634	3635	3639	rBV3	427	216	0.02%	0.003%
96	12.908	3689	3691	3694	rBV2	331	205	0.02%	0.003%
97	13.175	3772	3774	3775	rBV	396	191	0.02%	0.003%
98	13.207	3782	3784	3787	rBV3	467	187	0.02%	0.003%
99	13.503	3874	3876	3878	rBV	554	297	0.03%	0.004%
100	13.641	3916	3919	3921	rBV3	563	385	0.04%	0.005%




Sum of corrected areas: 7152025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032075.D
Acq On : 13 Sep 2023 14:42
Operator : SY/MD
Sample : 04387-08ME
Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

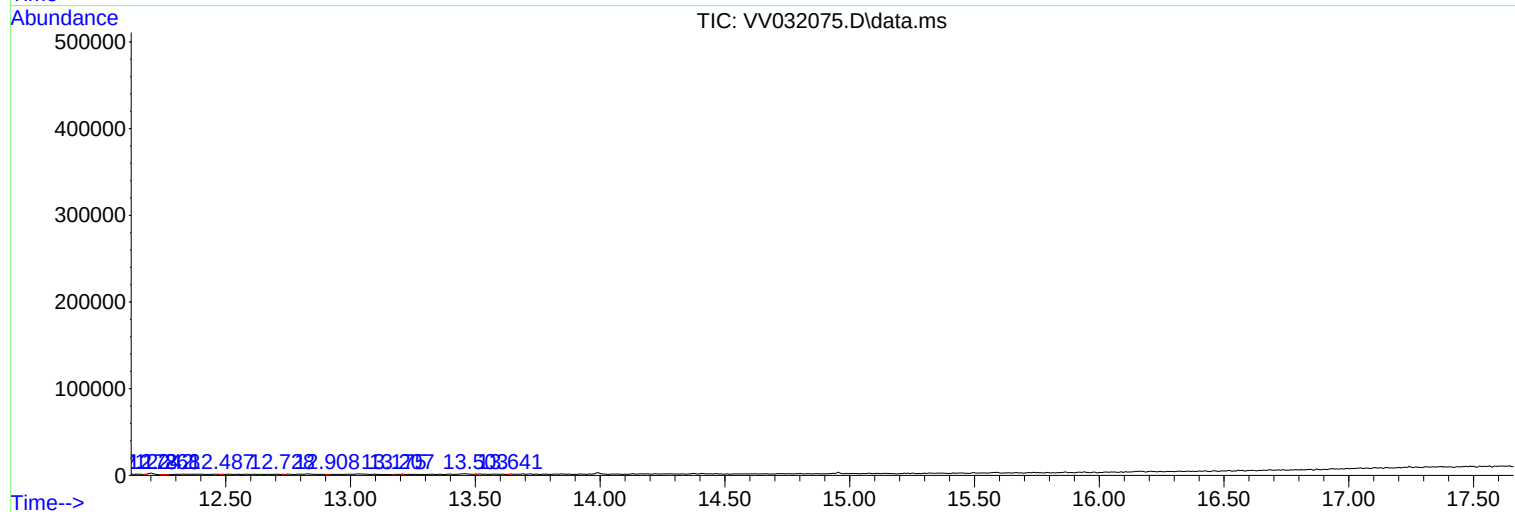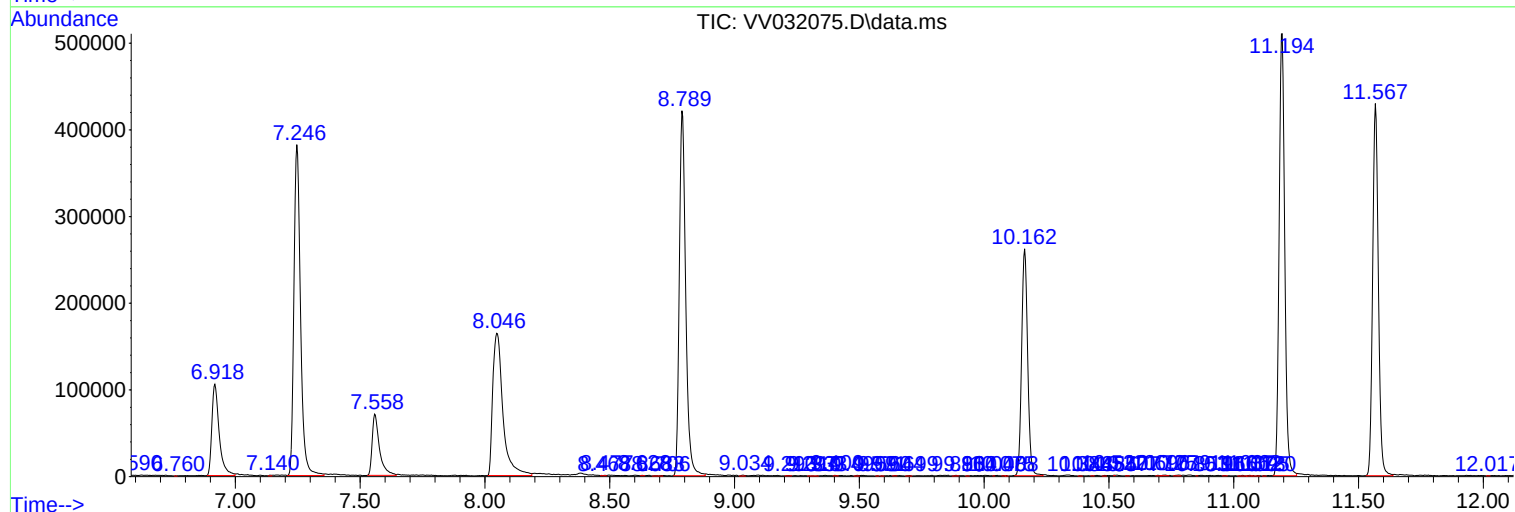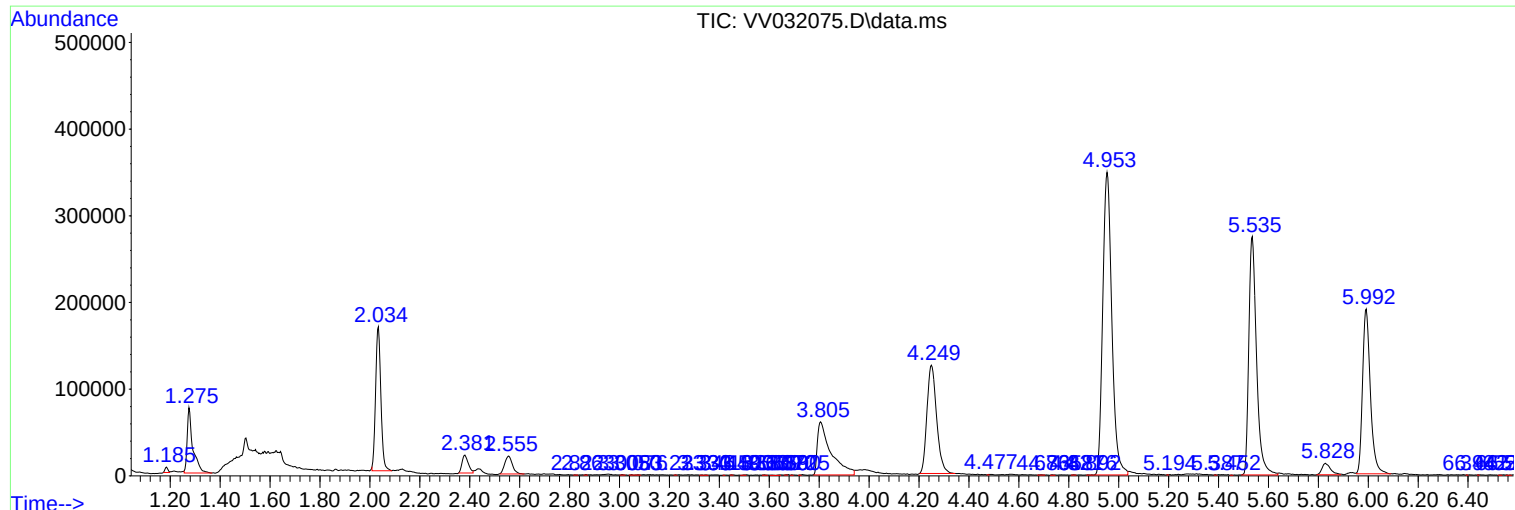

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032075.D
Acq On : 13 Sep 2023 14:42
Operator : SY/MD
Sample : 04387-08ME
Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032075.D
Acq On : 13 Sep 2023 14:42
Operator : SY/MD
Sample : 04387-08ME
Misc : 2.91g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------