

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032076.D
 Acq On : 13 Sep 2023 15:05
 Operator : SY/MD
 Sample : 04387-11ME
 Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	40	45	50	rBV	9976	9757	1.22%	0.150%
2	1.275	67	73	100	rVB	63621	103244	12.96%	1.585%
3	2.031	300	308	323	rVB	145201	210014	26.36%	3.225%
4	2.555	460	471	486	rVB	21356	44641	5.60%	0.685%
5	3.098	638	640	644	rBV3	736	632	0.08%	0.010%
6	3.252	686	688	690	rBV	465	213	0.03%	0.003%
7	3.378	724	727	729	rVB	390	198	0.02%	0.003%
8	3.397	729	733	735	rBV2	627	451	0.06%	0.007%
9	3.516	767	770	773	rBV2	265	213	0.03%	0.003%
10	3.603	793	797	799	rBV	313	219	0.03%	0.003%
11	3.619	799	802	809	rVB4	466	531	0.07%	0.008%
12	3.686	821	823	827	rVB3	608	328	0.04%	0.005%
13	3.764	845	847	848	rBV2	450	202	0.03%	0.003%
14	3.809	852	861	895	rBV	50999	194066	24.35%	2.980%
15	4.249	984	998	1028	rVB	110642	294813	37.00%	4.527%
16	4.481	1067	1070	1073	rBV3	702	545	0.07%	0.008%
17	4.513	1078	1080	1084	rVV3	652	398	0.05%	0.006%
18	4.629	1112	1116	1118	rBV3	408	320	0.04%	0.005%
19	4.719	1138	1144	1147	rBV4	453	516	0.06%	0.008%
20	4.780	1160	1163	1167	rVB3	585	476	0.06%	0.007%
21	4.802	1167	1170	1172	rBV3	474	369	0.05%	0.006%
22	4.889	1193	1197	1199	rBV2	495	298	0.04%	0.005%
23	4.953	1201	1217	1251	rVV2	309036	784320	98.43%	12.043%
24	5.275	1310	1317	1321	rBV6	1186	1995	0.25%	0.031%
25	5.420	1359	1362	1363	rBV2	316	209	0.03%	0.003%
26	5.535	1386	1398	1434	rBV	285512	617932	77.55%	9.488%
27	5.738	1458	1461	1462	rBV	565	286	0.04%	0.004%
28	5.828	1479	1489	1509	rBV3	11982	30013	3.77%	0.461%
29	5.992	1529	1540	1571	rVB	167401	366067	45.94%	5.621%
30	6.320	1640	1642	1646	rVB2	460	272	0.03%	0.004%
31	6.339	1646	1648	1650	rBV3	350	202	0.03%	0.003%
32	6.371	1654	1658	1659	rBV2	343	253	0.03%	0.004%
33	6.439	1676	1679	1683	rBV2	378	347	0.04%	0.005%
34	6.526	1701	1706	1709	rBV2	509	378	0.05%	0.006%
35	6.545	1709	1712	1715	rBV3	485	276	0.03%	0.004%
36	6.776	1782	1784	1787	rBV2	364	227	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032076.D
 Acq On : 13 Sep 2023 15:05
 Operator : SY/MD
 Sample : 04387-11ME
 Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.799	1787	1791	1794	rVV3	653	476	0.06%	0.007%
38	6.918	1817	1828	1859	rBV	93834	189920	23.83%	2.916%
39	7.246	1918	1930	1965	rBV	331579	612259	76.83%	9.401%
40	7.561	2018	2028	2052	rBV	62118	127133	15.95%	1.952%
41	7.702	2069	2072	2076	rVB4	717	459	0.06%	0.007%
42	7.773	2092	2094	2098	rVB2	519	346	0.04%	0.005%
43	7.854	2117	2119	2121	rBV2	409	247	0.03%	0.004%
44	7.876	2123	2126	2127	rBV2	897	467	0.06%	0.007%
45	8.043	2168	2178	2219	rBV	153473	395221	49.60%	6.069%
46	8.509	2321	2323	2328	rVB3	675	402	0.05%	0.006%
47	8.677	2371	2375	2377	rBV2	437	323	0.04%	0.005%
48	8.696	2377	2381	2386	rBV2	341	370	0.05%	0.006%
49	8.731	2389	2392	2396	rBV6	561	495	0.06%	0.008%
50	8.789	2398	2410	2438	rBV	444122	767754	96.35%	11.789%
51	9.066	2493	2496	2499	rVB2	591	370	0.05%	0.006%
52	9.091	2499	2504	2508	rBV4	651	696	0.09%	0.011%
53	9.191	2533	2535	2539	rBV3	746	537	0.07%	0.008%
54	9.236	2545	2549	2552	rBV	340	268	0.03%	0.004%
55	9.316	2572	2574	2578	rVB2	468	293	0.04%	0.004%
56	9.336	2578	2580	2582	rBV2	477	228	0.03%	0.004%
57	9.358	2584	2587	2597	rVB3	621	785	0.10%	0.012%
58	9.410	2597	2603	2605	rBV2	546	492	0.06%	0.008%
59	9.464	2616	2620	2622	rBV	273	218	0.03%	0.003%
60	9.490	2624	2628	2629	rBV2	435	208	0.03%	0.003%
61	9.558	2648	2649	2652	rBV	451	295	0.04%	0.005%
62	9.812	2723	2728	2730	rBV3	557	462	0.06%	0.007%
63	9.870	2744	2746	2748	rBV3	580	244	0.03%	0.004%
64	9.969	2774	2777	2778	rBV	506	339	0.04%	0.005%
65	10.085	2810	2813	2816	rBV2	371	219	0.03%	0.003%
66	10.120	2821	2824	2825	rBV	654	274	0.03%	0.004%
67	10.162	2825	2837	2851	rBV	226021	371853	46.67%	5.710%
68	10.410	2911	2914	2916	rBV2	529	333	0.04%	0.005%
69	10.554	2956	2959	2963	rVB3	524	371	0.05%	0.006%
70	10.596	2970	2972	2975	rBV2	345	249	0.03%	0.004%
71	10.722	3005	3011	3014	rBV4	1127	1090	0.14%	0.017%
72	10.934	3072	3077	3079	rBV2	345	284	0.04%	0.004%
73	10.992	3090	3095	3098	rBV3	498	558	0.07%	0.009%
74	11.062	3114	3117	3119	rVB	574	332	0.04%	0.005%
75	11.078	3119	3122	3124	rBV3	557	361	0.05%	0.006%
76	11.120	3131	3135	3137	rBV	616	361	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032076.D
 Acq On : 13 Sep 2023 15:05
 Operator : SY/MD
 Sample : 04387-11ME
 Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.140	3139	3141	3145	rBV2	442	203	0.03%	0.003%
78	11.191	3145	3157	3176	rBV	515214	796856	100.00%	12.236%
79	11.390	3215	3219	3222	rVB4	598	406	0.05%	0.006%
80	11.410	3222	3225	3228	rBV4	438	341	0.04%	0.005%
81	11.426	3228	3230	3238	rVB5	832	911	0.11%	0.014%
82	11.461	3239	3241	3243	rBV2	484	225	0.03%	0.003%
83	11.567	3263	3274	3296	rBV	360711	564481	70.84%	8.668%
84	11.789	3338	3343	3345	rBV4	641	545	0.07%	0.008%
85	12.014	3411	3413	3417	rBV4	411	344	0.04%	0.005%
86	12.365	3520	3522	3525	rBV2	445	283	0.04%	0.004%
87	12.406	3533	3535	3539	rBV2	401	257	0.03%	0.004%
88	12.493	3558	3562	3565	rBV2	607	328	0.04%	0.005%
89	12.628	3602	3604	3608	rBV4	402	304	0.04%	0.005%
90	12.728	3633	3635	3640	rVB3	454	251	0.03%	0.004%
91	12.828	3664	3666	3670	rBV2	774	680	0.09%	0.010%
92	12.885	3682	3684	3688	rBV2	530	306	0.04%	0.005%
93	12.963	3705	3708	3710	rBV2	345	212	0.03%	0.003%
94	13.098	3748	3750	3751	rBV	458	249	0.03%	0.004%
95	13.120	3755	3757	3759	rBV	507	258	0.03%	0.004%
96	13.336	3821	3824	3826	rBV2	487	272	0.03%	0.004%
97	13.429	3849	3853	3856	rBV3	661	535	0.07%	0.008%
98	13.538	3885	3887	3891	rBV2	560	492	0.06%	0.008%
99	13.638	3916	3918	3921	rVB2	570	306	0.04%	0.005%
100	14.059	4044	4049	4052	rBV4	522	610	0.08%	0.009%




Sum of corrected areas: 6512468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032076.D
Acq On : 13 Sep 2023 15:05
Operator : SY/MD
Sample : 04387-11ME
Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

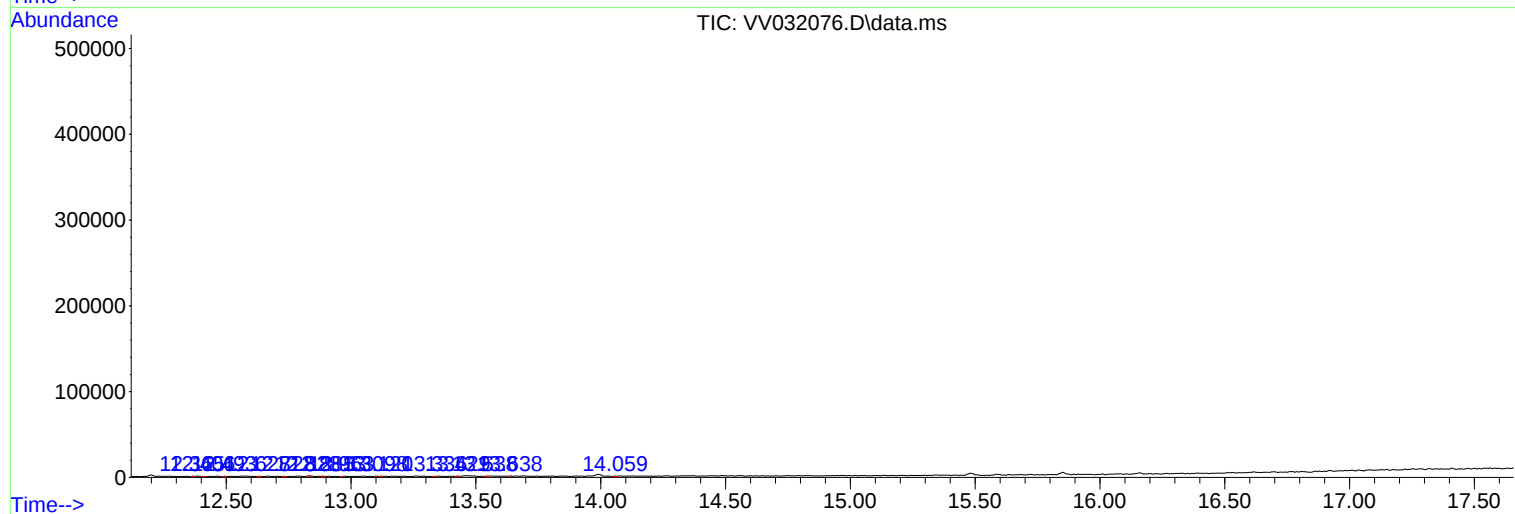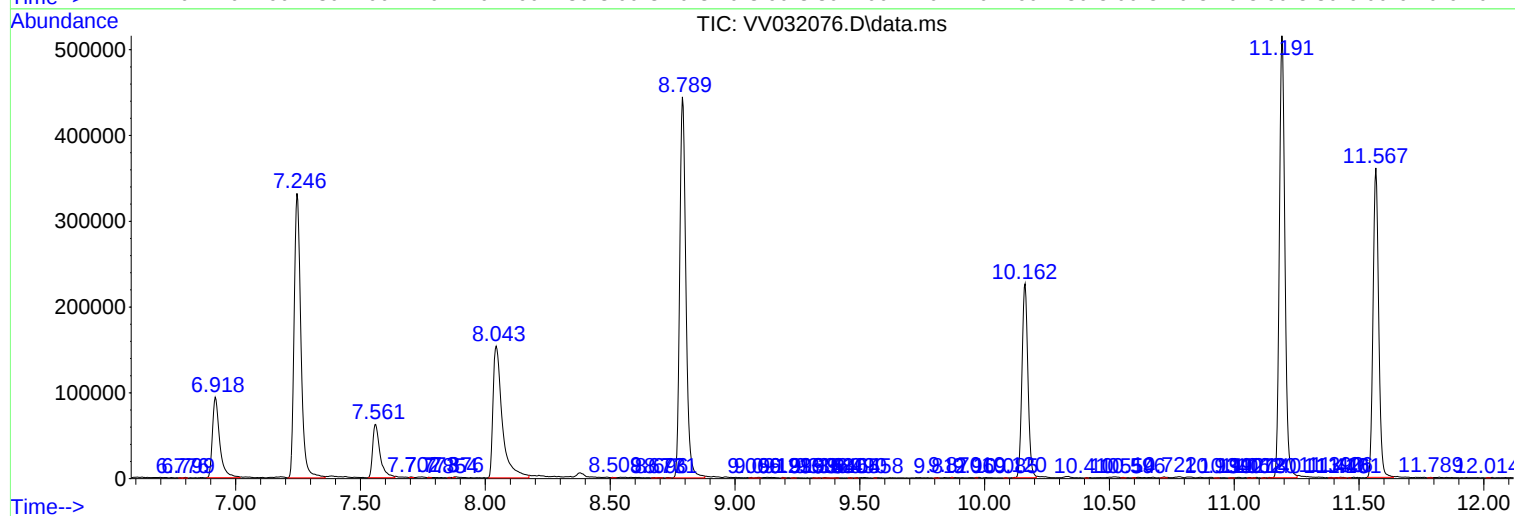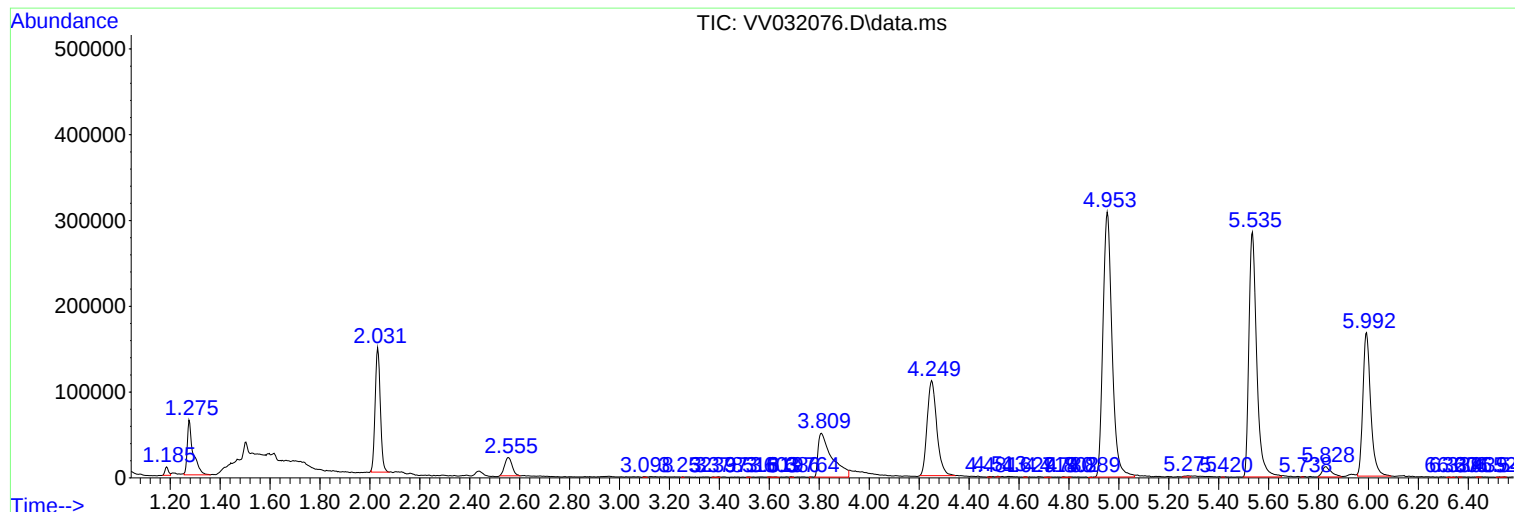

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032076.D
Acq On : 13 Sep 2023 15:05
Operator : SY/MD
Sample : 04387-11ME
Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032076.D
Acq On : 13 Sep 2023 15:05
Operator : SY/MD
Sample : 04387-11ME
Misc : 2.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc