

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032078.D
 Acq On : 13 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04387-15ME
 Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	40	45	49	rBV	10135	9653	1.23%	0.150%
2	1.275	67	73	103	rVB	61340	101539	12.93%	1.574%
3	2.031	300	308	325	rVB	142693	208840	26.59%	3.237%
4	2.555	460	471	490	rVB	22338	46815	5.96%	0.726%
5	2.860	563	566	568	rBV3	416	291	0.04%	0.005%
6	2.886	572	574	575	rBV2	366	152	0.02%	0.002%
7	3.098	635	640	641	rBV3	608	449	0.06%	0.007%
8	3.214	674	676	678	rBV2	268	116	0.01%	0.002%
9	3.342	711	716	719	rVB3	564	402	0.05%	0.006%
10	3.397	730	733	735	rBV3	256	153	0.02%	0.002%
11	3.503	764	766	771	rVB3	407	227	0.03%	0.004%
12	3.532	773	775	779	rVB3	375	236	0.03%	0.004%
13	3.564	783	785	788	rBV	294	203	0.03%	0.003%
14	3.590	788	793	794	rBV3	330	221	0.03%	0.003%
15	3.648	807	811	814	rBV2	356	344	0.04%	0.005%
16	3.809	852	861	904	rBV	54932	218991	27.88%	3.395%
17	4.249	985	998	1025	rVB	107890	286014	36.42%	4.434%
18	4.493	1072	1074	1075	rBV	505	215	0.03%	0.003%
19	4.696	1135	1137	1139	rBV2	384	223	0.03%	0.003%
20	4.725	1145	1146	1150	rVB2	494	209	0.03%	0.003%
21	4.747	1150	1153	1154	rBV	472	205	0.03%	0.003%
22	4.805	1169	1171	1173	rBV	432	187	0.02%	0.003%
23	4.902	1199	1201	1202	rBV2	414	189	0.02%	0.003%
24	4.953	1202	1217	1248	rBV2	301381	767452	97.72%	11.897%
25	5.185	1287	1289	1291	rBV	442	278	0.04%	0.004%
26	5.387	1350	1352	1354	rBV2	516	245	0.03%	0.004%
27	5.471	1375	1378	1380	rBV2	692	465	0.06%	0.007%
28	5.535	1386	1398	1430	rBV	279380	606519	77.22%	9.402%
29	5.828	1481	1489	1505	rVB4	9757	22244	2.83%	0.345%
30	5.992	1528	1540	1564	rVB	162938	350210	44.59%	5.429%
31	6.233	1612	1615	1618	rVB3	511	304	0.04%	0.005%
32	6.249	1618	1620	1621	rBV2	405	190	0.02%	0.003%
33	6.317	1638	1641	1646	rVB2	805	694	0.09%	0.011%
34	6.345	1646	1650	1652	rBV3	567	460	0.06%	0.007%
35	6.426	1673	1675	1678	rBV2	385	296	0.04%	0.005%
36	6.574	1719	1721	1722	rBV	650	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032078.D
 Acq On : 13 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04387-15ME
 Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.754	1774	1777	1778	rBV2	412	242	0.03%	0.004%
38	6.837	1802	1803	1807	rBV2	226	160	0.02%	0.002%
39	6.860	1807	1810	1813	rBV3	564	330	0.04%	0.005%
40	6.918	1817	1828	1859	rBV	90210	187203	23.84%	2.902%
41	7.246	1919	1930	1956	rBV	328595	598918	76.26%	9.284%
42	7.561	2019	2028	2045	rBV	59411	117529	14.96%	1.822%
43	7.841	2112	2115	2116	rBV	332	176	0.02%	0.003%
44	7.879	2125	2127	2129	rBV2	311	210	0.03%	0.003%
45	7.989	2159	2161	2163	rBV2	554	339	0.04%	0.005%
46	8.043	2168	2178	2212	rBV2	158150	403464	51.37%	6.254%
47	8.522	2325	2327	2331	rBV2	448	302	0.04%	0.005%
48	8.789	2399	2410	2435	rBV	440958	759853	96.75%	11.779%
49	8.988	2470	2472	2475	rBV	444	301	0.04%	0.005%
50	9.033	2484	2486	2489	rBV5	429	287	0.04%	0.004%
51	9.095	2503	2505	2510	rBV4	770	508	0.06%	0.008%
52	9.130	2512	2516	2520	rBV3	617	463	0.06%	0.007%
53	9.159	2523	2525	2529	rVB3	644	348	0.04%	0.005%
54	9.259	2553	2556	2558	rVB2	306	183	0.02%	0.003%
55	9.268	2558	2559	2562	rBV	275	103	0.01%	0.002%
56	9.284	2562	2564	2567	rBV2	472	204	0.03%	0.003%
57	9.304	2567	2570	2571	rBV	449	209	0.03%	0.003%
58	9.349	2583	2584	2586	rBV	275	116	0.01%	0.002%
59	9.378	2591	2593	2595	rBV2	305	192	0.02%	0.003%
60	9.394	2595	2598	2600	rVB	460	246	0.03%	0.004%
61	9.464	2616	2620	2624	rBV3	464	414	0.05%	0.006%
62	9.500	2624	2631	2632	rVV3	581	435	0.06%	0.007%
63	9.529	2636	2640	2645	rVB5	553	549	0.07%	0.009%
64	9.567	2650	2652	2653	rBV	229	121	0.02%	0.002%
65	9.619	2666	2668	2670	rBV2	266	136	0.02%	0.002%
66	9.635	2670	2673	2675	rVV3	398	203	0.03%	0.003%
67	9.705	2692	2695	2697	rBV2	397	335	0.04%	0.005%
68	9.744	2705	2707	2710	rBV	392	278	0.04%	0.004%
69	9.770	2713	2715	2718	rVV3	411	209	0.03%	0.003%
70	9.805	2724	2726	2728	rBV2	283	123	0.02%	0.002%
71	9.889	2750	2752	2754	rBV3	388	211	0.03%	0.003%
72	9.966	2774	2776	2781	rVB2	644	372	0.05%	0.006%
73	10.011	2788	2790	2792	rBV	393	207	0.03%	0.003%
74	10.117	2819	2823	2824	rBV	651	491	0.06%	0.008%
75	10.162	2825	2837	2851	rVV	224527	368390	46.91%	5.711%
76	10.416	2914	2916	2920	rVB3	540	372	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
 Data File : VV032078.D
 Acq On : 13 Sep 2023 15:52
 Operator : SY/MD
 Sample : 04387-15ME
 Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COANOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.439	2920	2923	2925	rBV3	515	246	0.03%	0.004%
78	10.525	2948	2950	2954	rVV4	512	366	0.05%	0.006%
79	10.847	3048	3050	3053	rBV2	638	445	0.06%	0.007%
80	10.892	3055	3064	3079	rBV5	7169	17978	2.29%	0.279%
81	11.191	3146	3157	3178	rBV	499692	785395	100.00%	12.175%
82	11.397	3219	3221	3222	rBV	397	160	0.02%	0.002%
83	11.509	3254	3256	3260	rVB3	511	245	0.03%	0.004%
84	11.567	3260	3274	3292	rBV	358516	565255	71.97%	8.762%
85	11.766	3335	3336	3337	rBV	498	137	0.02%	0.002%
86	11.879	3366	3371	3377	rBV3	661	669	0.09%	0.010%
87	12.197	3462	3470	3479	rVB4	2096	3105	0.40%	0.048%
88	12.262	3487	3490	3492	rVB3	363	214	0.03%	0.003%
89	12.310	3499	3505	3511	rBV7	1092	1952	0.25%	0.030%
90	12.683	3618	3621	3622	rBV2	533	277	0.04%	0.004%
91	12.773	3643	3649	3652	rBV4	613	639	0.08%	0.010%
92	12.837	3663	3669	3672	rBV2	905	1144	0.15%	0.018%
93	12.937	3696	3700	3701	rBV2	323	207	0.03%	0.003%
94	13.069	3739	3741	3743	rBV	417	134	0.02%	0.002%
95	13.168	3765	3772	3776	rBV3	489	650	0.08%	0.010%
96	13.609	3906	3909	3912	rBV3	642	350	0.04%	0.005%
97	13.625	3912	3914	3916	rBV2	696	348	0.04%	0.005%
98	13.889	3993	3996	4000	rBV3	460	361	0.05%	0.006%
99	14.040	4040	4043	4045	rBV3	610	323	0.04%	0.005%
100	14.220	4097	4099	4101	rBV2	522	333	0.04%	0.005%

Sum of corrected areas: 6451066




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032078.D
Acq On : 13 Sep 2023 15:52
Operator : SY/MD
Sample : 04387-15ME
Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COANOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

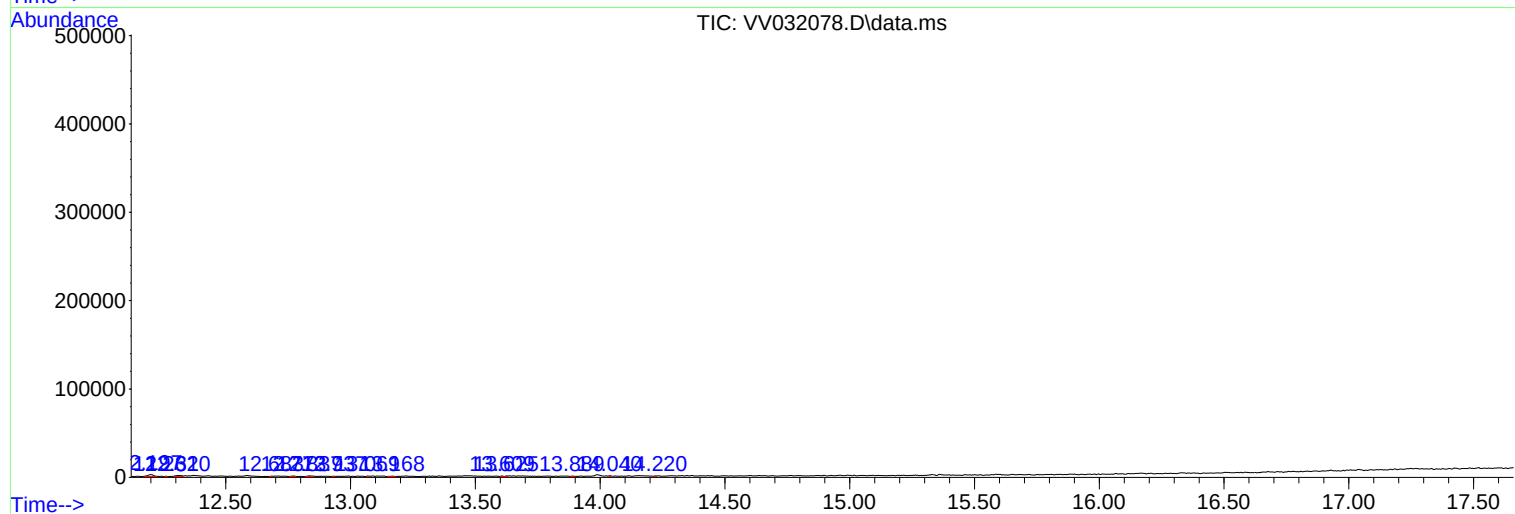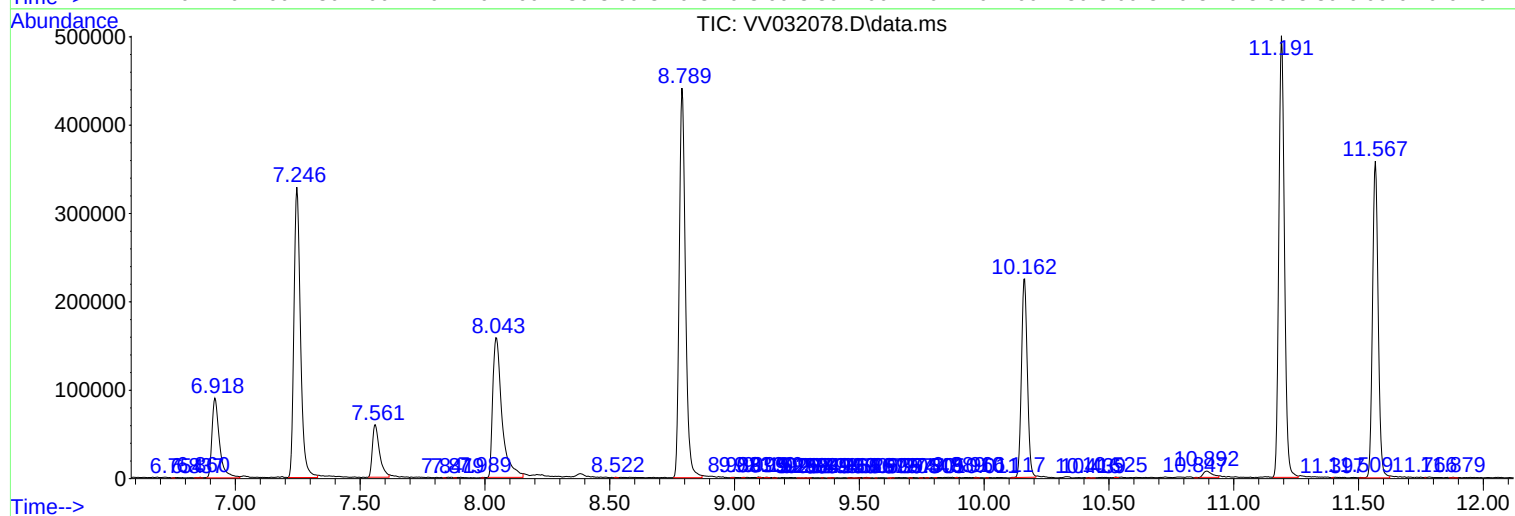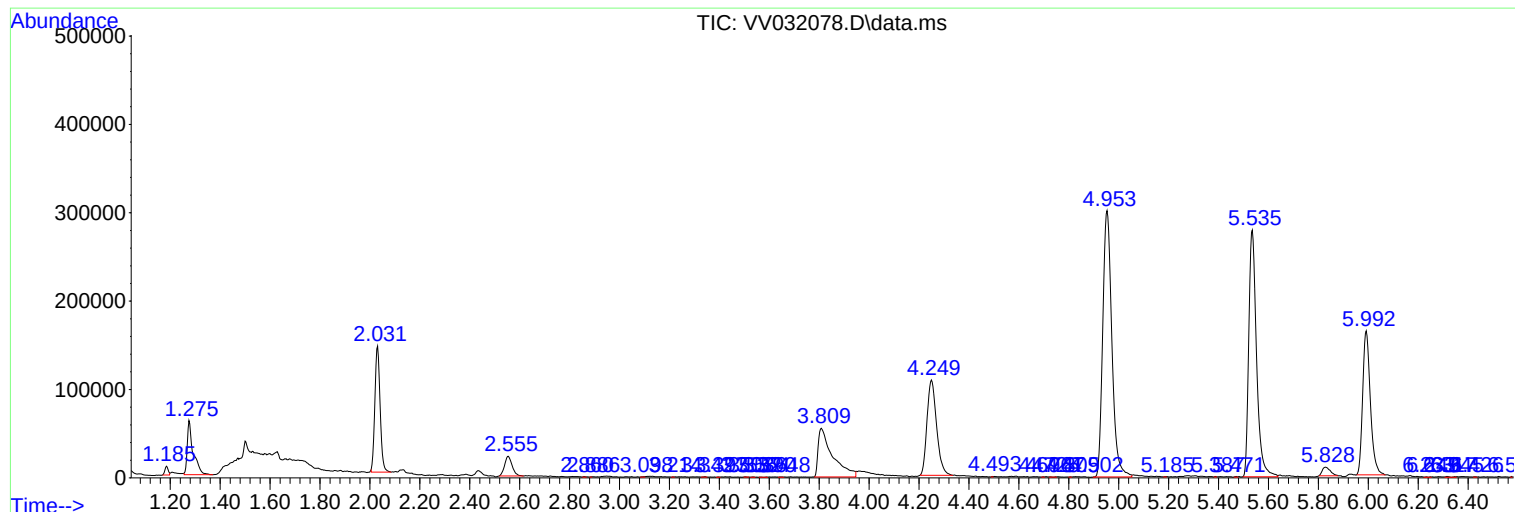

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032078.D
Acq On : 13 Sep 2023 15:52
Operator : SY/MD
Sample : 04387-15ME
Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032078.D
Acq On : 13 Sep 2023 15:52
Operator : SY/MD
Sample : 04387-15ME
Misc : 2.39g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc