
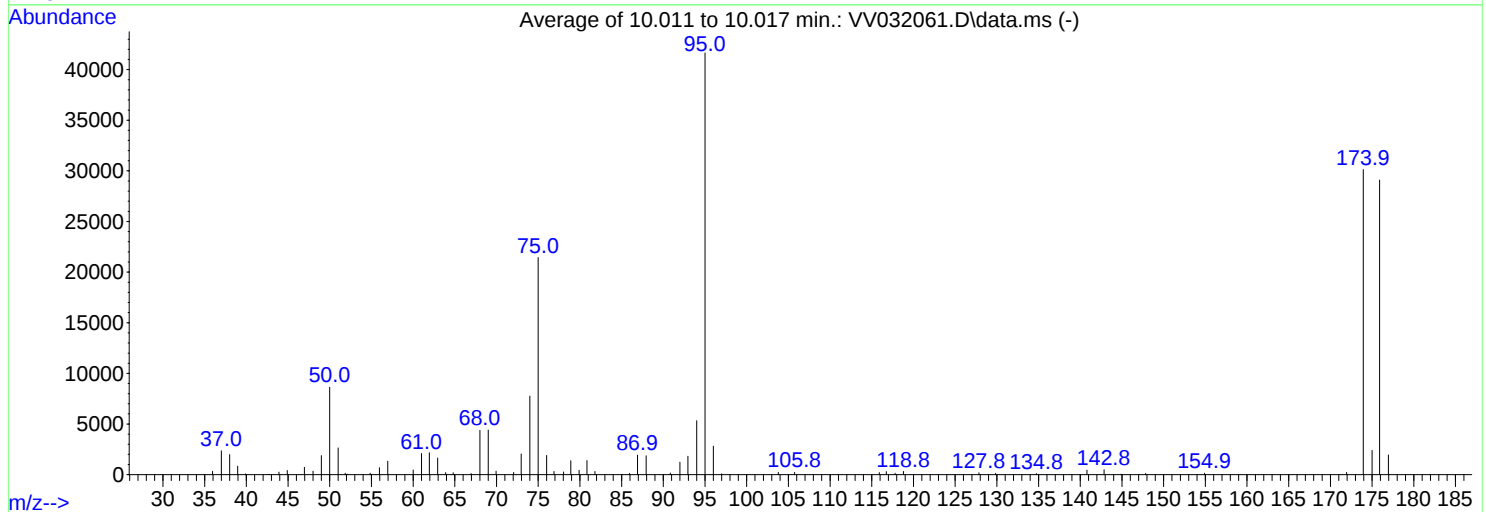


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091323\
Data File : VV032061.D
Acq On : 13 Sep 2023 08:45
Operator : SY/MD
Sample : BFB211
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB211

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Sep 16 02:09:37 2023

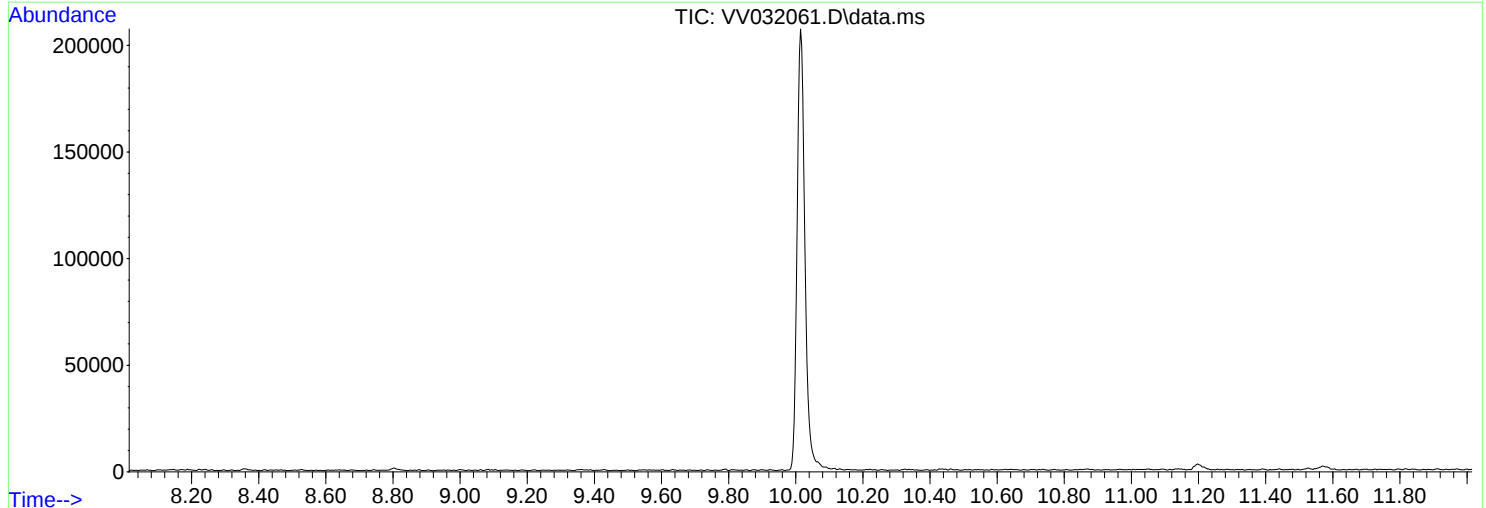

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	8624	PASS
75	95	30	80	51.5	21445	PASS
95	95	100	100	100.0	41653	PASS
96	95	5	9	6.8	2813	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	30141	PASS
175	174	5	9	8.0	2402	PASS
176	174	95	105	96.5	29088	PASS
177	176	5	10	6.7	1951	PASS

m/z	Abundance
36.00	146.0
38.90	113.0
39.80	202.0
43.90	469.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	522.0
37.00	2275.0
38.00	1953.0
39.00	938.0
40.00	256.0
42.70	110.0
43.90	704.0
44.90	365.0
47.00	722.0
48.00	343.0
49.00	1858.0
50.00	8478.0
51.00	2562.0
51.90	129.0
52.10	130.0
54.90	131.0
56.00	692.0
57.00	1264.0
60.00	489.0
61.00	2034.0
62.00	2093.0
62.90	1632.0
63.90	205.0
64.80	195.0
66.90	147.0
68.00	4262.0
69.00	4344.0
70.00	403.0
72.00	226.0
72.90	1948.0
74.00	7520.0
75.00	21040.0
76.00	1851.0
76.90	322.0
78.00	277.0
78.90	1341.0
79.90	381.0
80.80	1374.0
81.80	332.0
86.00	121.0
86.90	1815.0
88.00	1793.0
90.90	185.0
92.00	1214.0
93.00	1864.0
94.00	5193.0
95.00	40712.0
96.00	2811.0
97.00	122.0
103.80	248.0
105.80	223.0
115.90	209.0
116.70	295.0
117.80	163.0
118.80	310.0
127.90	197.0
129.90	130.0
134.80	102.0
140.80	385.0
142.80	523.0
144.90	122.0
146.00	112.0
147.90	135.0
154.90	110.0
172.00	194.0
174.00	28784.0
175.00	2385.0
175.90	27704.0
176.90	1876.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
35.90	489.0
37.00	2453.0
38.00	2059.0
39.00	993.0
40.00	283.0
41.00	109.0
43.90	731.0
44.90	418.0
46.90	725.0
48.00	370.0
49.00	1953.0
50.00	8952.0
51.00	2754.0
51.80	147.0
54.80	150.0
56.00	686.0
56.90	1364.0
60.00	467.0
61.00	2134.0
61.90	2234.0
62.90	1685.0
63.90	219.0
64.80	195.0
67.00	164.0
68.00	4504.0
69.00	4558.0
70.00	354.0
72.10	237.0
72.90	2087.0
74.00	8087.0
75.00	22024.0
76.00	1946.0
76.90	321.0
78.00	277.0
78.90	1424.0
79.90	446.0
80.80	1421.0
81.80	335.0
86.00	132.0
86.90	1997.0
87.90	1934.0
90.90	159.0
92.00	1268.0
92.90	1850.0
94.00	5530.0
95.00	42856.0
96.00	2889.0
97.00	115.0
103.80	231.0
105.80	230.0
115.90	227.0
116.80	318.0
117.80	153.0
118.80	325.0
127.90	197.0
129.90	122.0
134.80	125.0
140.80	458.0
142.90	513.0
147.90	128.0
154.90	150.0
172.00	211.0
173.90	31232.0
175.00	2527.0
175.90	30048.0
177.00	1996.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
35.90	428.0
37.00	2347.0
38.00	1924.0
39.00	939.0
40.00	293.0
43.90	730.0
44.90	440.0
46.90	738.0
48.00	343.0
49.00	1827.0
50.00	8442.0
51.00	2590.0
51.90	154.0
54.90	162.0
55.90	662.0
56.90	1349.0
60.00	430.0
61.00	2098.0
62.00	2164.0
63.00	1590.0
63.90	212.0
64.80	187.0
68.00	4377.0
69.00	4315.0
69.90	303.0
72.00	224.0
73.00	2063.0
74.00	7693.0
75.00	21272.0
76.00	1882.0
76.90	296.0
78.10	276.0
78.90	1358.0
79.90	443.0
80.90	1356.0
81.80	290.0
85.90	125.0
86.90	1984.0
87.90	1889.0
90.80	145.0
92.00	1201.0
92.90	1760.0
94.00	5256.0
95.00	41392.0
96.00	2739.0
103.80	196.0
105.70	225.0
115.90	178.0
116.80	309.0
117.80	121.0
118.80	298.0
127.80	176.0
129.80	136.0
134.70	113.0
140.80	467.0
142.80	461.0
147.80	106.0
154.90	149.0
171.90	237.0
173.90	30408.0
175.00	2293.0
175.90	29512.0
177.00	1982.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211