

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091418\
 Data File : VV007543.D
 Acq On : 15 Sep 2018 00:19
 Operator : SY/MD
 Sample : J4888-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KW5

Quant Time: Sep 15 04:25:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 15 02:08:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	112668	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	94670	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42376	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24964	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.58	69	28086	5.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.80%
11) 1,1-Dichloroethene-d2	2.13	63	42729	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.97	46	59102	72.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	144.00%#
24) Chloroform-d	4.41	84	54560	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
26) 1,2-Dichloroethane-d4	5.09	65	27945	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
32) Benzene-d6	5.10	84	107310	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.12	67	31788	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.36	98	99202	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.67	79	10619	3.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.80%
46) 2-Hexanone-d5	8.15	63	31038	65.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	131.26%#
57) 1,1,2,2-Tetrachloroethane-	10.27	84	20577	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	37831	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	1473	0.246 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091418\
Data File : VV007543.D
Acq On : 15 Sep 2018 00:19
Operator : SY/MD
Sample : J4888-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KW5

Quant Time: Sep 15 04:25:52 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 15 02:08:52 2018
Response via : Initial Calibration

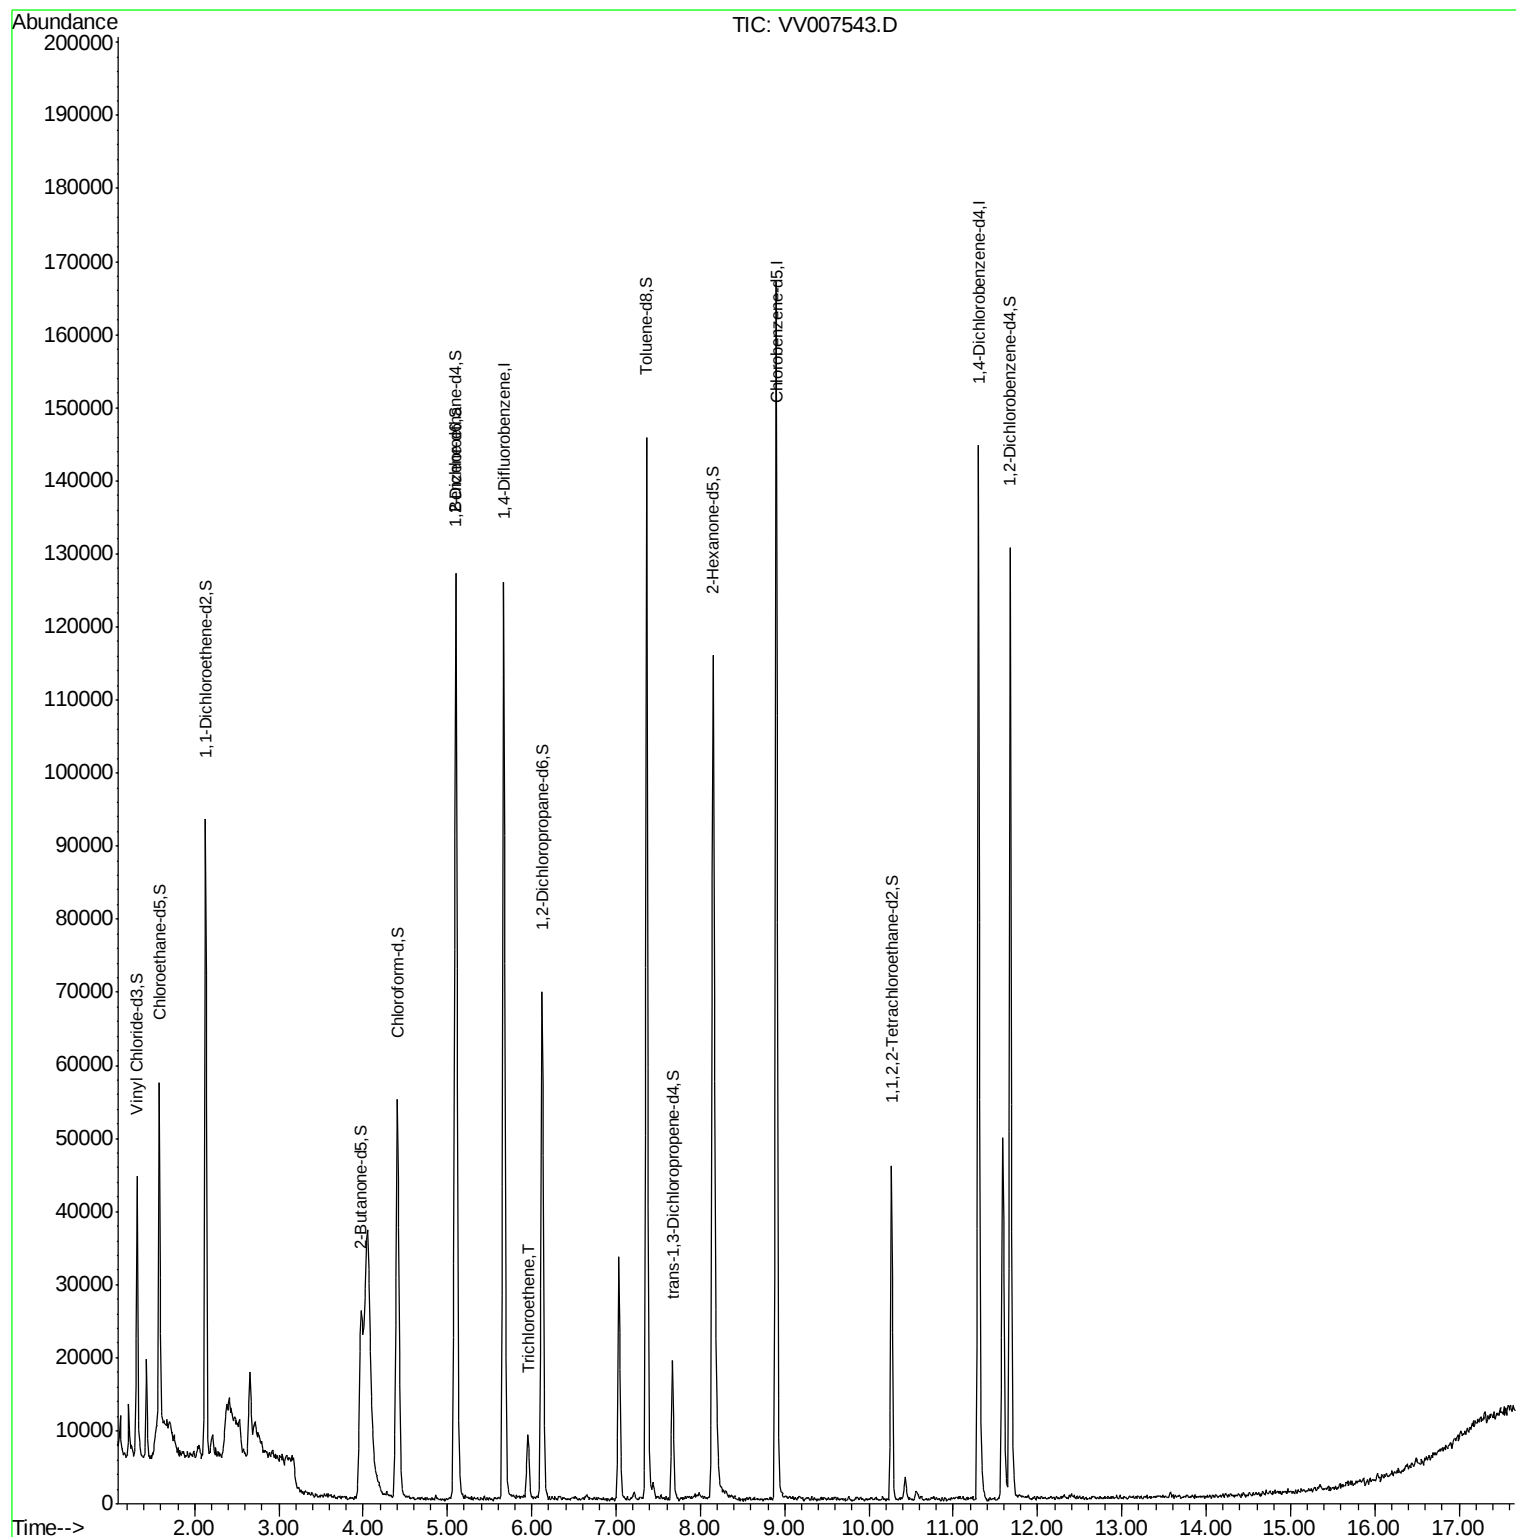

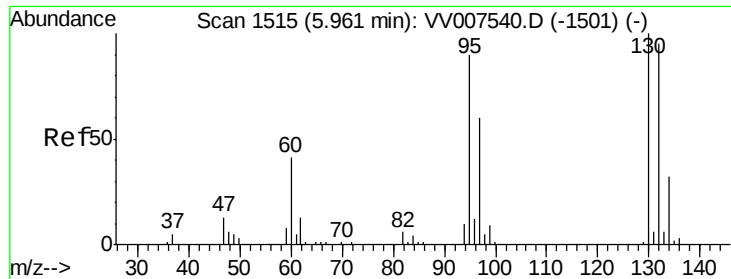

#34

Trichloroethene

Concen: 0.246 ug/L

RT: 5.96 min Scan# 1516

Delta R.T. 0.00 min

Lab File: VV007543.D

Acq: 15 Sep 2018 00:19

Instrument :

MSVOA_V

ClientSampleId :

C0KW5

Tot Ion: 95 Resp: 1473


Ion Ratio Lower Upper

95 100

97 82.9 45.5 84.5

132 100.6 74.9 139.1

130 98.8 80.0 148.6

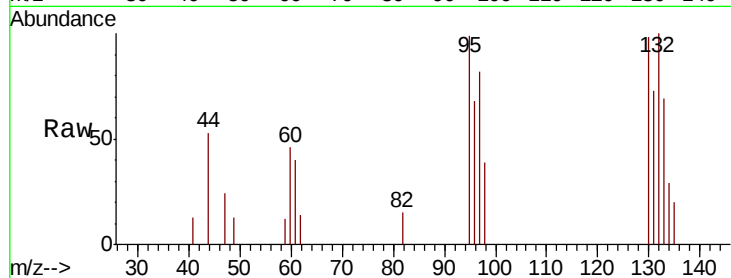

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

