

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091418\
 Data File : VV007550.D
 Acq On : 15 Sep 2018 03:35
 Operator : SY/MD
 Sample : J4872-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KR0

Quant Time: Sep 15 04:47:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 15 02:08:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	105661	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88655	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	38227	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23047	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.58	69	23973	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	2.13	63	39764	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	3.97	46	39806	51.71	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.42%
24) Chloroform-d	4.41	84	53522	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.09	65	27962	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.10	84	101234	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.12	67	31975	5.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.60%
41) Toluene-d8	7.36	98	94760	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.67	79	10850	3.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.20%
46) 2-Hexanone-d5	8.15	63	32640	73.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	147.40%#
57) 1,1,2,2-Tetrachloroethane-	10.27	84	20375	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	36287	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	1413	0.252 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091418\
Data File : VV007550.D
Acq On : 15 Sep 2018 03:35
Operator : SY/MD
Sample : J4872-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KR0

Quant Time: Sep 15 04:47:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 15 02:08:52 2018
Response via : Initial Calibration

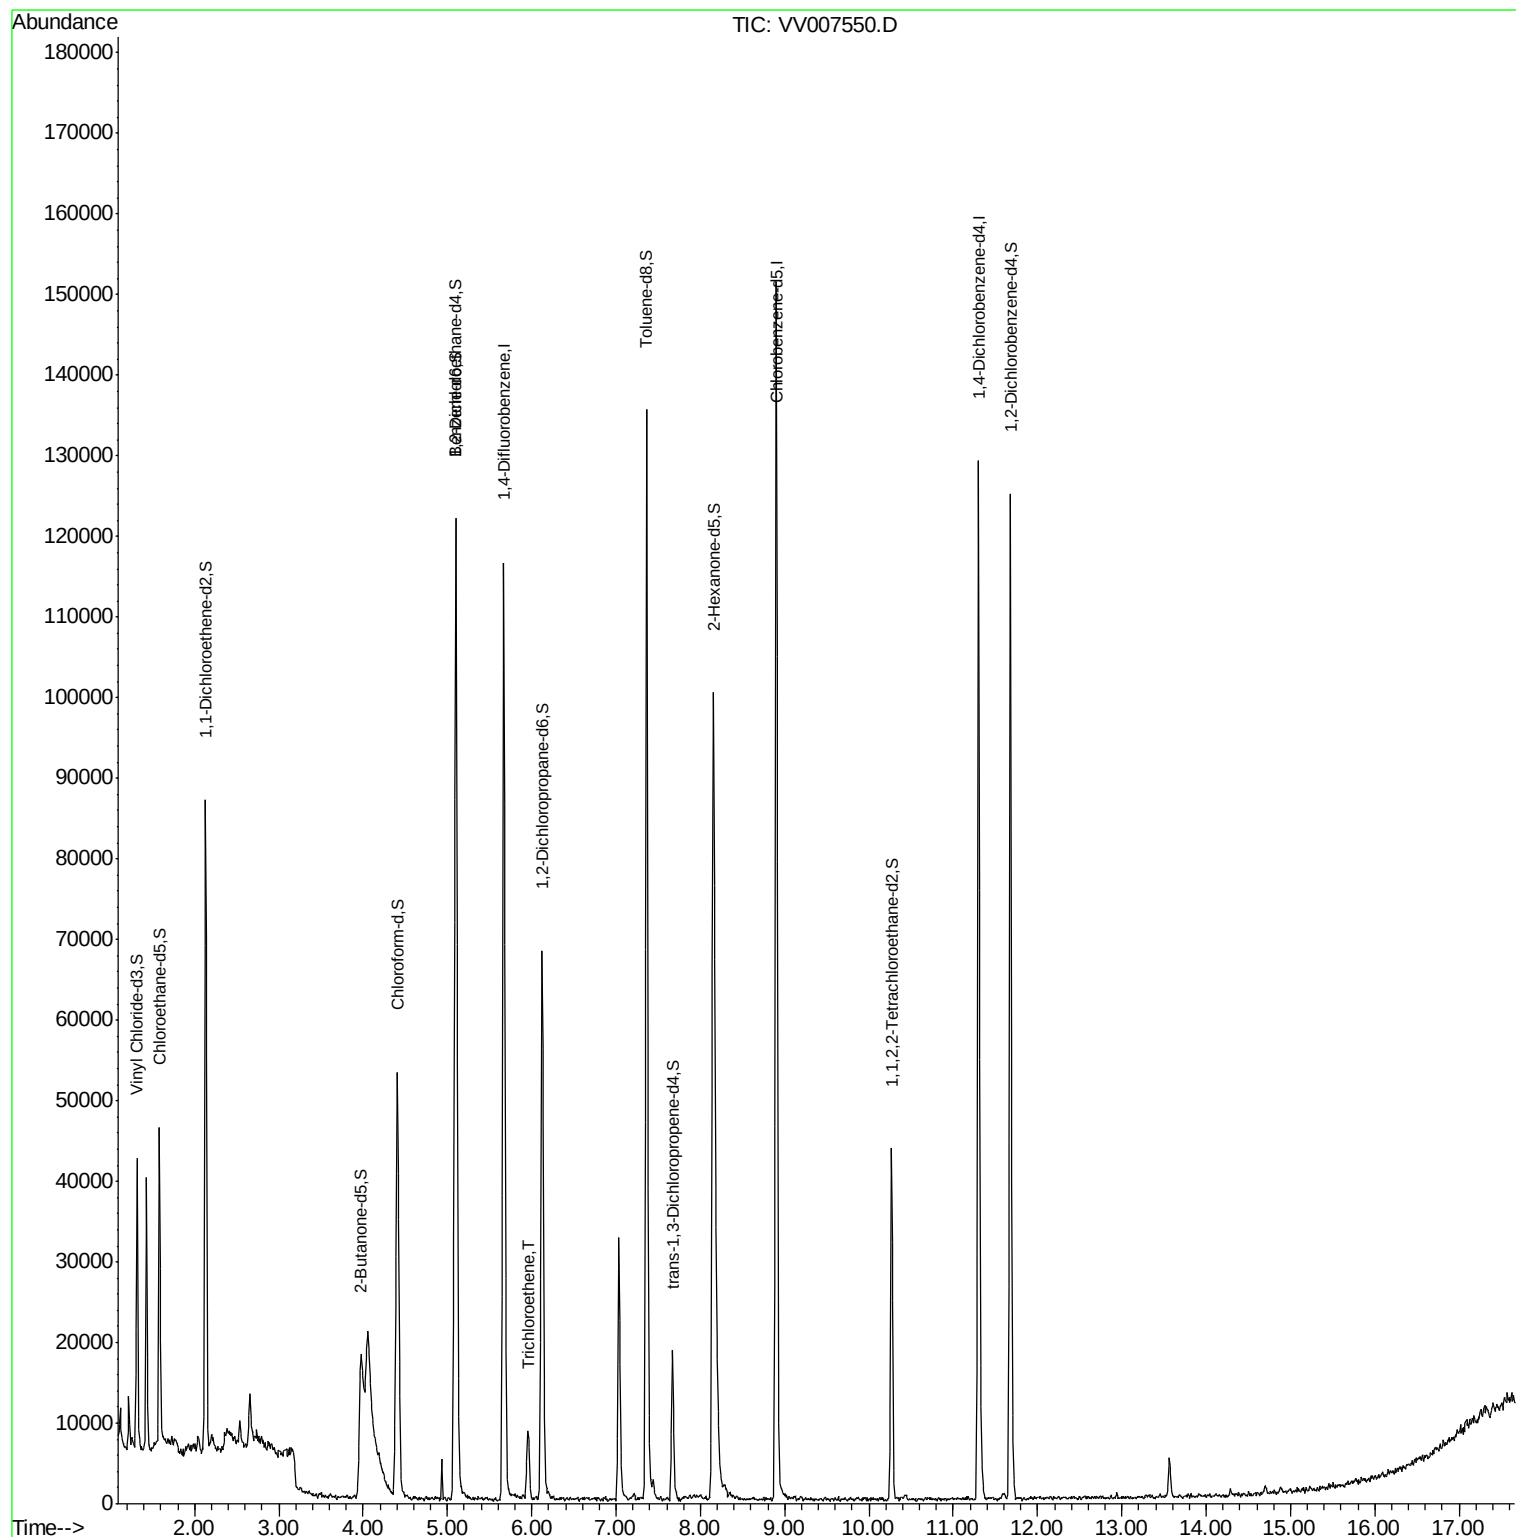

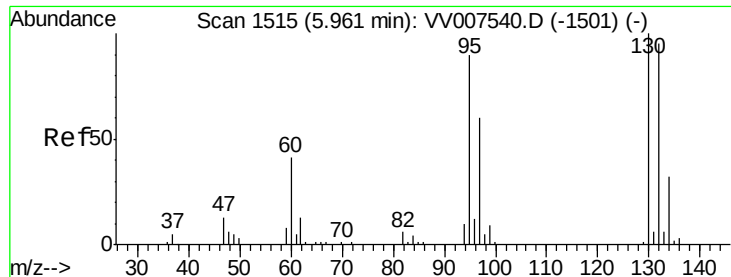

#34
 Trichloroethene
 Concen: 0.252 ug/L
 RT: 5.96 min Scan# 1515
 Delta R.T. 0.00 min
 Lab File: VV007550.D
 Acq: 15 Sep 2018 03:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KR0

Tot Ion:	95	Resp:	1413
Ion	Ratio	Lower	Upper
95	100		
97	71.3	45.5	84.5
132	109.7	74.9	139.1
130	111.1	80.0	148.6

