

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091418\
 Data File : VV007551.D
 Acq On : 15 Sep 2018 04:03
 Operator : SY/MD
 Sample : J4872-13
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KR3

Quant Time: Sep 15 04:50:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 15 02:08:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	111169	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	95672	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42690	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22955	3.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.00%
7) Chloroethane-d5	1.58	69	23489	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.40%
11) 1,1-Dichloroethene-d2	2.13	63	40779	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	3.97	46	42410	52.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.72%
24) Chloroform-d	4.41	84	52471	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.09	65	26409	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
32) Benzene-d6	5.10	84	100836	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.13	67	30493	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.36	98	95607	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.67	79	10274	3.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.60%
46) 2-Hexanone-d5	8.15	63	29822	62.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.80%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	19472	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	37077	4.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.80%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	2568	0.424 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091418\
Data File : VV007551.D
Acq On : 15 Sep 2018 04:03
Operator : SY/MD
Sample : J4872-13
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KR3

Quant Time: Sep 15 04:50:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 15 02:08:52 2018
Response via : Initial Calibration

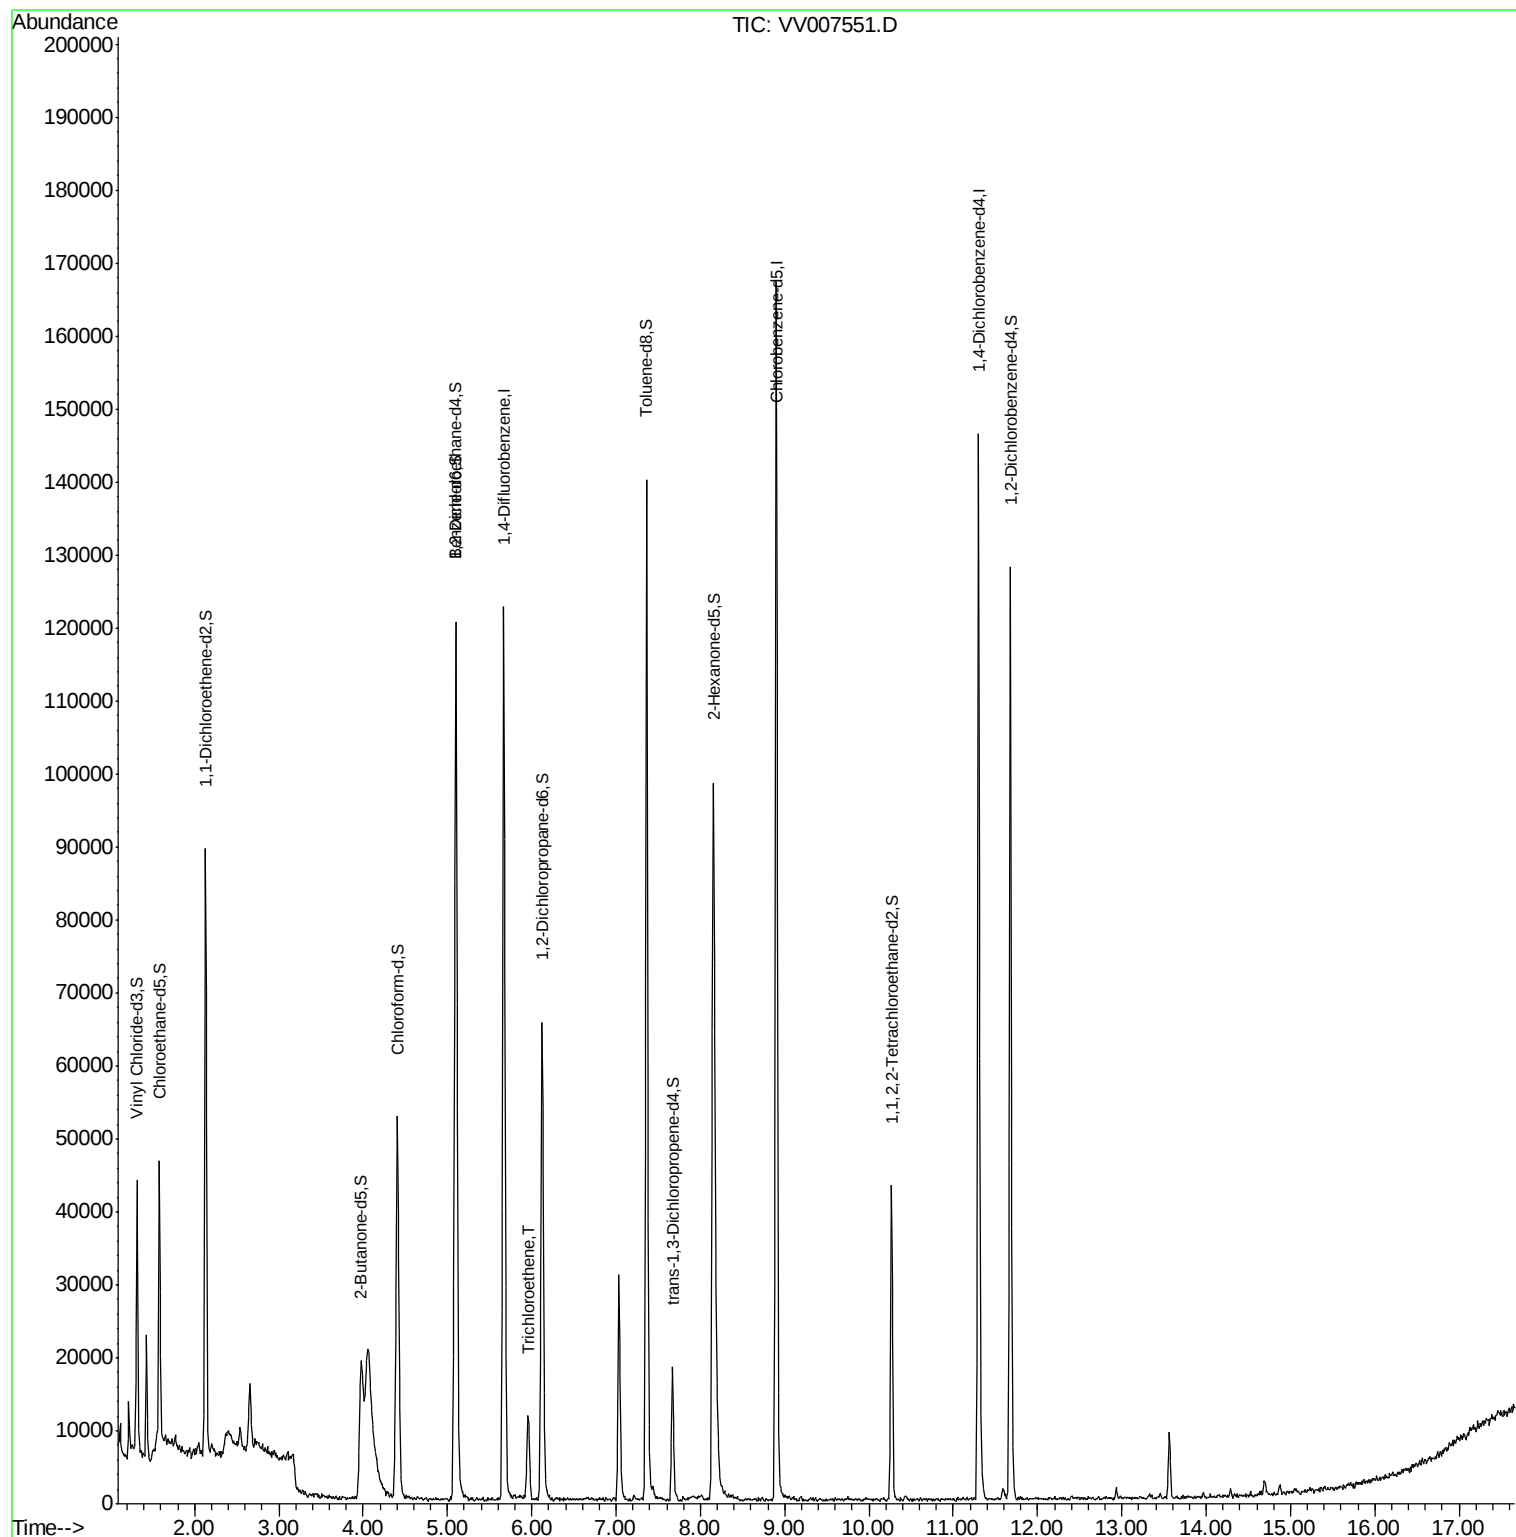

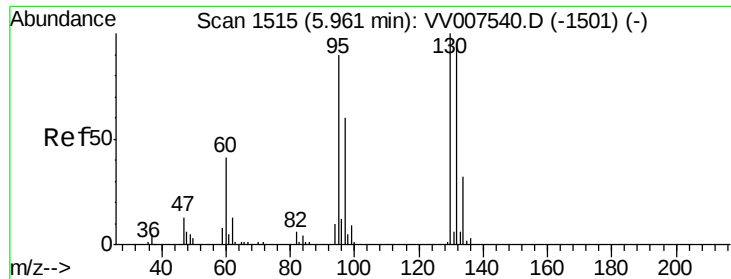

#34
 Trichloroethene
 Concen: 0.424 ug/L
 RT: 5.96 min Scan# 1515
 Delta R.T. 0.00 min
 Lab File: VV007551.D
 Acq: 15 Sep 2018 04:03

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KR3

Tot Ion:	95	Resp:	2568
Ion	Ratio	Lower	Upper
95	100		
97	78.5	45.5	84.5
132	104.3	74.9	139.1
130	117.5	80.0	148.6

